
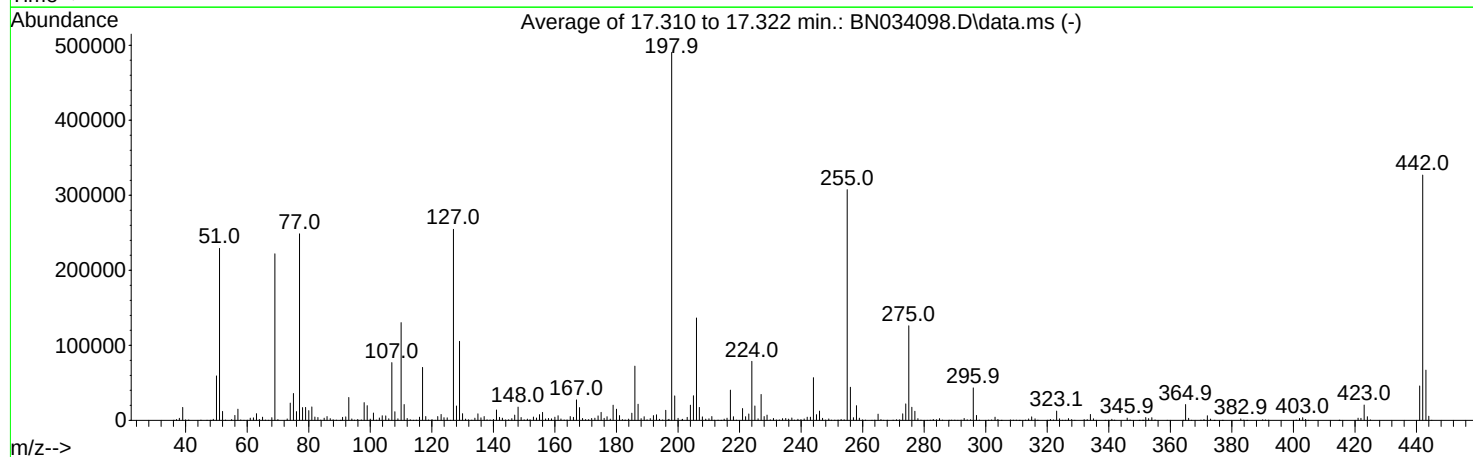


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034098.D
Acq On : 20 Sep 2024 22:24
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 18 16:09:28 2024

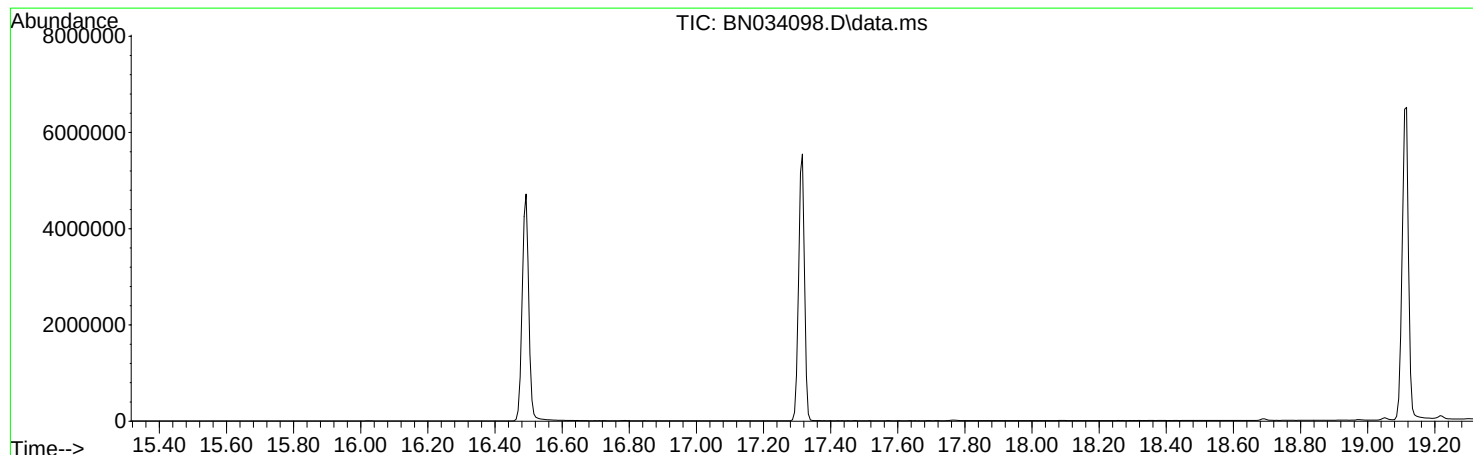

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	229346	PASS
68	69	0.00	2	1.6	3652	PASS
69	198	0.00	100	45.3	222085	PASS
70	69	0.00	2	0.5	1157	PASS
127	198	10	80	51.9	254677	PASS
197	198	0.00	2	0.3	1563	PASS
198	198	100	100	100.0	490304	PASS
199	198	5	9	6.6	32563	PASS
275	198	10	60	25.7	126021	PASS
365	198	1	100	4.3	21101	PASS
441	198	0.01	100	9.4	45952	PASS
442	442	50	100	100.0	326933	PASS
443	442	15	24	20.5	66928	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/21/2024	BNA_N	<u>BN034098.D</u>
Compound Name	Response	Retention Time
DDT	1607043	20.363
DDD	17568	19.969
DDE	123	19.404
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17691	1624734	1.09

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034098.D
Acq On : 20 Sep 2024 22:24
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 02:07:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

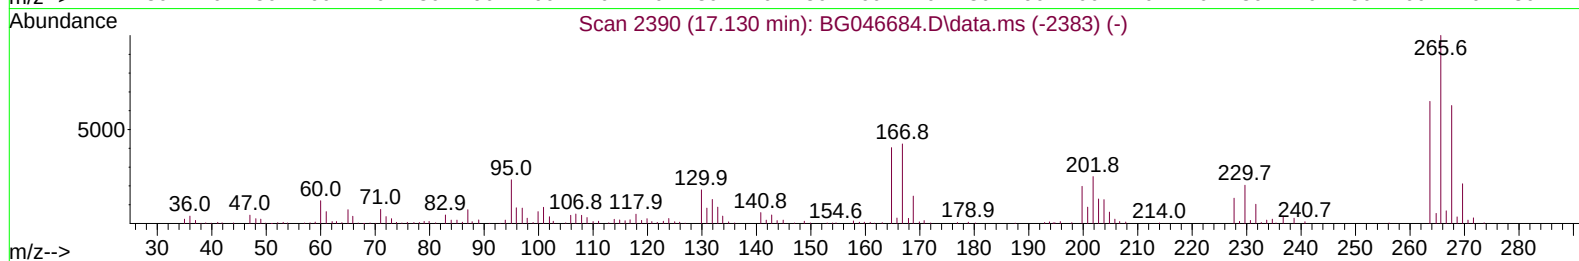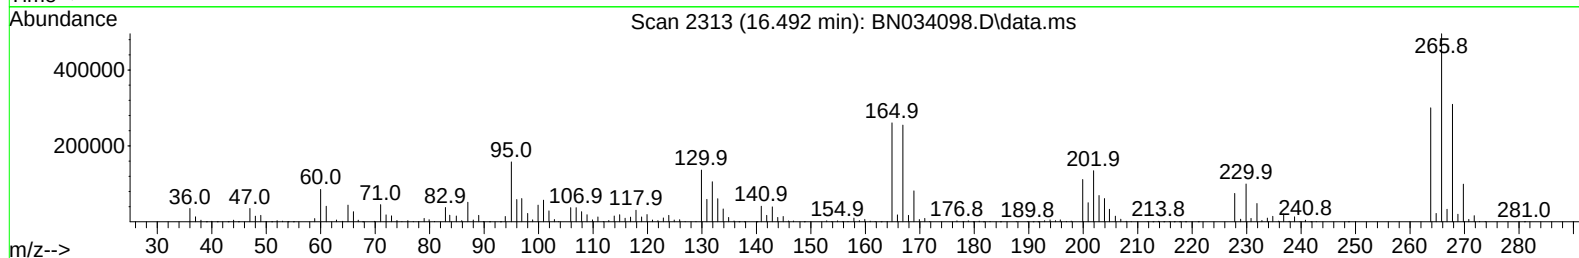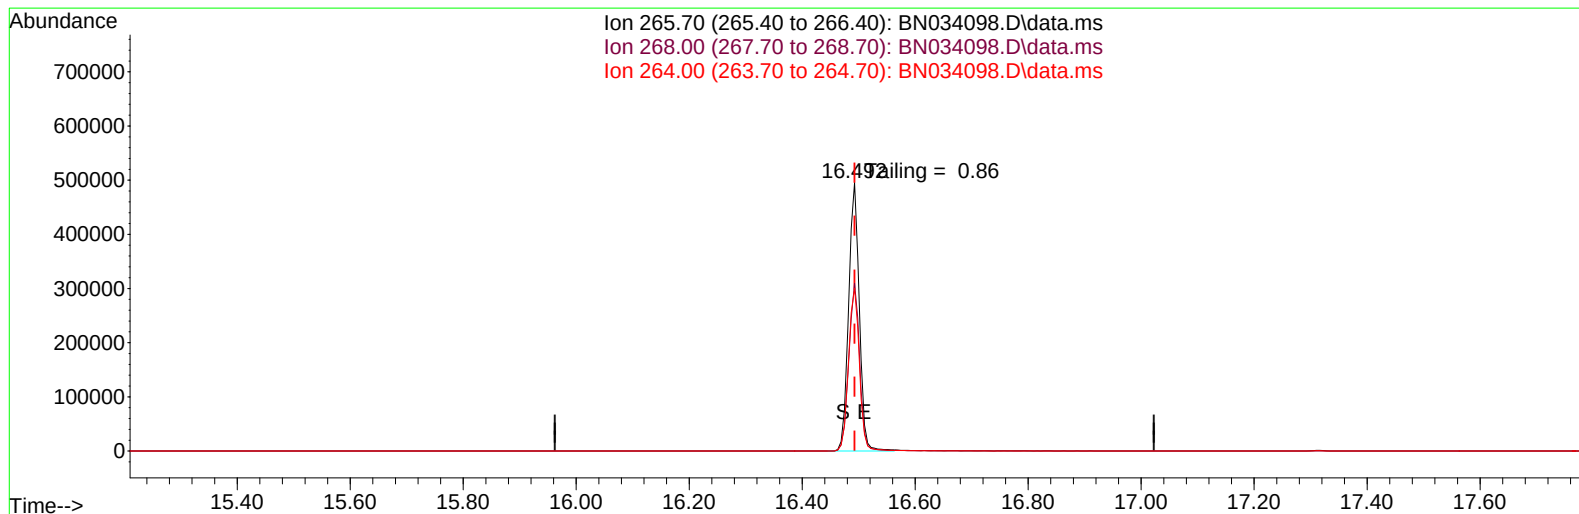

TIC: BN034098.D\data.ms

(70) Pentachlorophenol (C)

16.492min (0.000) 23726.54 ng




response 655610

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.52
264.00	61.60	60.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034098.D
Acq On : 20 Sep 2024 22:24
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 02:07:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

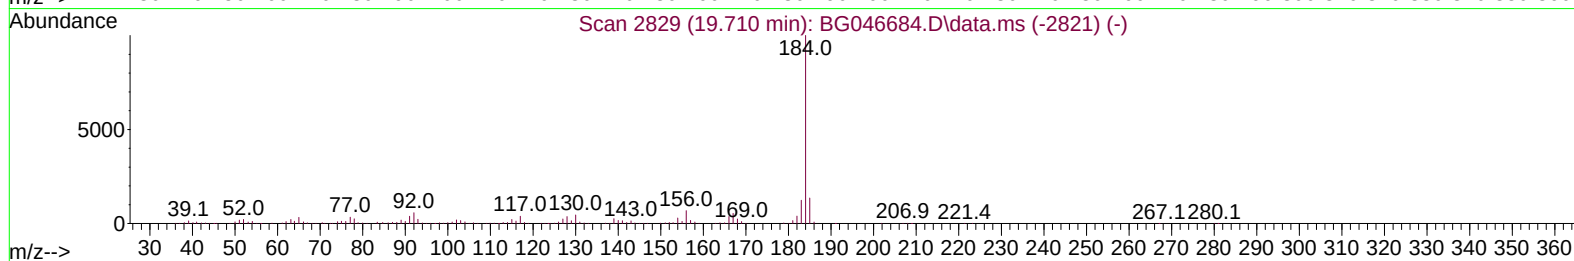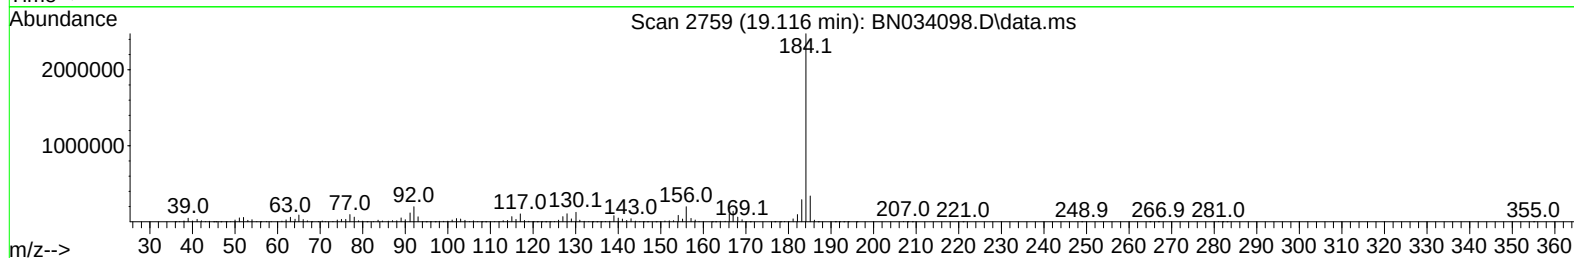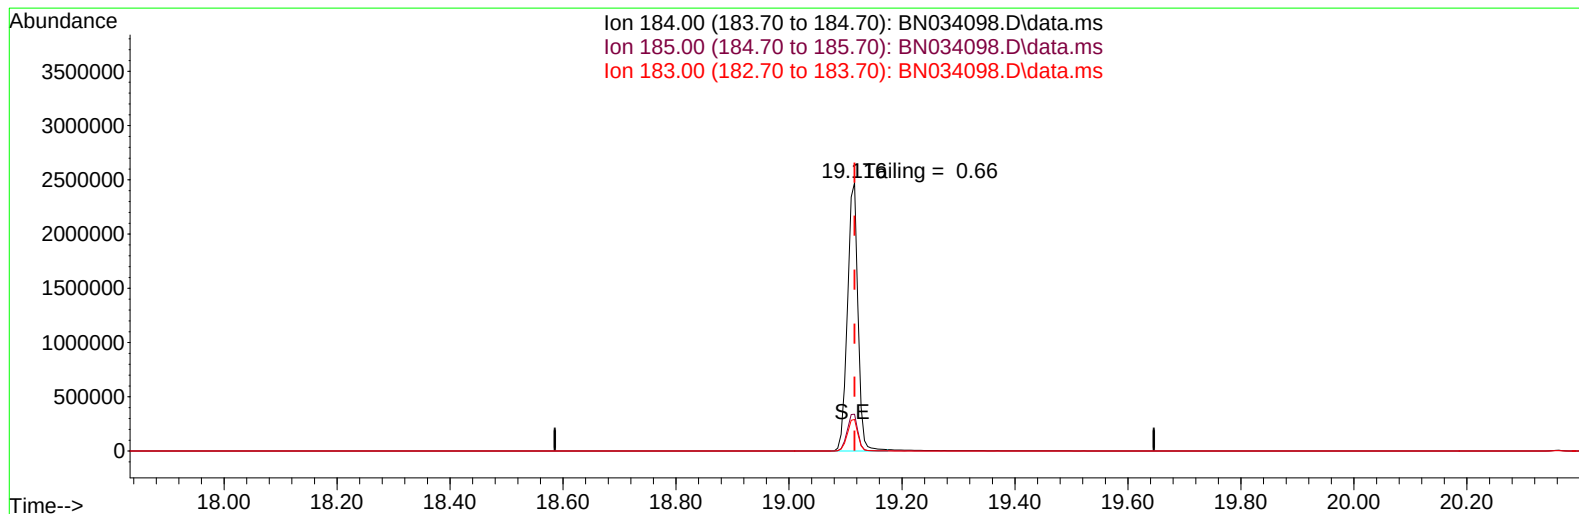

TIC: BN034098.D\data.ms

(77) Benzidine

19.116min (0.000) 0.00 ng

response 3222864

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.74
183.00	13.20	11.73
0.00	0.00	0.00