
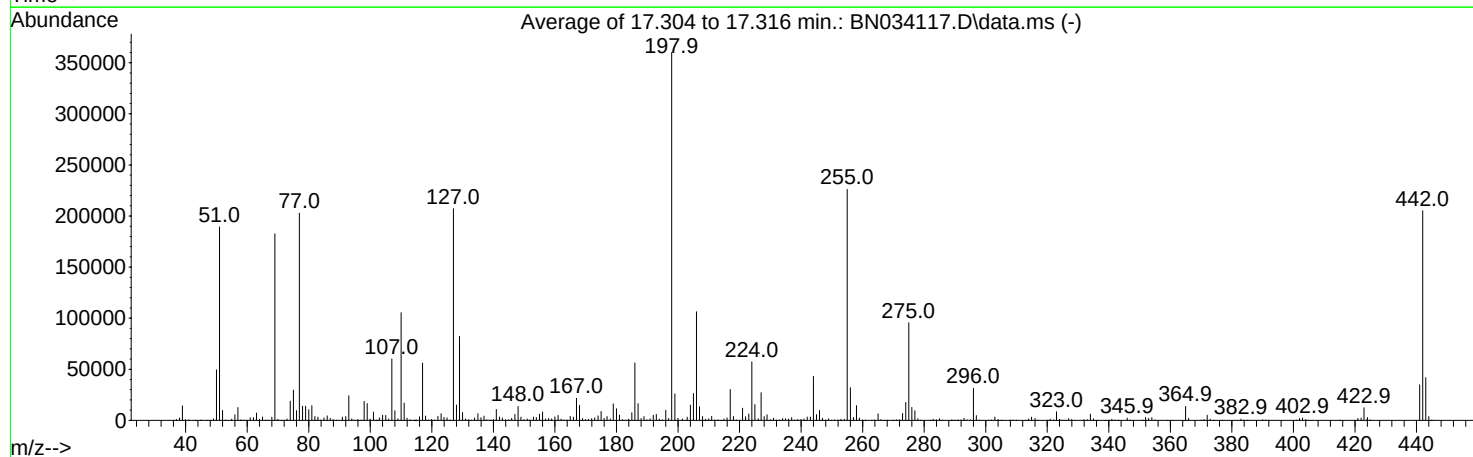


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034117.D
Acq On : 21 Sep 2024 10:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 18 16:09:28 2024

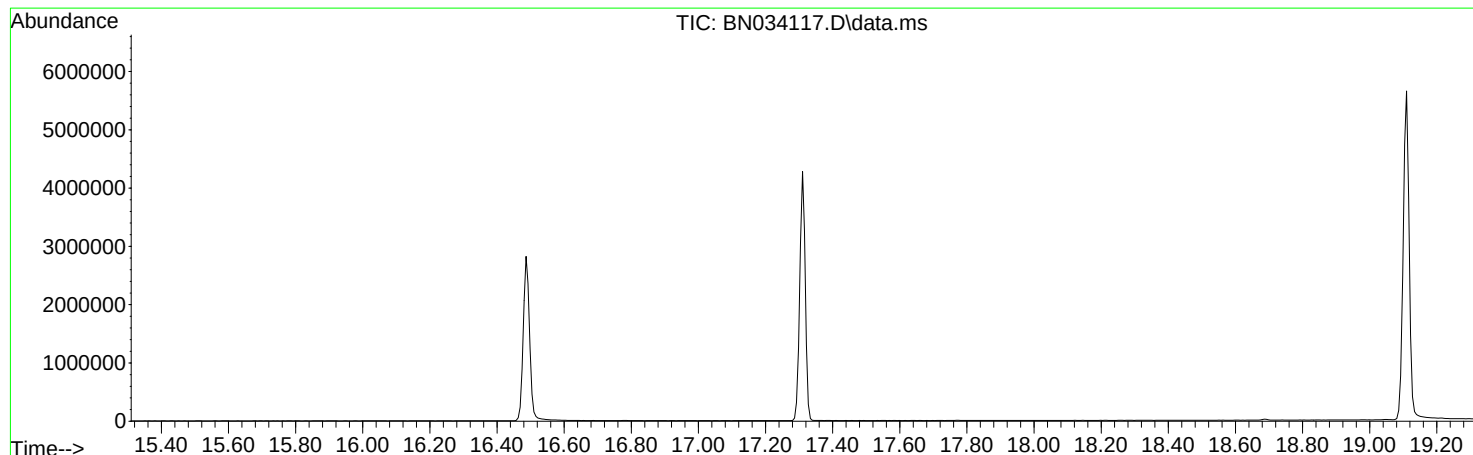

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	189301	PASS
68	69	0.00	2	1.7	3092	PASS
69	198	0.00	100	50.7	182528	PASS
70	69	0.00	2	0.6	1057	PASS
127	198	10	80	57.6	207253	PASS
197	198	0.00	2	0.5	1846	PASS
198	198	100	100	100.0	360021	PASS
199	198	5	9	7.2	26035	PASS
275	198	10	60	26.5	95496	PASS
365	198	1	100	3.8	13696	PASS
441	198	0.01	100	9.7	34781	PASS
442	442	50	100	100.0	205099	PASS
443	442	15	24	20.4	41797	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/21/2024	BNA_N	<u>BN034117.D</u>
Compound Name	Response	Retention Time
DDT	1340796	20.363
DDD	14211	19.963
DDE	63	19.404
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14274	1355070	1.05

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034117.D
Acq On : 21 Sep 2024 10:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 23 01:13:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

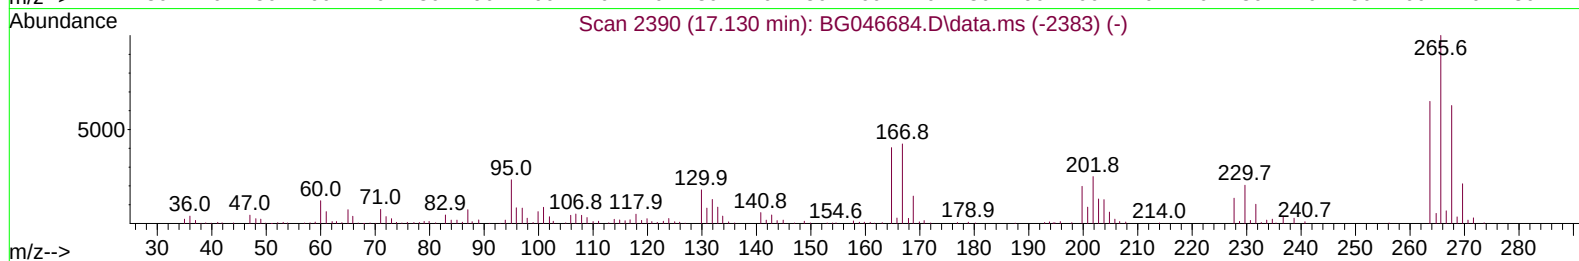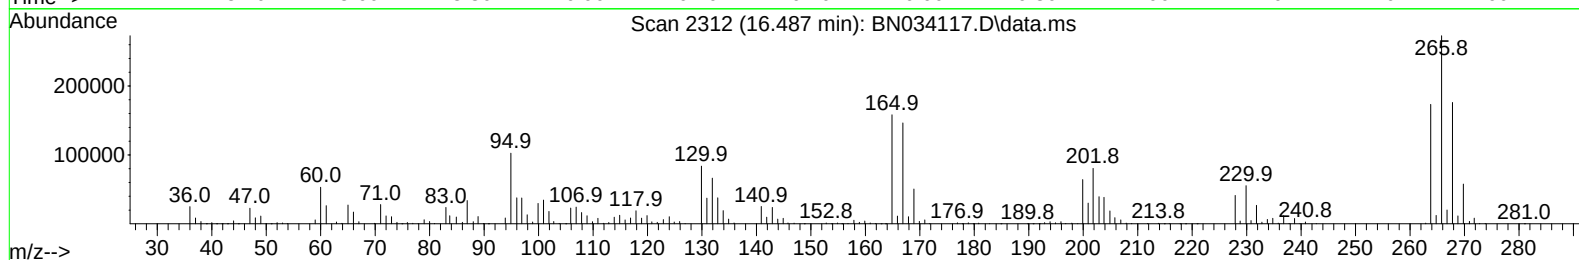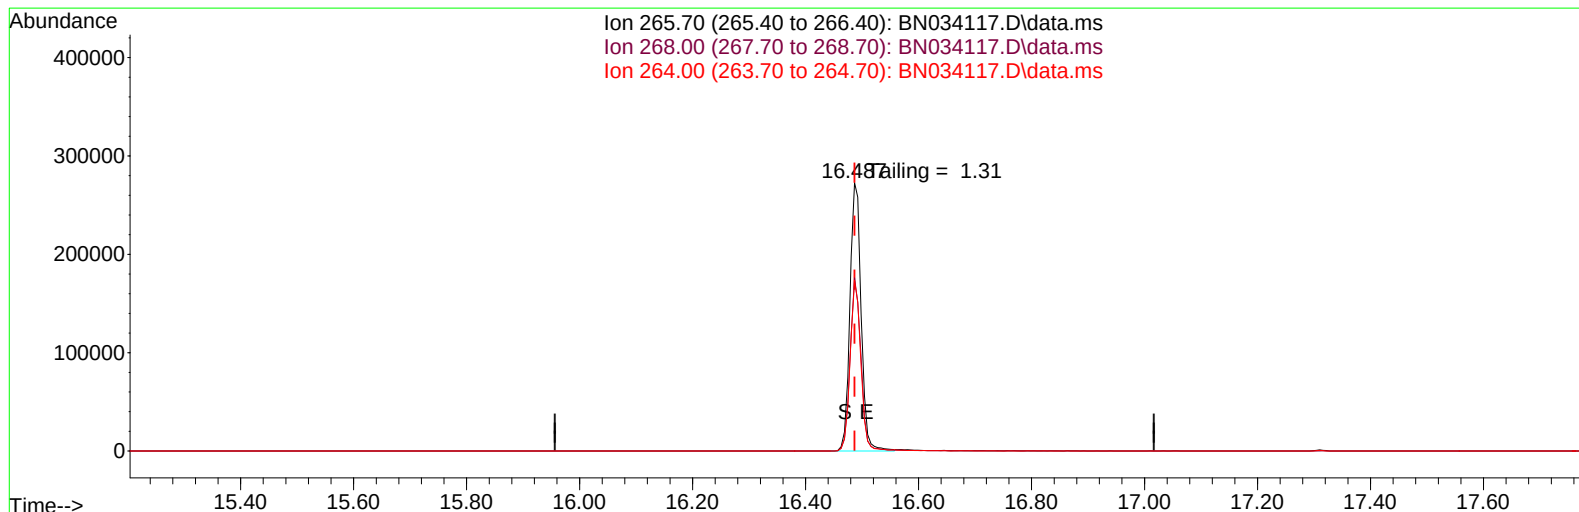

TIC: BN034117.D\data.ms

(70) Pentachlorophenol (C)

16.487min (0.000) 17685.57 ng




response 379457

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.49
264.00	61.60	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034117.D
Acq On : 21 Sep 2024 10:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 23 01:13:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

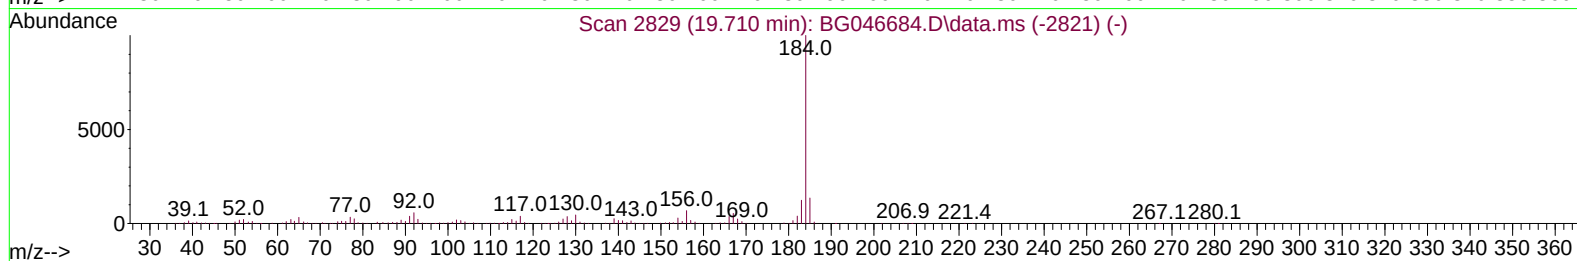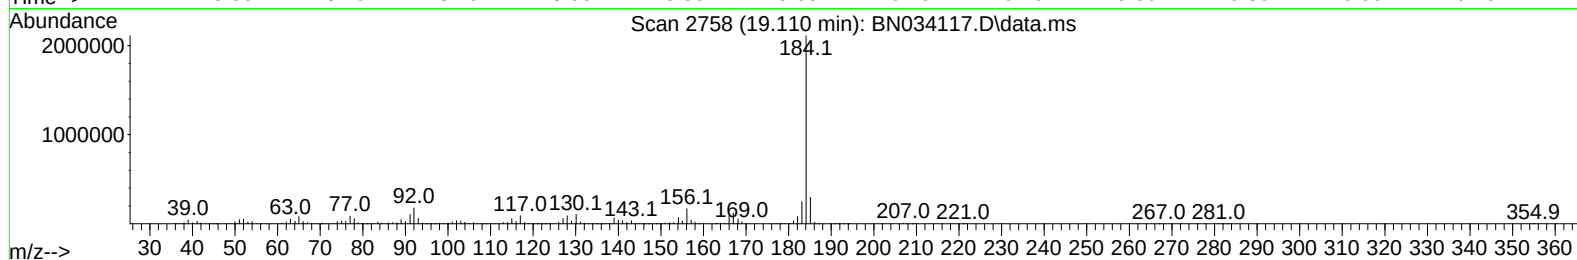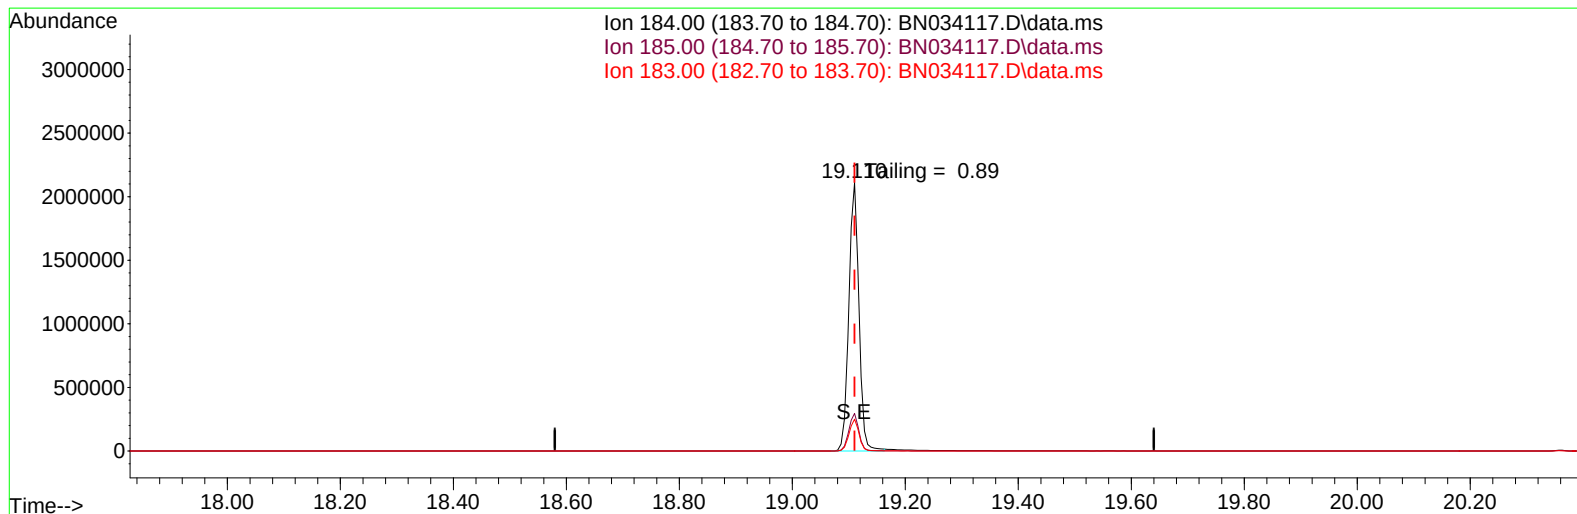

TIC: BN034117.D\data.ms

(77) Benzidine

19.110min (0.000) 0.00 ng

response 2676676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	11.87
0.00	0.00	0.00