
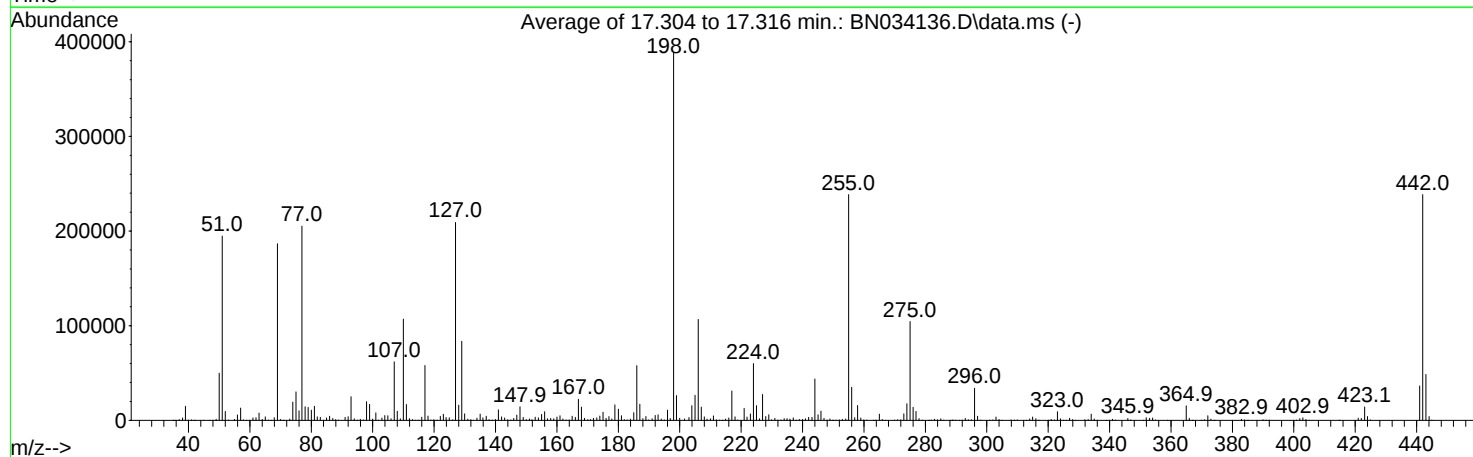


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034136.D
Acq On : 21 Sep 2024 22:43
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 18 16:09:28 2024

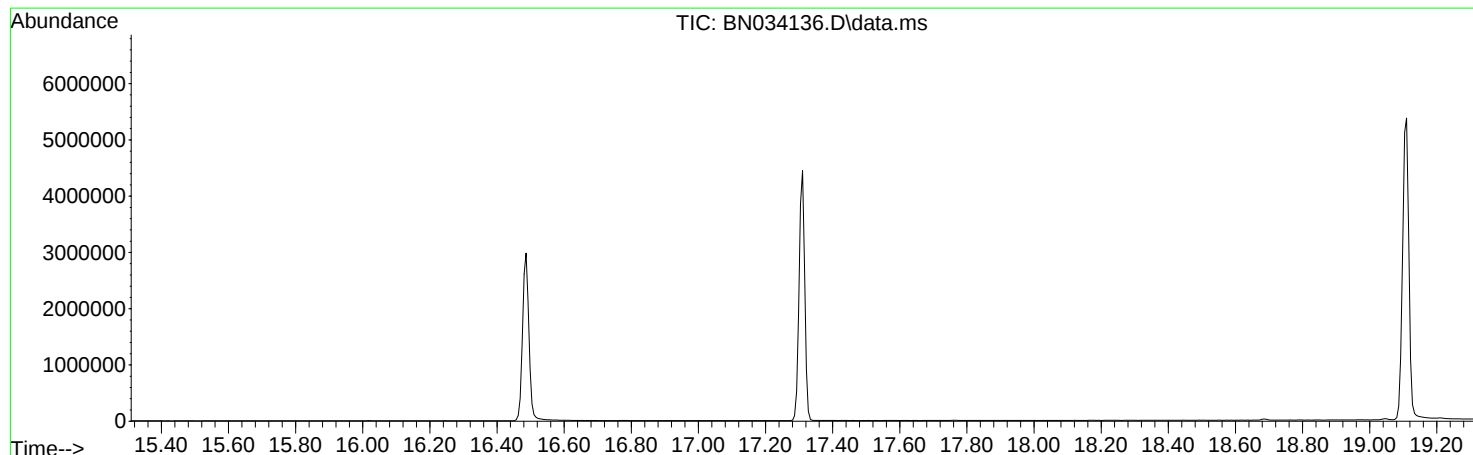

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	194744	PASS
68	69	0.00	2	1.5	2863	PASS
69	198	0.00	100	48.0	186712	PASS
70	69	0.00	2	0.6	1035	PASS
127	198	10	80	53.8	209131	PASS
197	198	0.00	2	0.5	1991	PASS
198	198	100	100	100.0	388672	PASS
199	198	5	9	6.7	26224	PASS
275	198	10	60	26.9	104523	PASS
365	198	1	100	4.0	15460	PASS
441	198	0.01	100	9.3	36304	PASS
442	442	50	100	100.0	238613	PASS
443	442	15	24	20.3	48491	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/21/2024	BNA_N	<u>BN034136.D</u>
Compound Name	Response	Retention Time
DDT	1280819	20.357
DDD	17554	19.963
DDE	199	19.404
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17753	1298572	1.37

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034136.D
Acq On : 21 Sep 2024 22:43
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 23 01:15:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

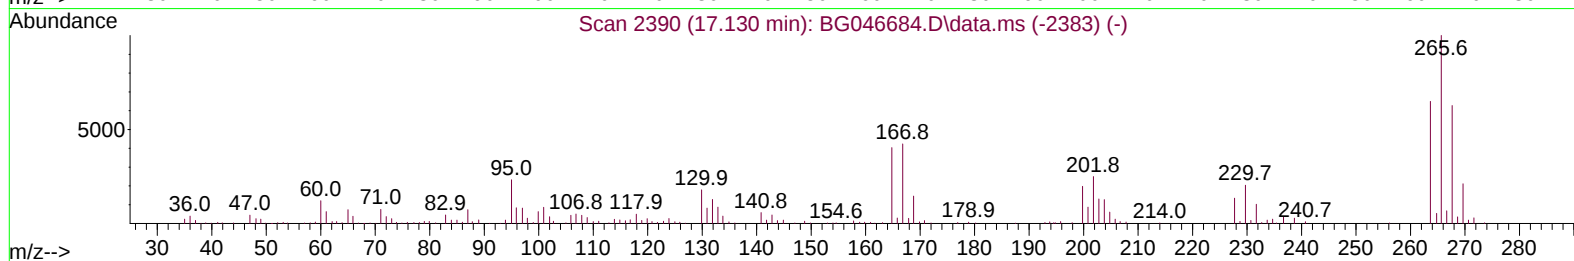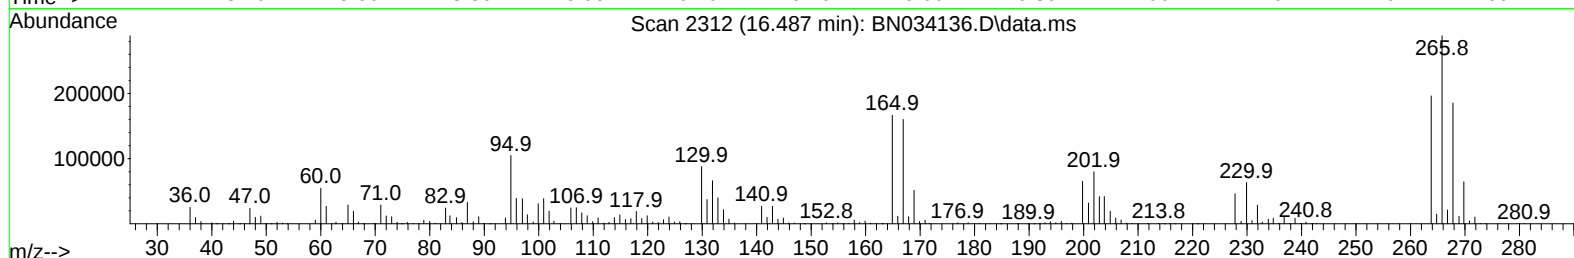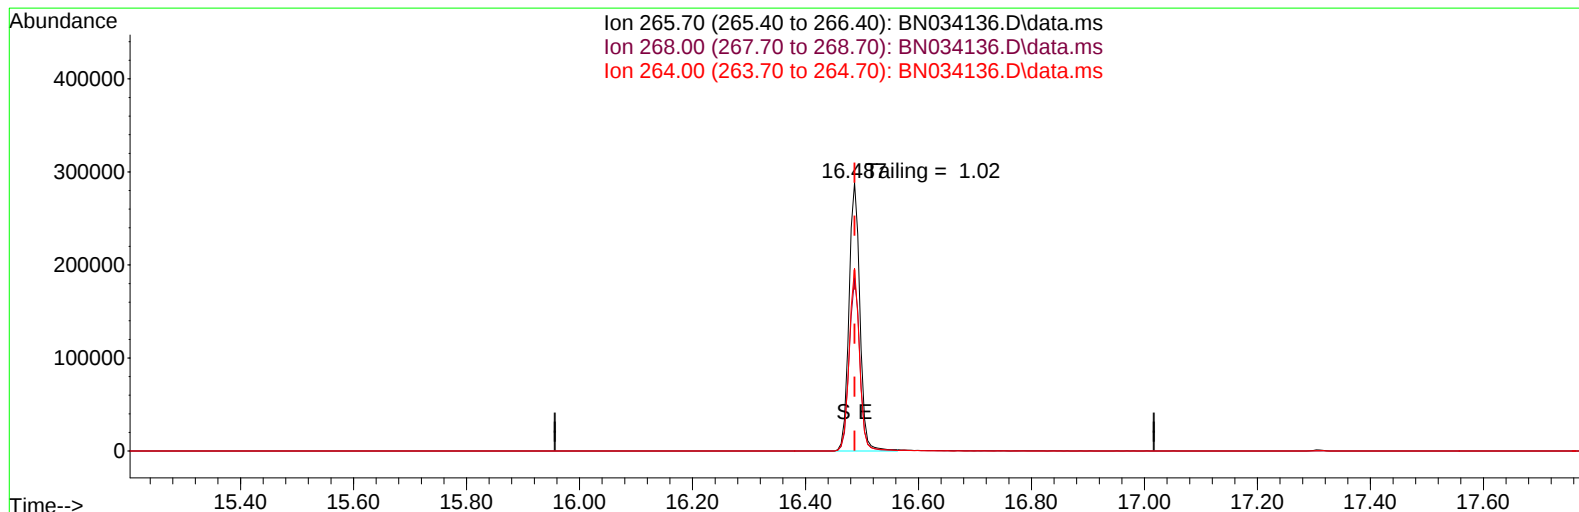

TIC: BN034136.D\data.ms

(70) Pentachlorophenol (C)

16.487min (+ 0.000) 18362.98 ng




response 389524

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.31
264.00	61.60	68.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034136.D
Acq On : 21 Sep 2024 22:43
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 23 01:15:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

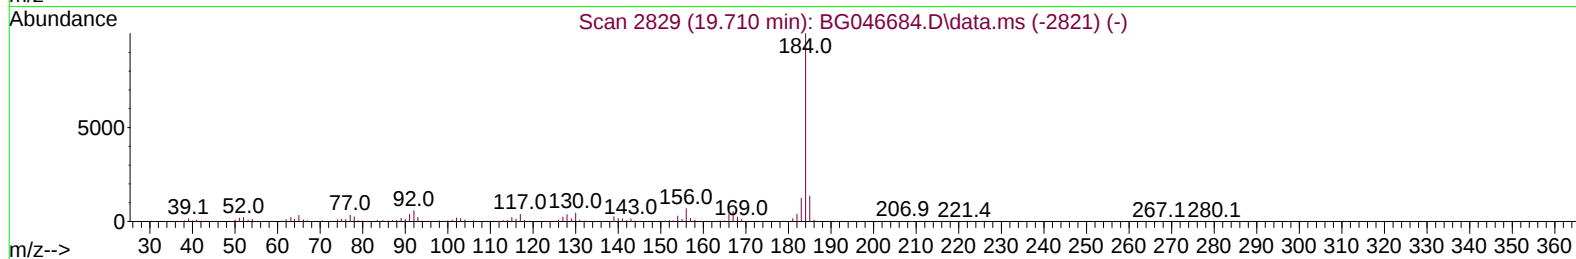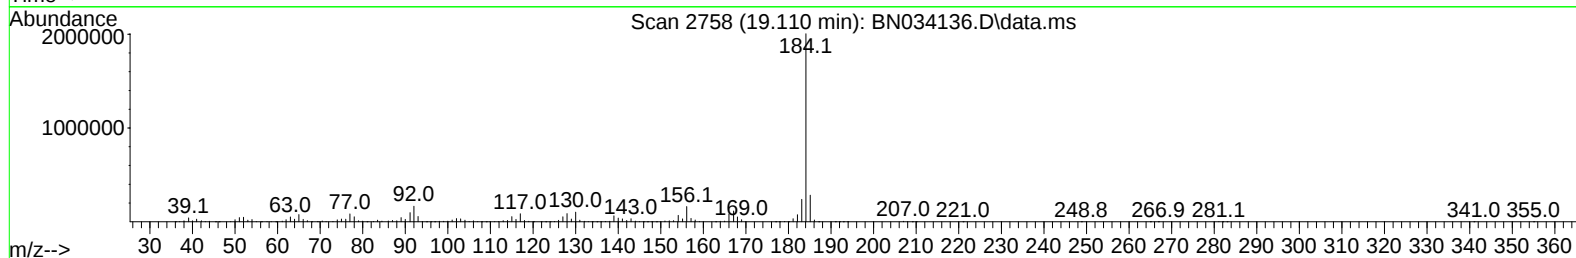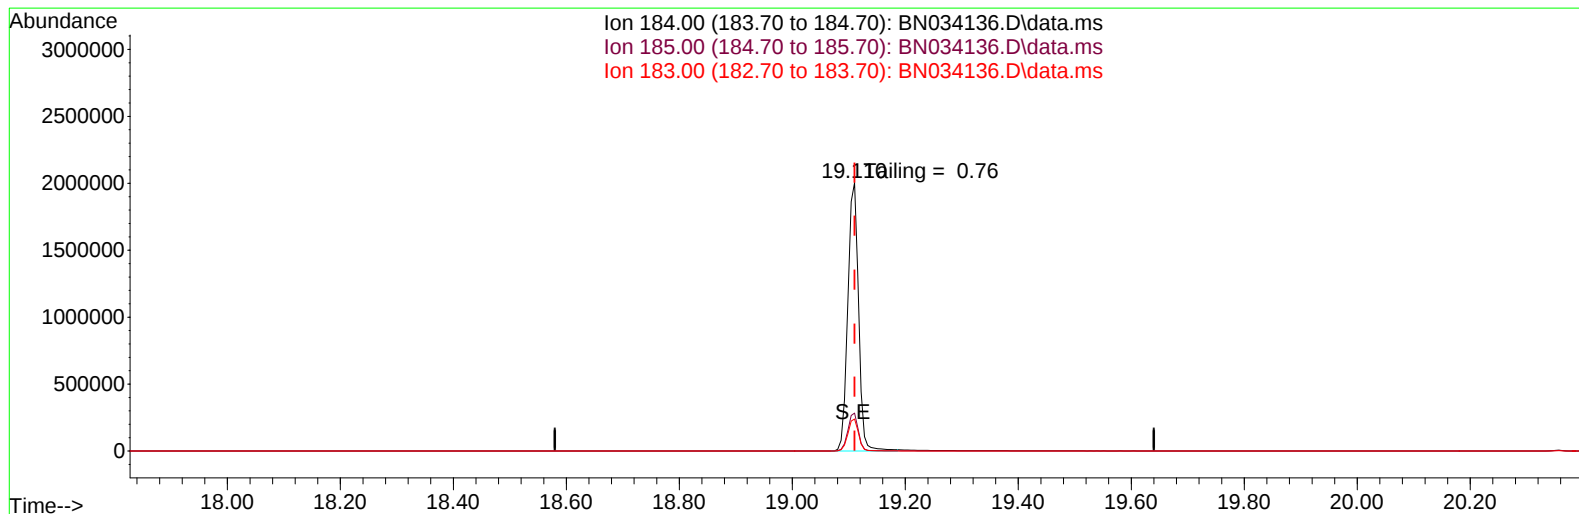

TIC: BN034136.D\data.ms

(77) Benzidine

19.110min (+ 0.000) 0.00 ng

response 2674968

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	11.94
0.00	0.00	0.00