

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002810.D
 Acq On : 21 Sep 2018 09:28
 Operator : JU/SJ
 Sample : J4900-16
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 21 23:10:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:09:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	1610	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.42	136	6508	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	3645	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	642533	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.25
20) Perylene-d12	23.46	264	6093	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	3712	0.40	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.28	166	1122	0.084	ng/ul#	21
23) Benzo(a)pyrene	23.30	252	1951	0.101	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
Data File : BN002810.D
Acq On : 21 Sep 2018 09:28
Operator : JU/SJ
Sample : J4900-16
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 21 23:10:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 23:09:42 2018
Response via : Initial Calibration




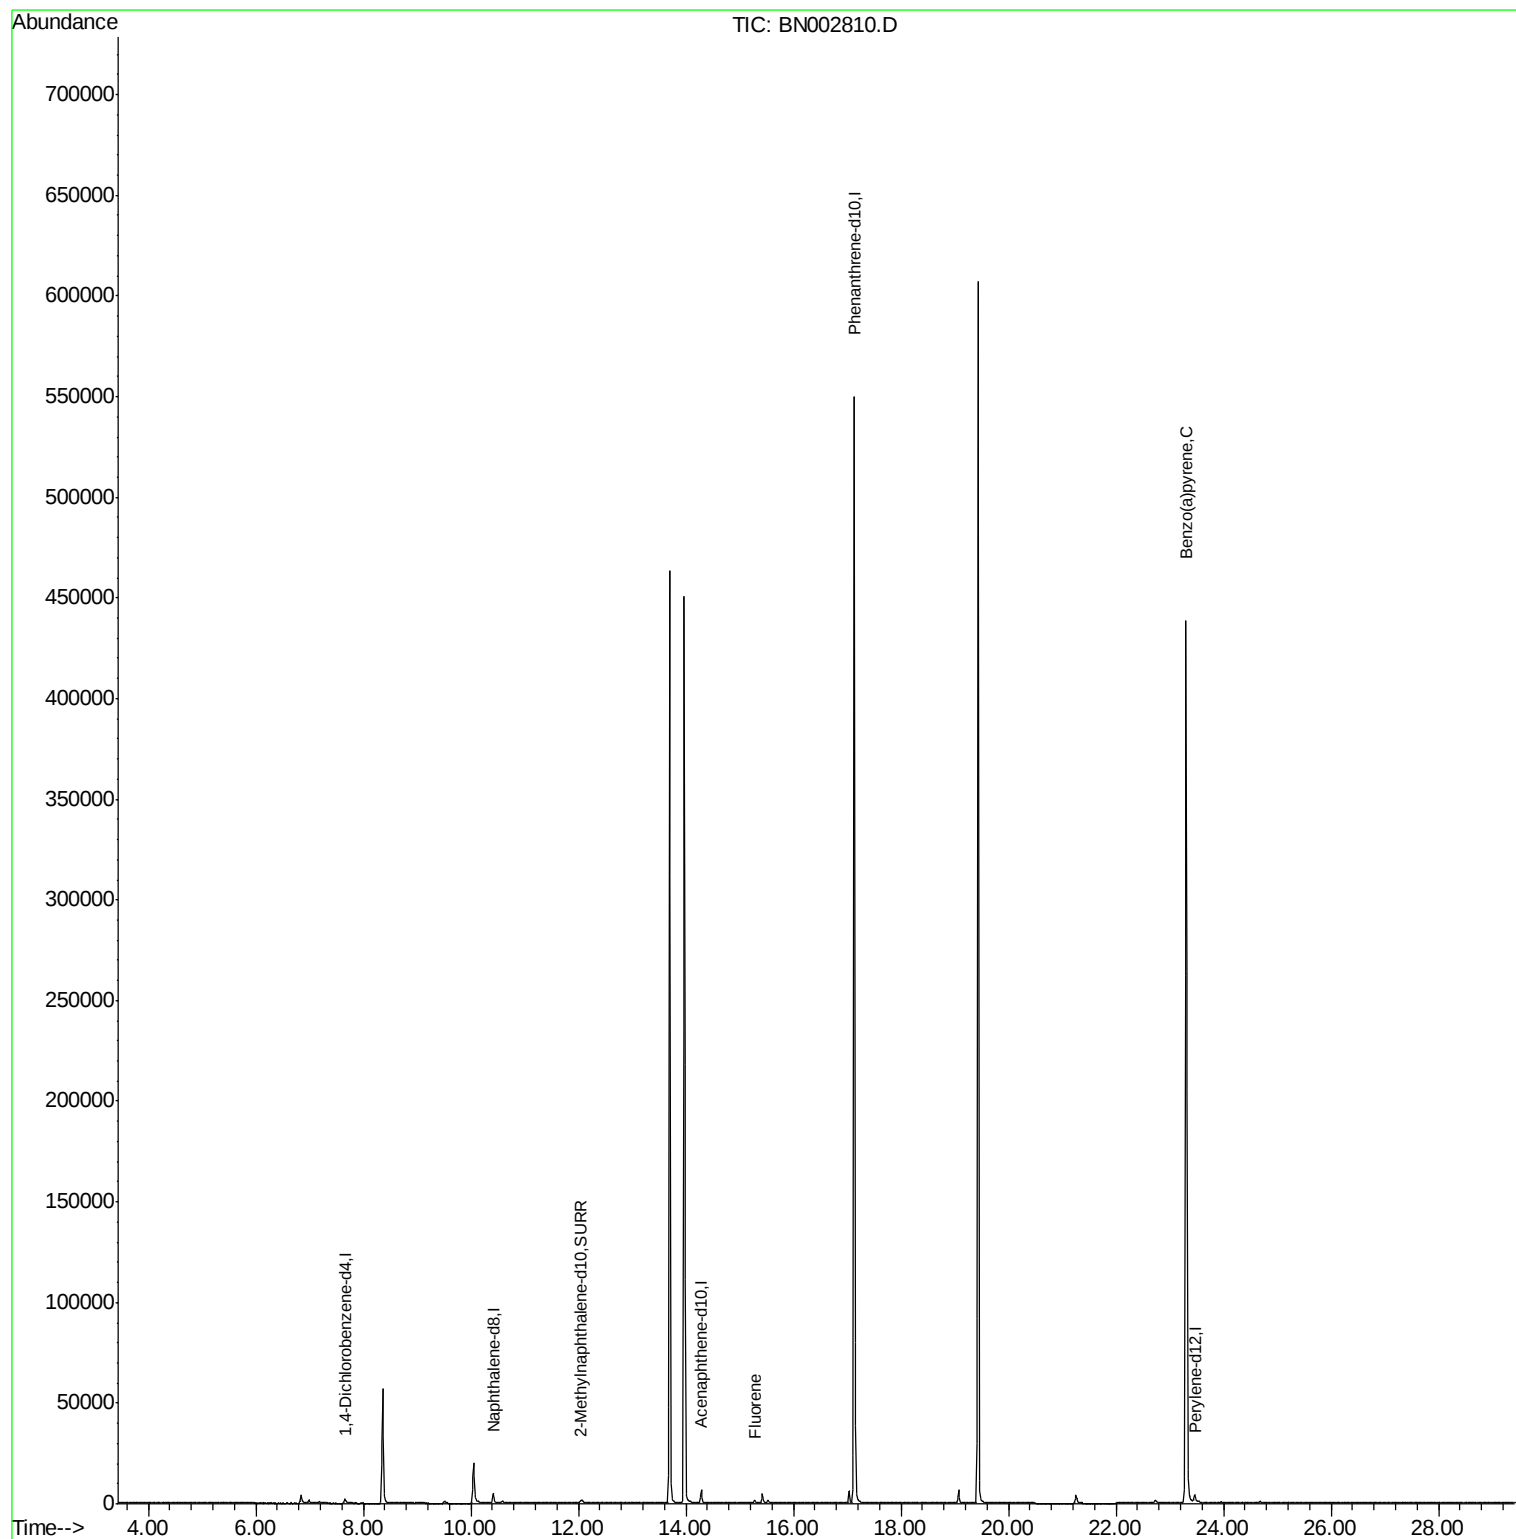


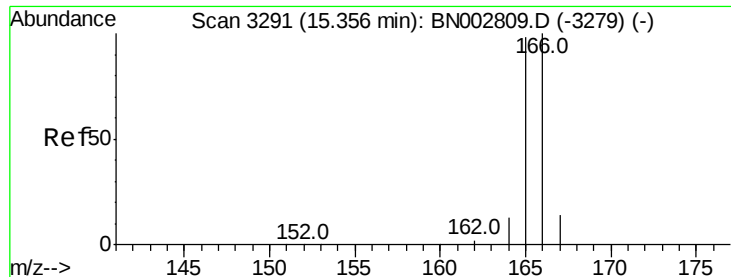

#9
Fluorene
 Concen: 0.084 ng/ul
 RT: 15.28 min Scan# 3275
 Delta R.T. -0.07 min
 Lab File: BN002810.D
 Acq: 21 Sep 2018 09:28

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 1122
 Ion Ratio Lower Upper
 166 100
 165 9.3 73.4 110.2#
 167 36.4 14.6 22.0#

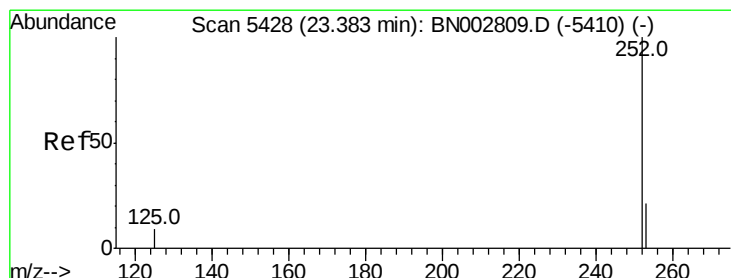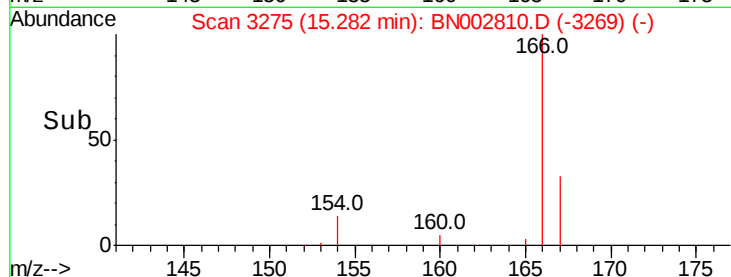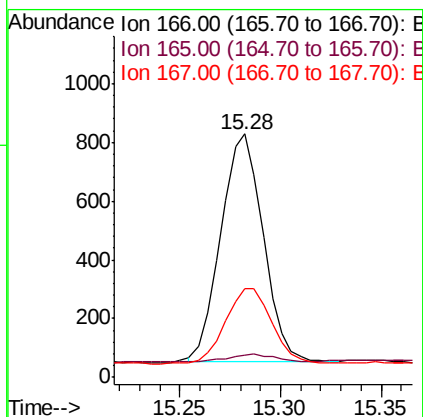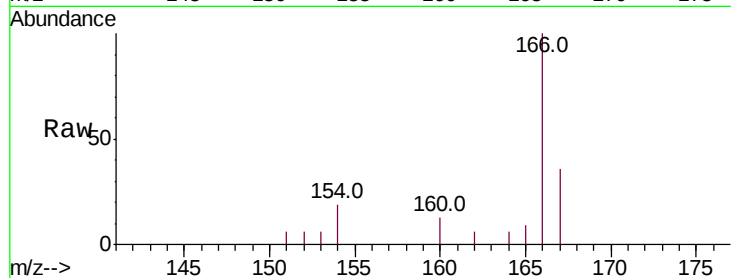

#23
Benzo(a)pyrene
 Concen: 0.101 ng/ul
 RT: 23.30 min Scan# 5401
 Delta R.T. -0.08 min
 Lab File: BN002810.D
 Acq: 21 Sep 2018 09:28

Tgt Ion:252 Resp: 1951
 Ion Ratio Lower Upper
 252 100
 253 38.3 16.0 24.0#
 125 27.5 12.0 18.0#

