

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002813.D
 Acq On : 21 Sep 2018 11:13
 Operator : JU/SJ
 Sample : J4874-23
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 21 23:10:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:09:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	1630	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.42	136	6363	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	3475	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	611962	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.25
20) Perylene-d12	23.46	264	6364	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	3767	0.41	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.28	166	1078	0.084	ng/ul#	21
23) Benzo(a)pyrene	23.30	252	1933	0.096	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
Data File : BN002813.D
Acq On : 21 Sep 2018 11:13
Operator : JU/SJ
Sample : J4874-23
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 21 23:10:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 23:09:42 2018
Response via : Initial Calibration




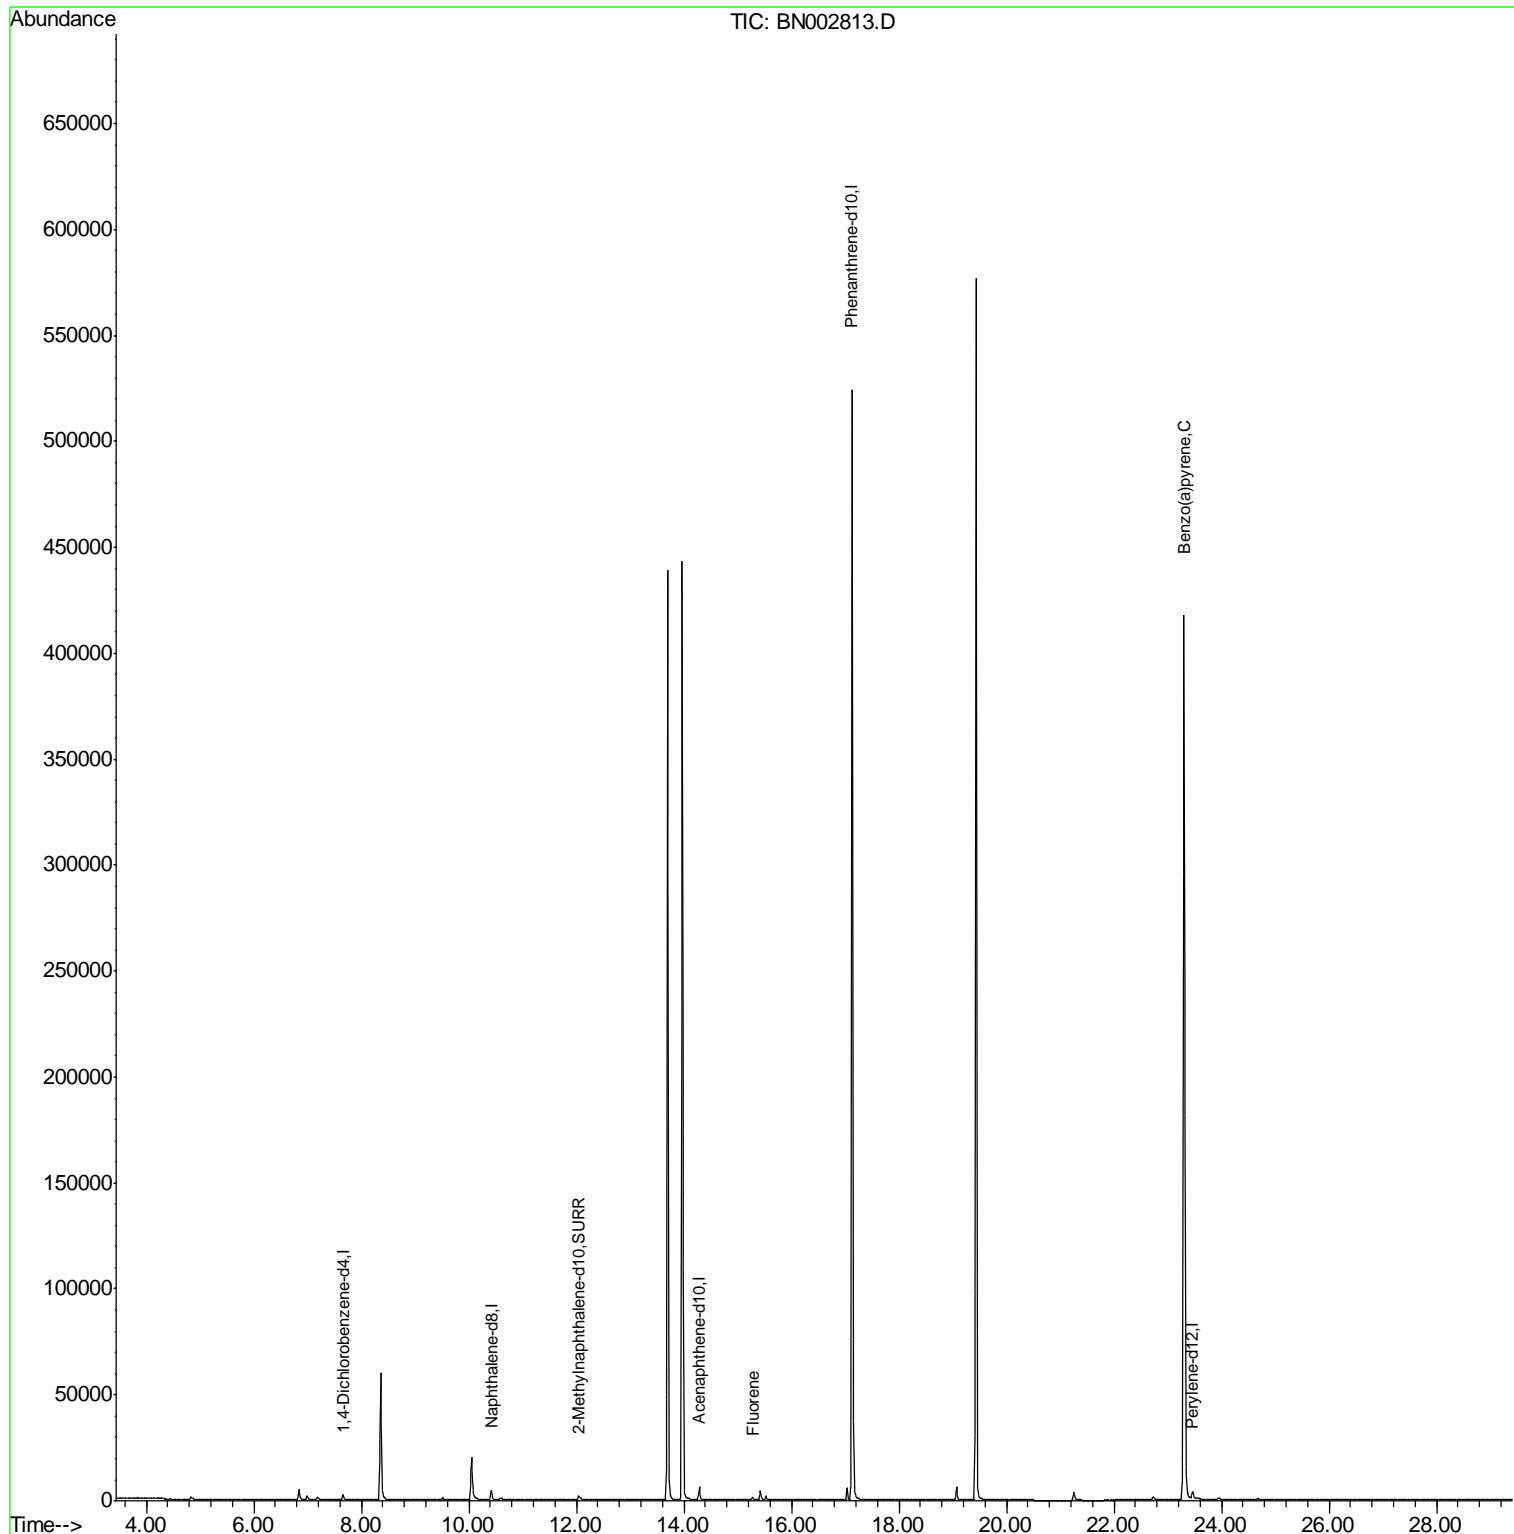


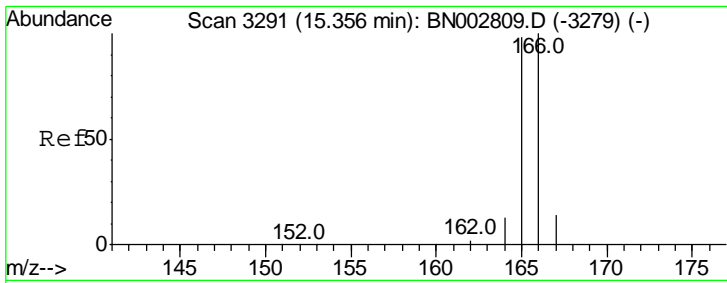

#9
 Fluorene
 Concen: 0.084 ng/ul
 RT: 15.28 min Scan# 3275
 Delta R.T. -0.07 min
 Lab File: BN002813.D
 Acq: 21 Sep 2018 11:13

Instrument :
 BNA_N
 ClientSampled :

Tgt Ion	Resp	Lower	Upper
166	1078		
165	9.8	73.4	110.2#
167	37.1	14.6	22.0#

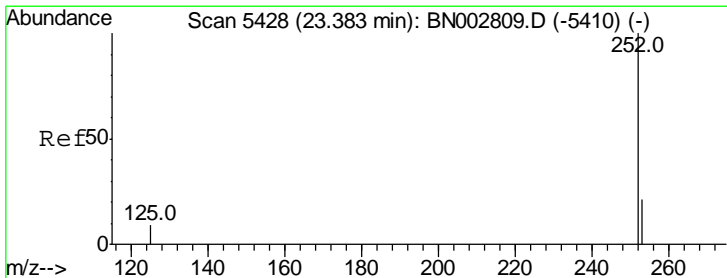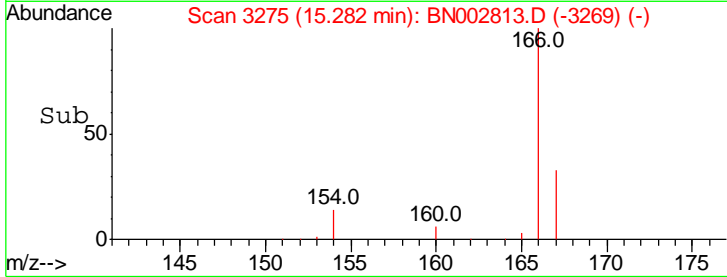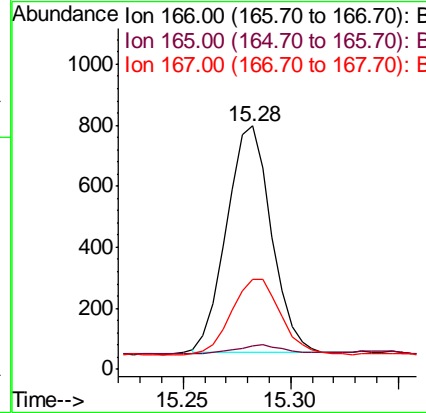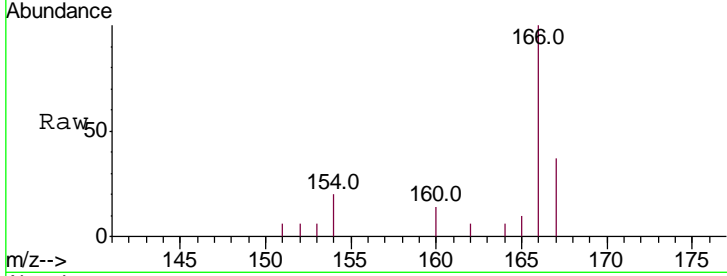

#23
 Benzo(a)pyrene
 Concen: 0.096 ng/ul
 RT: 23.30 min Scan# 5401
 Delta R.T. -0.08 min
 Lab File: BN002813.D
 Acq: 21 Sep 2018 11:13

Tgt Ion	Resp	Lower	Upper
252	1933		
253	38.2	16.0	24.0#
125	26.6	12.0	18.0#

