

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002822.D
 Acq On : 21 Sep 2018 17:34
 Operator : JU/SJ
 Sample : J4900-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 21 23:49:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	1321	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	5091	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	2788	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	531405	0.40	ng/ul	0.08
16) Chrysene-d12	21.26	240	3457	0.40	ng/ul	0.00
20) Perylene-d12	23.48	264	6057	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	3071	0.42	ng/ul	0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.43	202	895	0.079	ng/ul#	1
23) Benzo(a)pyrene	23.32	252	2100	0.110	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
Data File : BN002822.D
Acq On : 21 Sep 2018 17:34
Operator : JU/SJ
Sample : J4900-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 21 23:49:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 23:48:47 2018
Response via : Initial Calibration




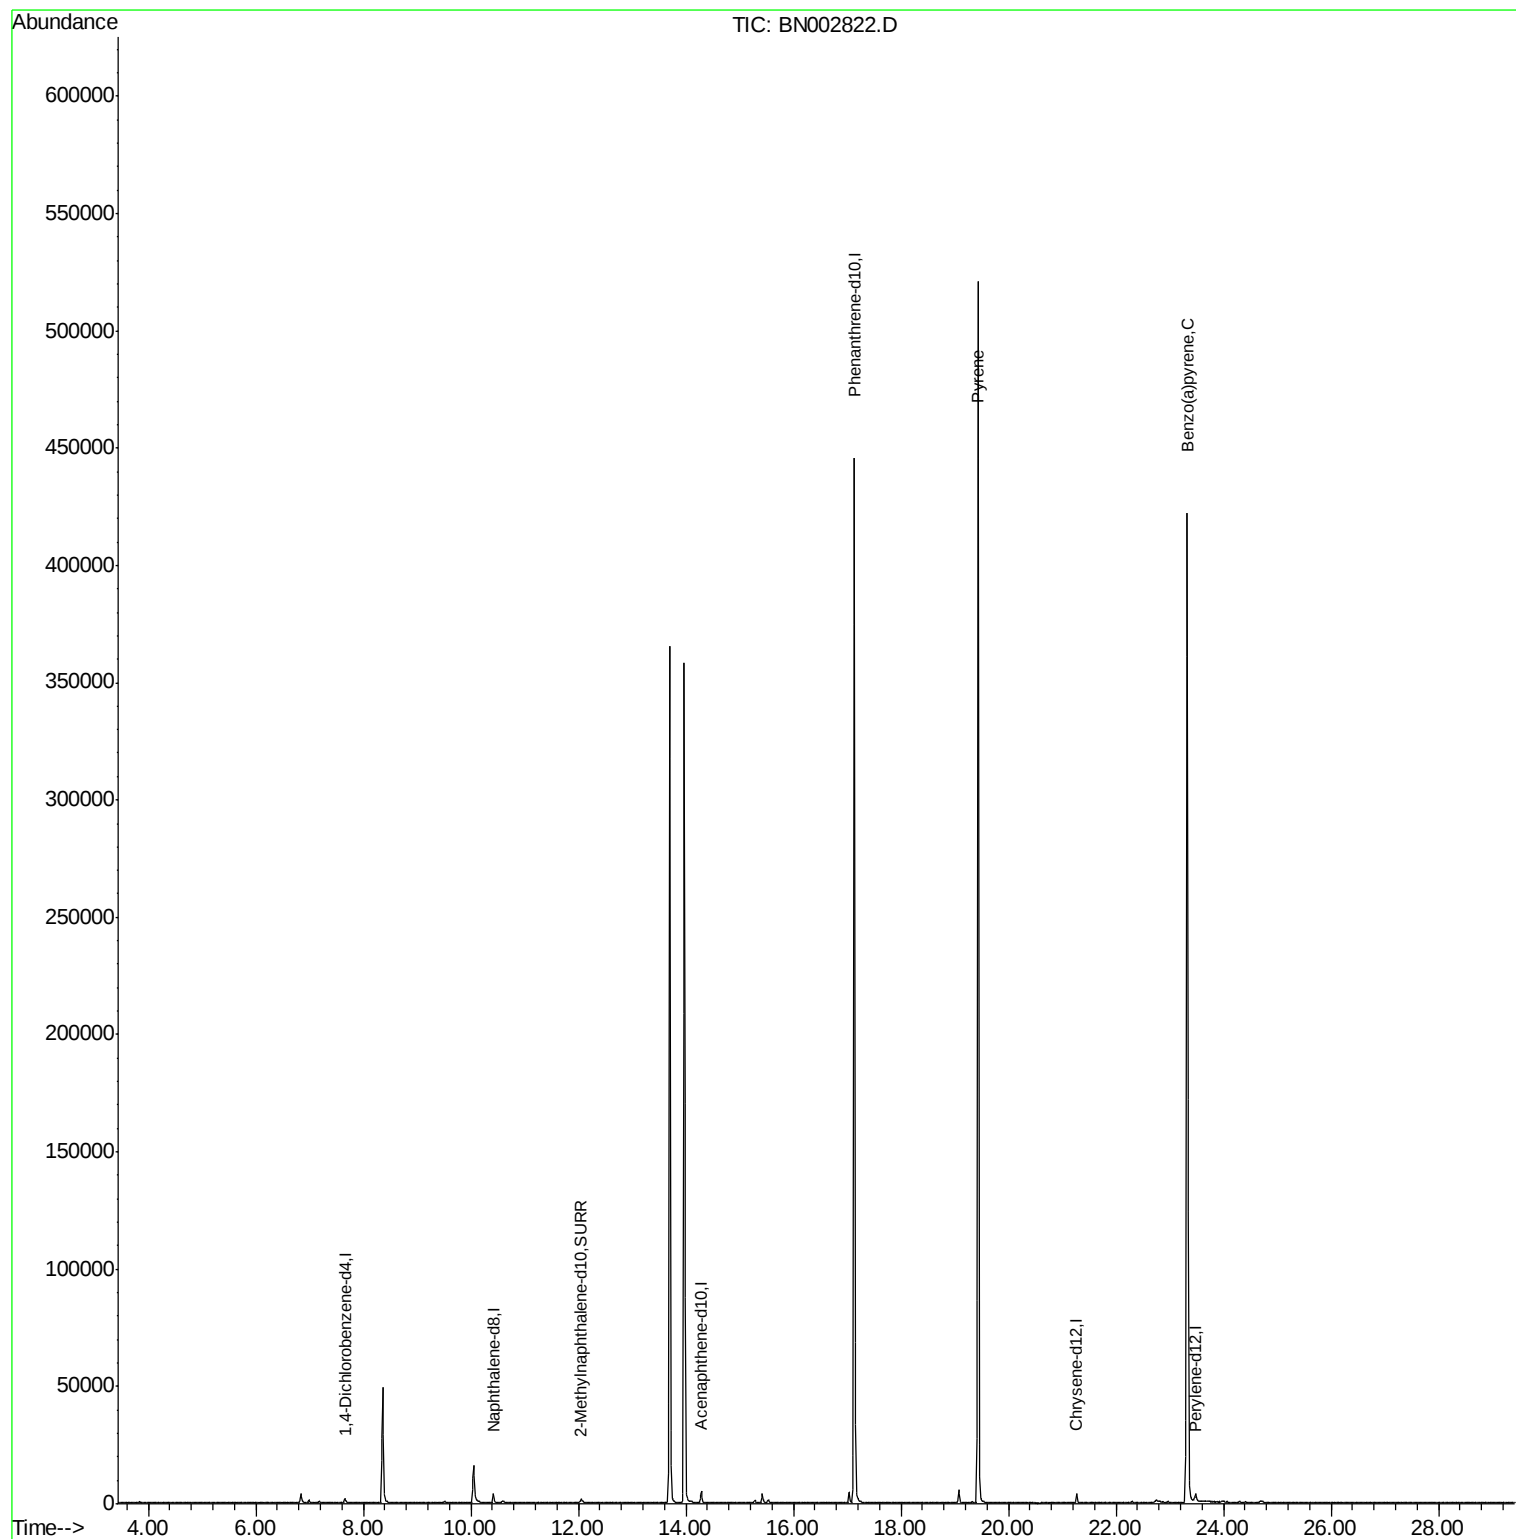


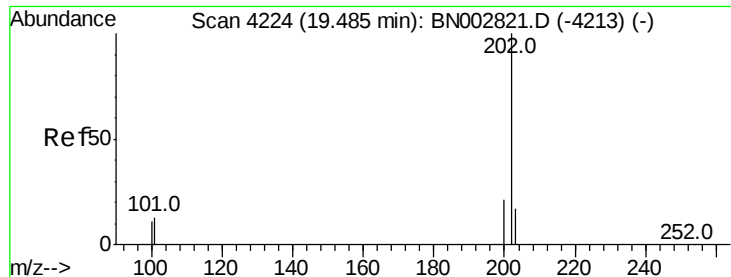

#17
Pvrene
Concen: 0.079 ng/ul
RT: 19.43 min Scan# 4213
Delta R.T. -0.05 min
Lab File: BN002822.D
Acq: 21 Sep 2018 17:34

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 895
Ion Ratio Lower Upper
202 100
101 139.5 12.0 18.0#
100 877.8 8.0 12.0#

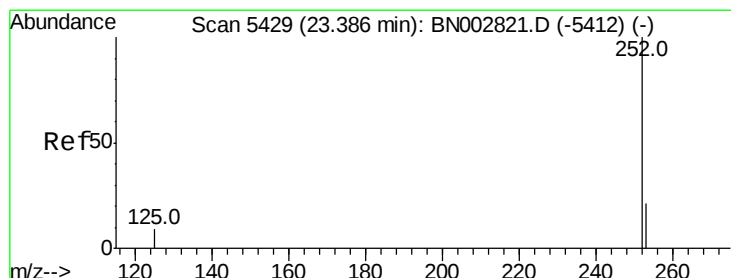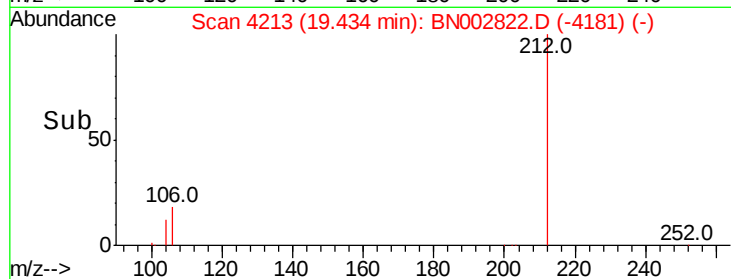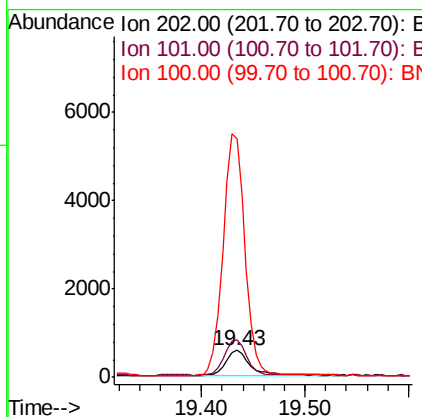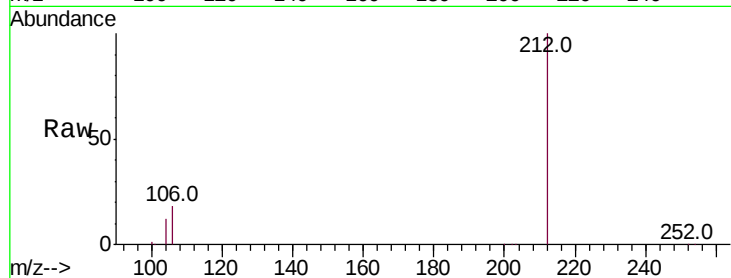

#23
Benzo(a)pyrene
Concen: 0.110 ng/ul
RT: 23.32 min Scan# 5408
Delta R.T. -0.06 min
Lab File: BN002822.D
Acq: 21 Sep 2018 17:34

Tgt Ion:252 Resp: 2100
Ion Ratio Lower Upper
252 100
253 38.7 16.0 24.0#
125 30.5 12.0 18.0#

