

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002823.D
 Acq On : 21 Sep 2018 18:09
 Operator : JU/SJ
 Sample : J4900-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 21 23:49:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	1416	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	5635	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	3108	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	525952	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.25
20) Perylene-d12	23.46	264	5675	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	2798	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
9) Fluorene	15.28	166	869	0.076	ng/ul#	23
23) Benzo(a)pyrene	23.31	252	1707	0.095	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
Data File : BN002823.D
Acq On : 21 Sep 2018 18:09
Operator : JU/SJ
Sample : J4900-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 21 23:49:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 23:48:47 2018
Response via : Initial Calibration




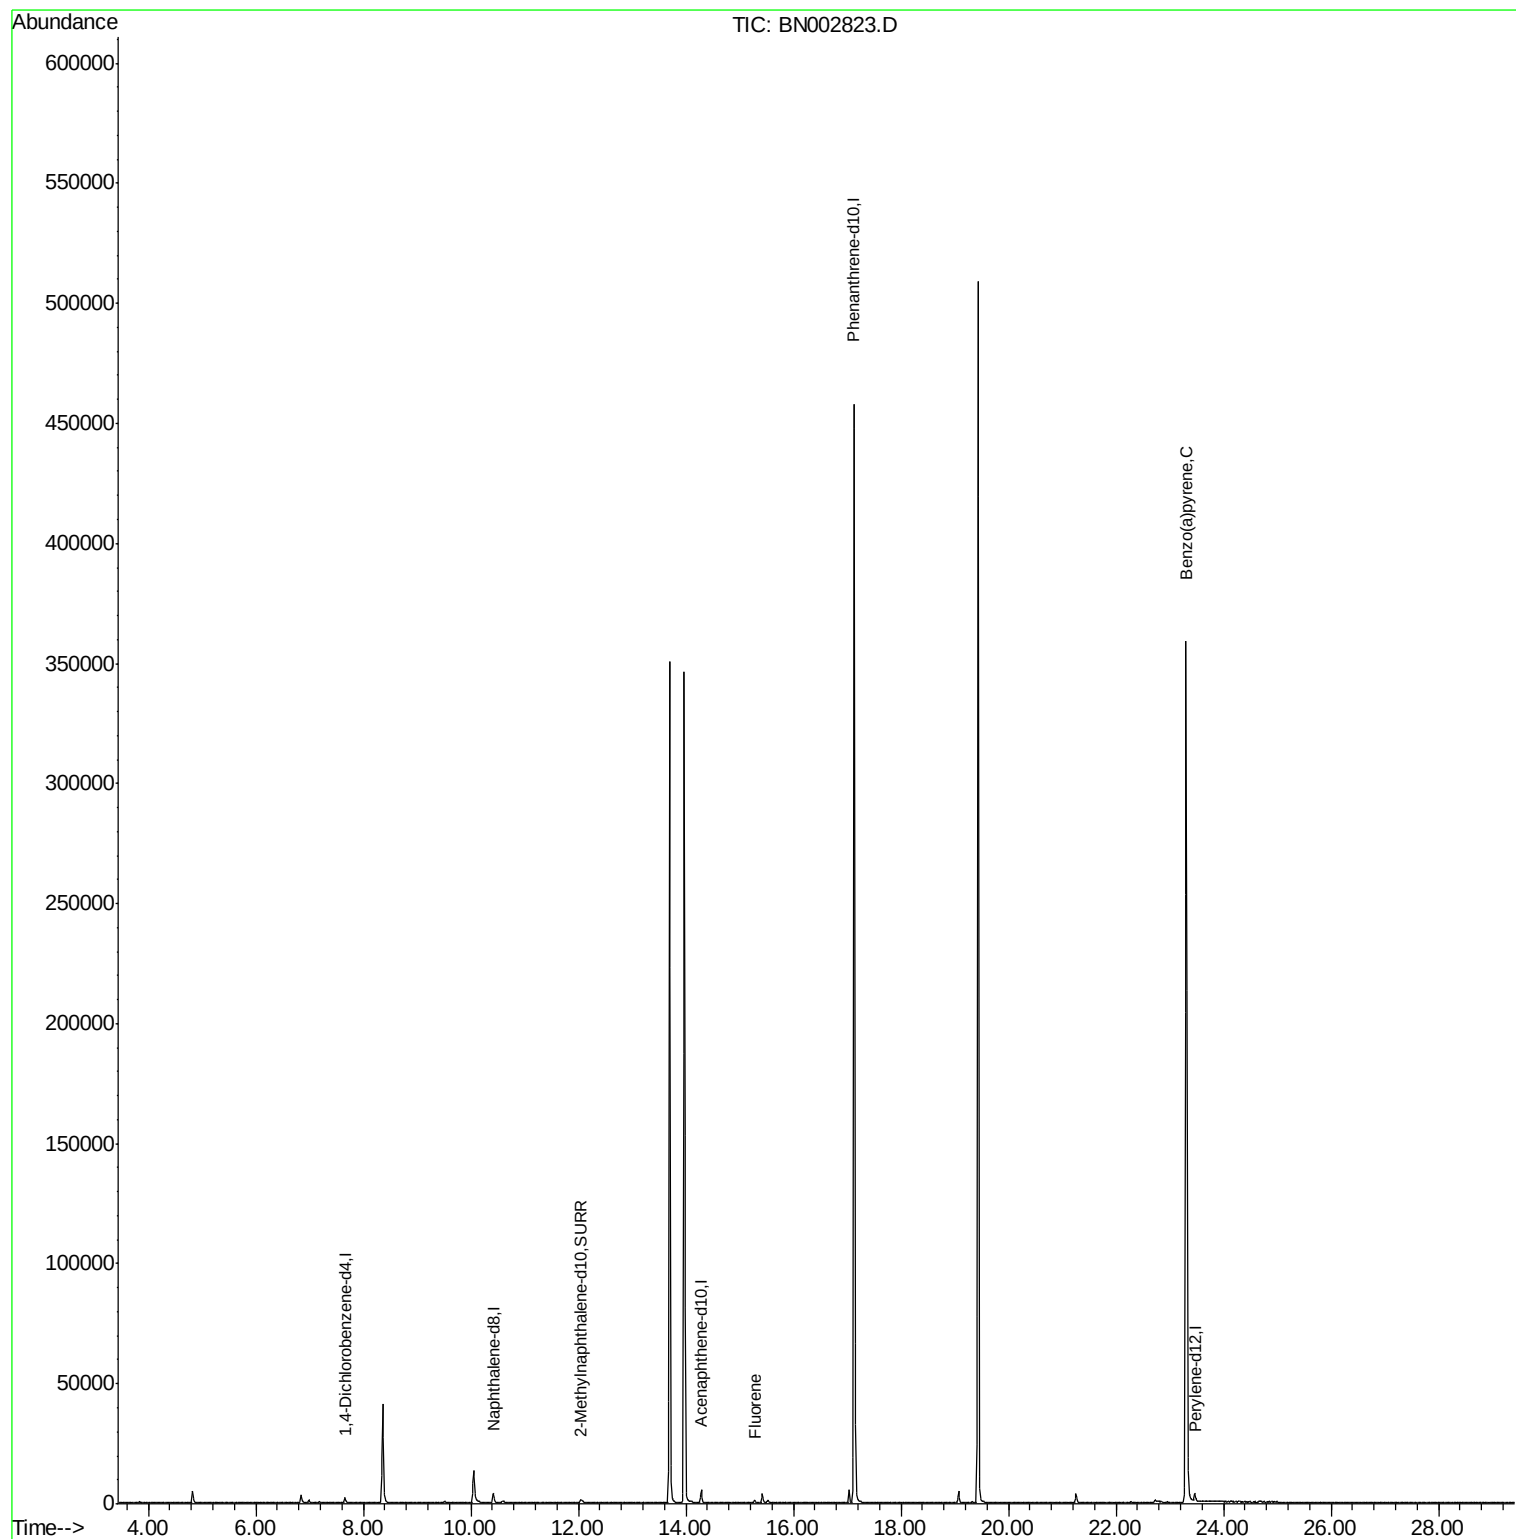


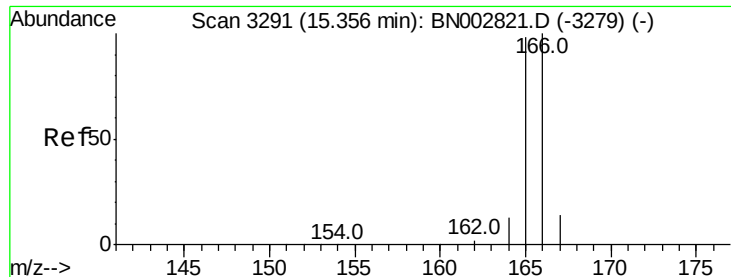

#9
Fluorene
Concen: 0.076 ng/ul
RT: 15.28 min Scan# 3274
Delta R.T. -0.08 min
Lab File: BN002823.D
Acq: 21 Sep 2018 18:09

Instrument :
BNA_N
ClientSampleId :

Tot Ion:166 Resp: 869
Ion Ratio Lower Upper
166 100
165 10.9 73.4 110.2#
167 34.5 14.6 22.0#

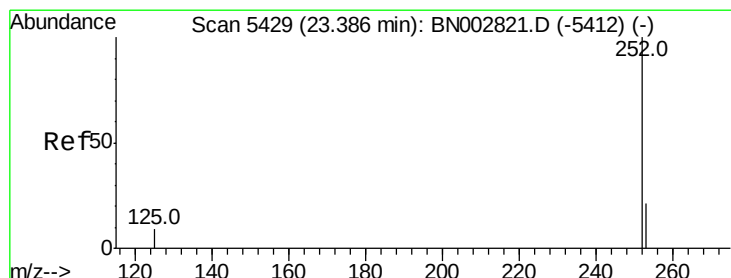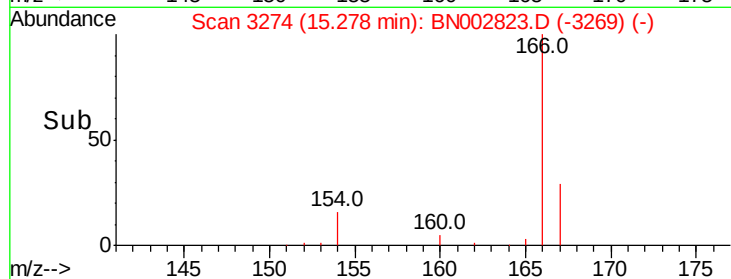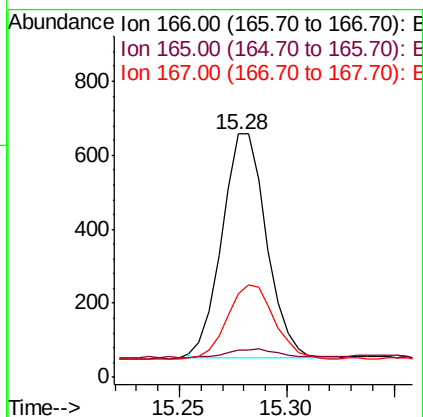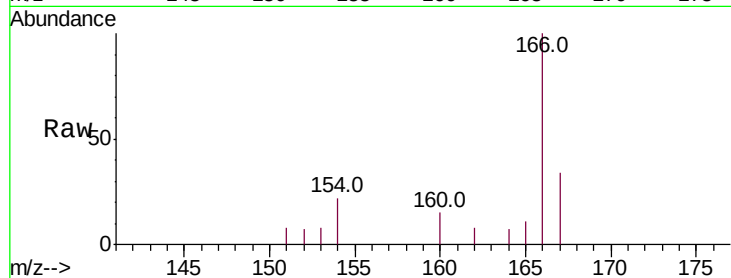

#23
Benzo(a)pyrene
Concen: 0.095 ng/ul
RT: 23.31 min Scan# 5403
Delta R.T. -0.08 min
Lab File: BN002823.D
Acq: 21 Sep 2018 18:09

Tgt Ion:252 Resp: 1707
Ion Ratio Lower Upper
252 100
253 39.8 16.0 24.0#
125 31.5 12.0 18.0#

