

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 21 23:49:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	1558	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	6209	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	3312	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	541595	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.25
20) Perylene-d12	23.46	264	6327	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	3406	0.38	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.31	252	2016	0.101	ng/ul#	Ovalue 53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
Data File : BN002826.D
Acq On : 21 Sep 2018 19:54
Operator : JU/SJ
Sample : J4874-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 21 23:49:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 23:48:47 2018
Response via : Initial Calibration

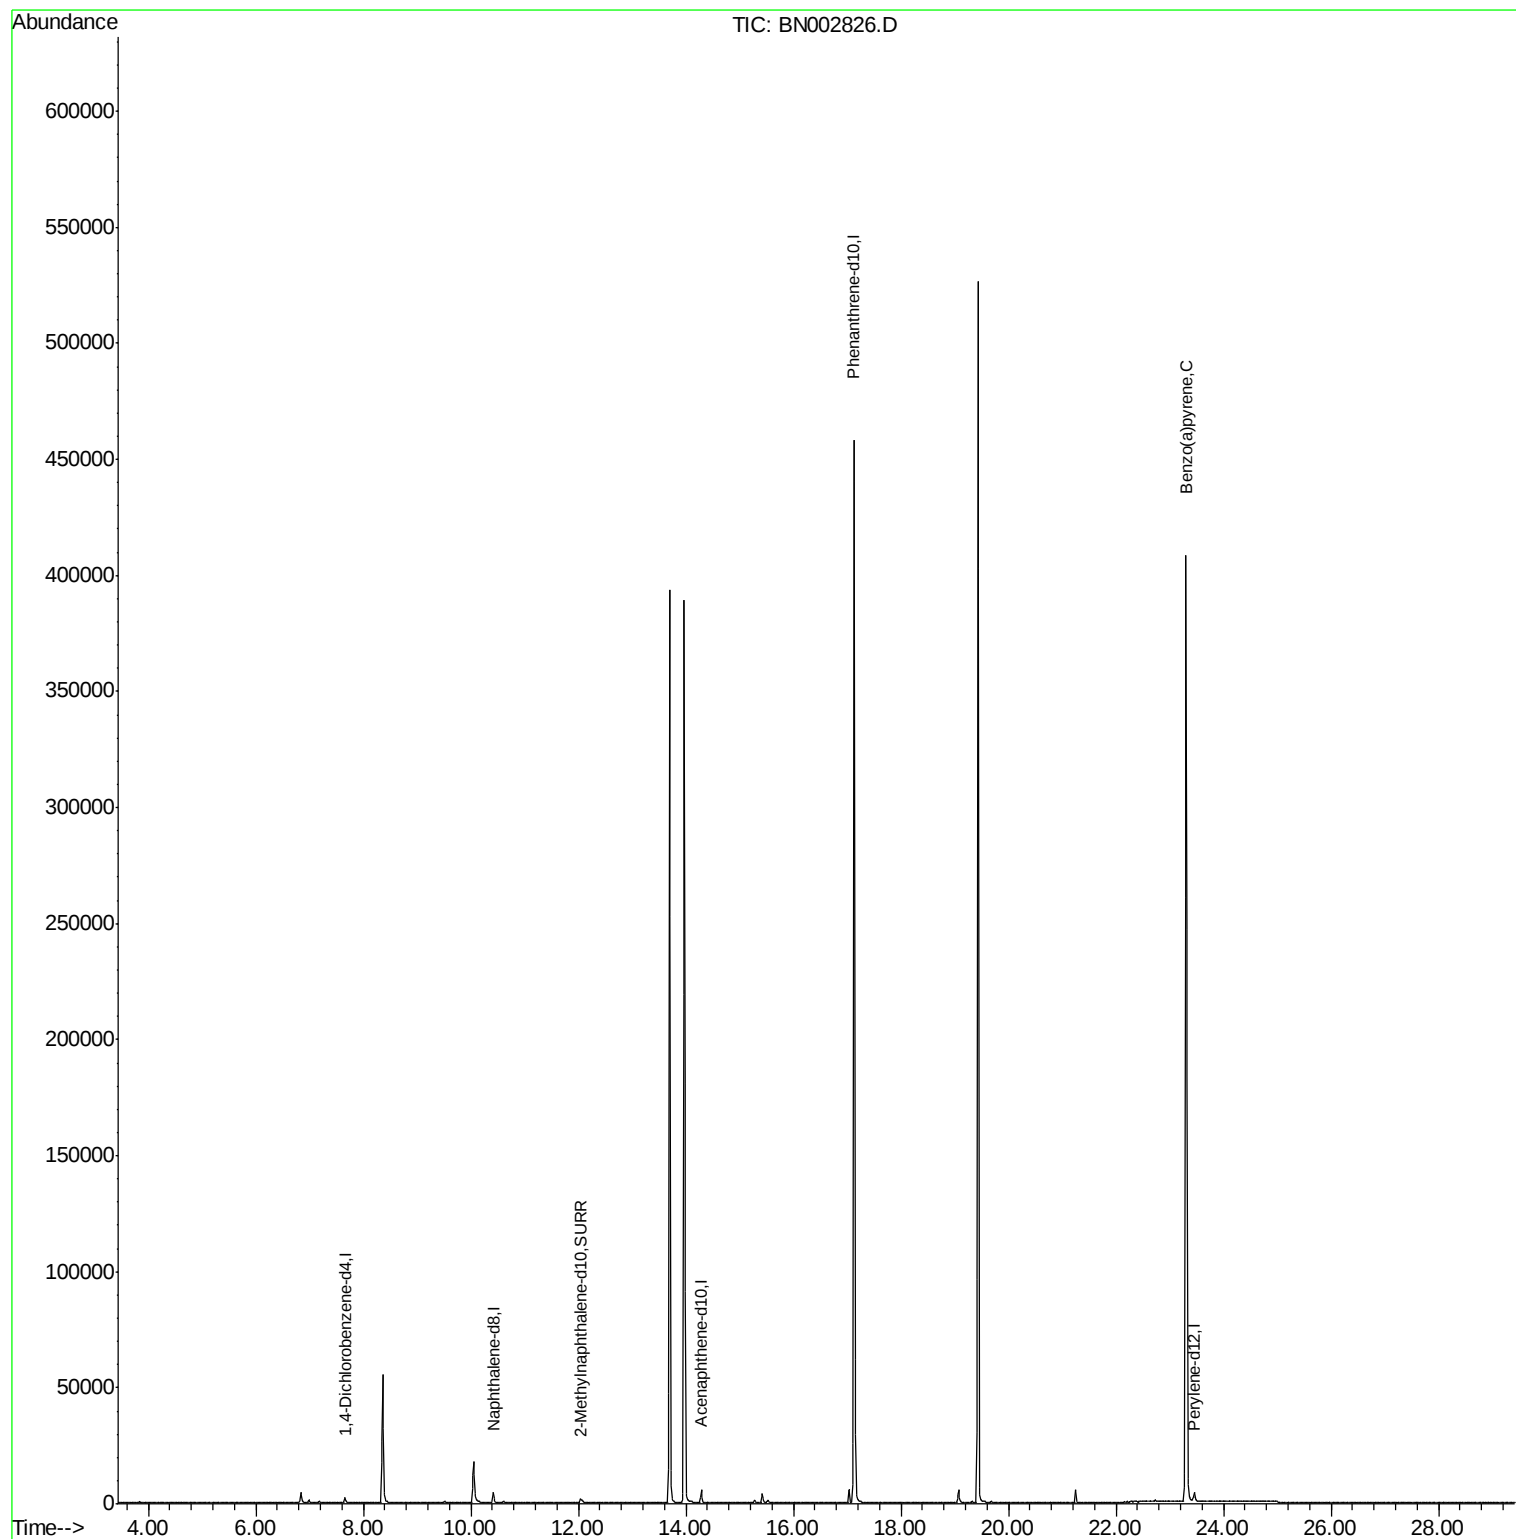

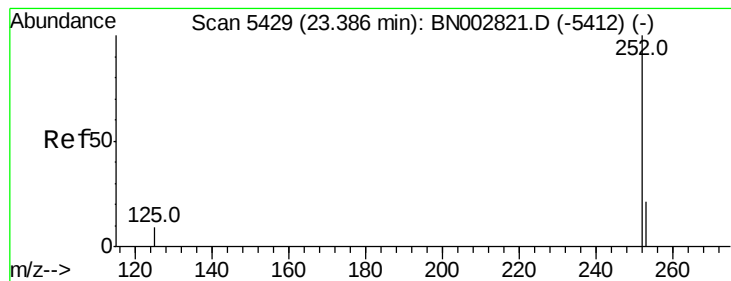

#23

Benzo(a)pyrene

Concen: 0.101 ng/ul

RT: 23.31 min Scan# 5402

Delta R.T. -0.08 min


Lab File: BN002826.D

Acq: 21 Sep 2018 19:54

Instrument :

BNA_N

ClientSampleId :

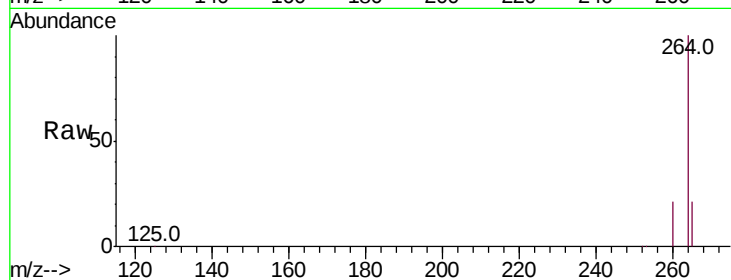


Tot Ion: 252 Resp: 2016

Ion Ratio Lower Upper

252 100

253 43.2 16.0 24.0#

125 32.4 12.0 18.0#

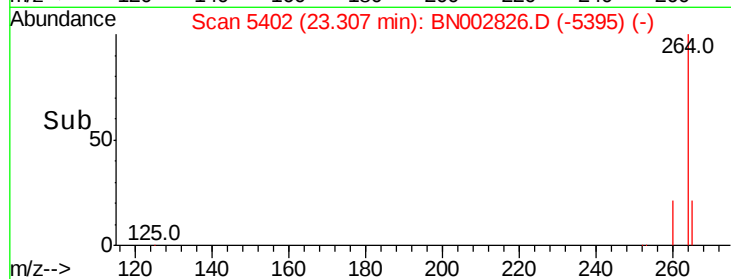

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

