

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:05:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

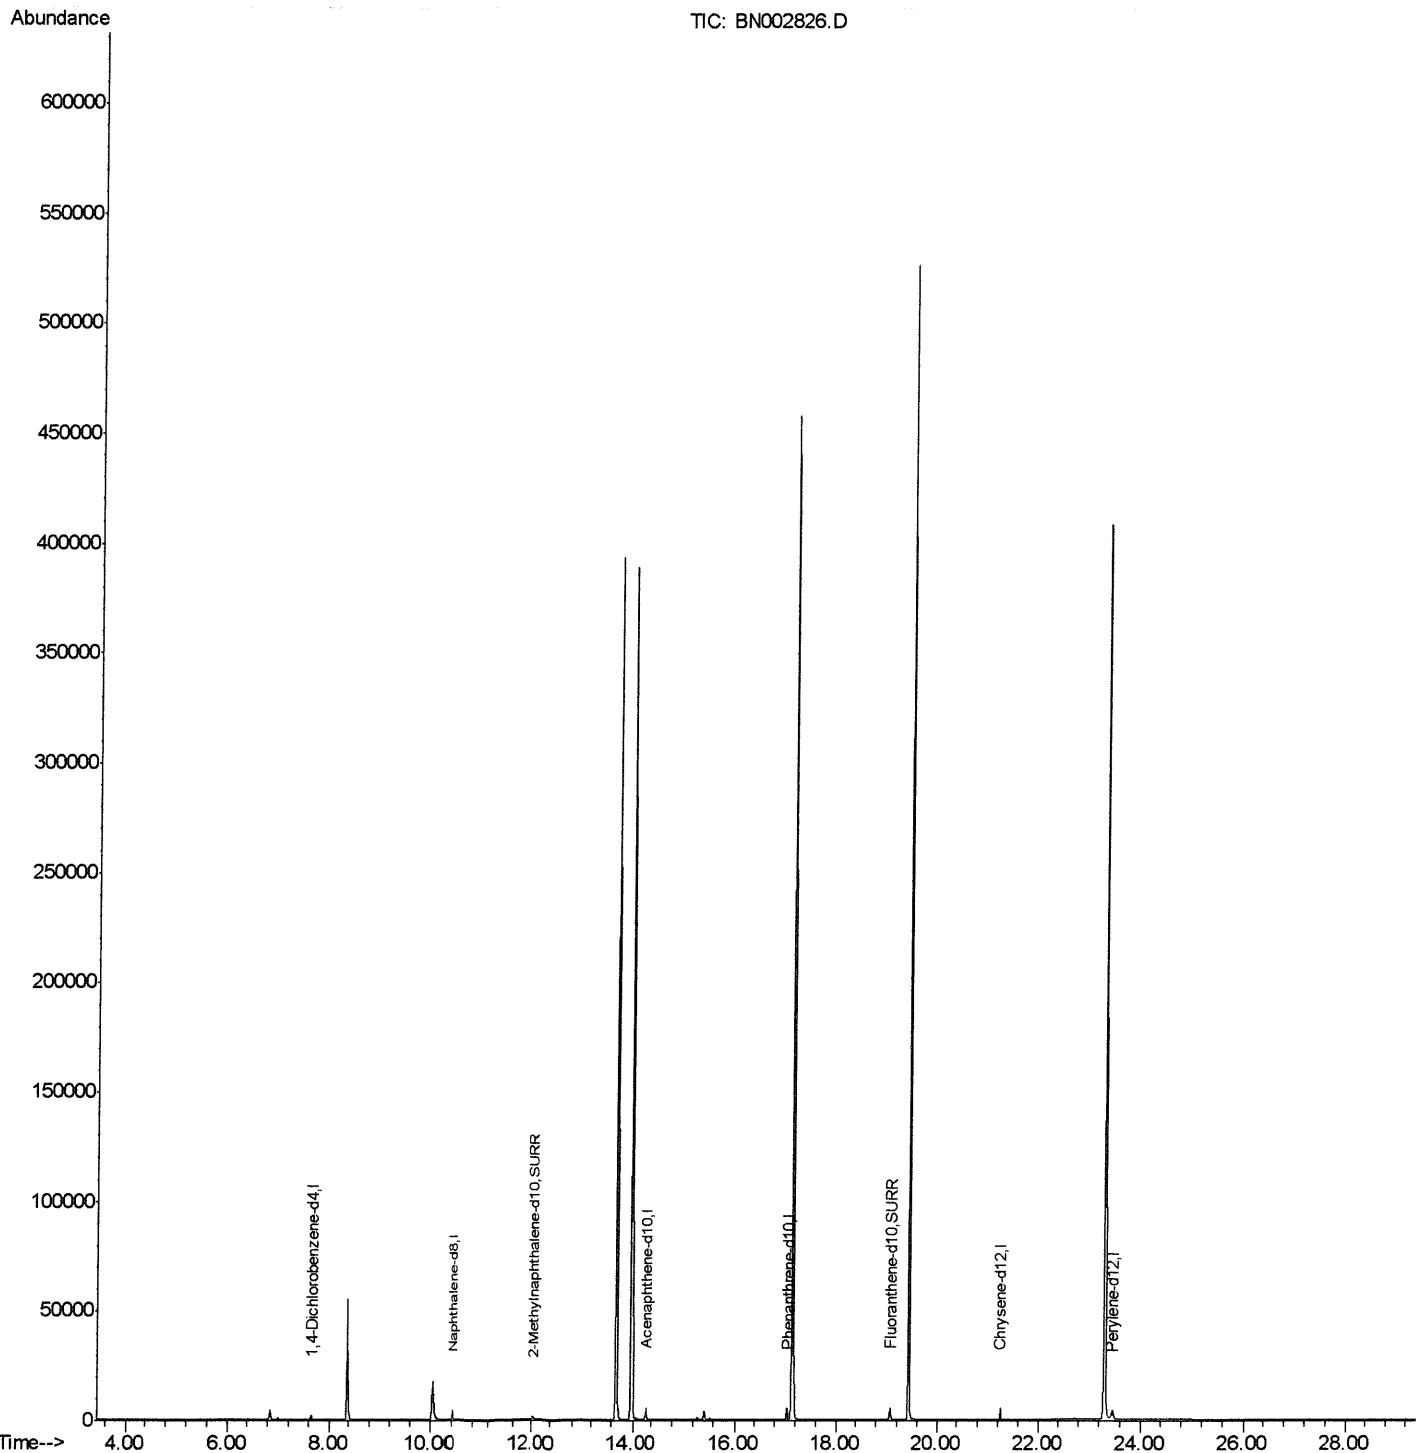

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 21 23:49:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

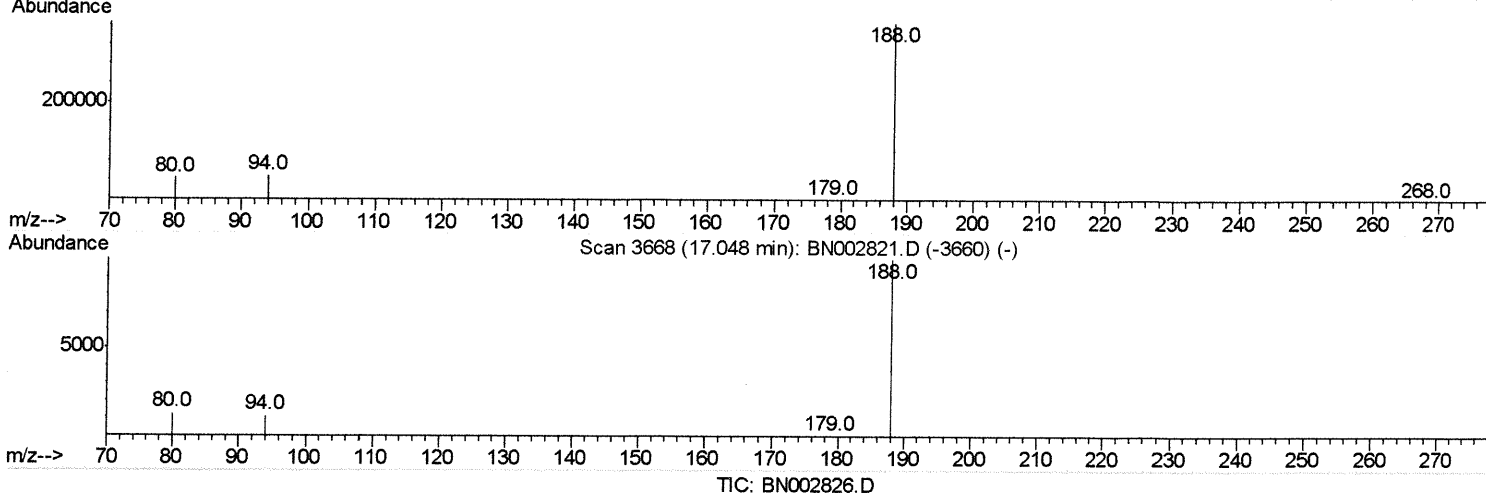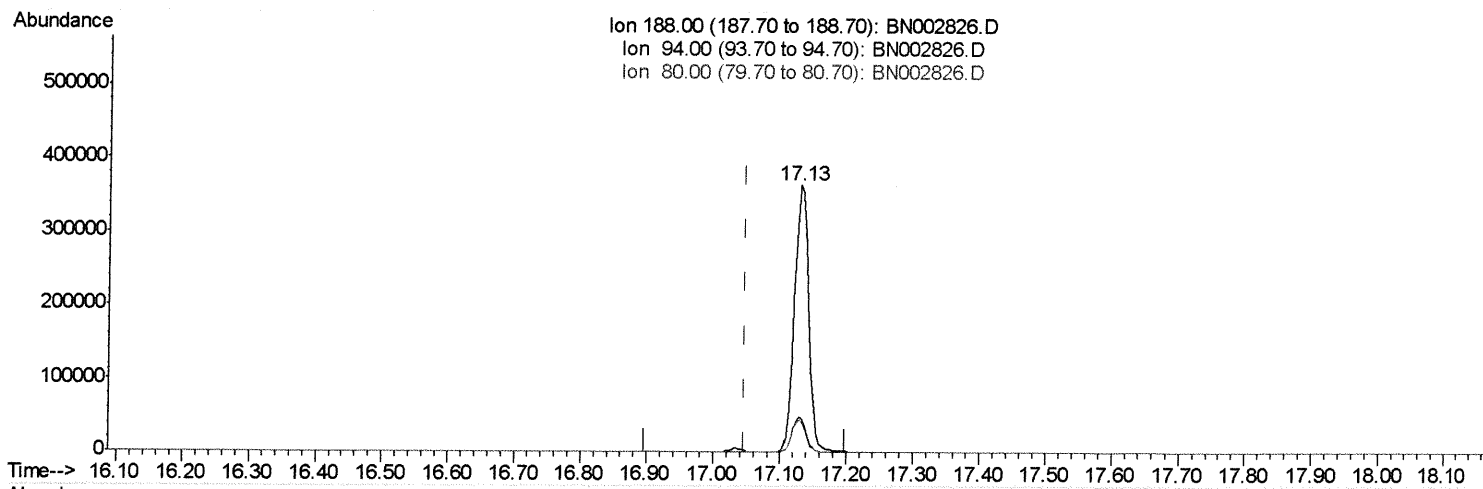

(10) Phenanthrene-d10 (I)
 17.128min (+0.080) 0.40ng/ul
 response 541595

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.34#
80.00	11.80	12.26
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 21 23:49:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

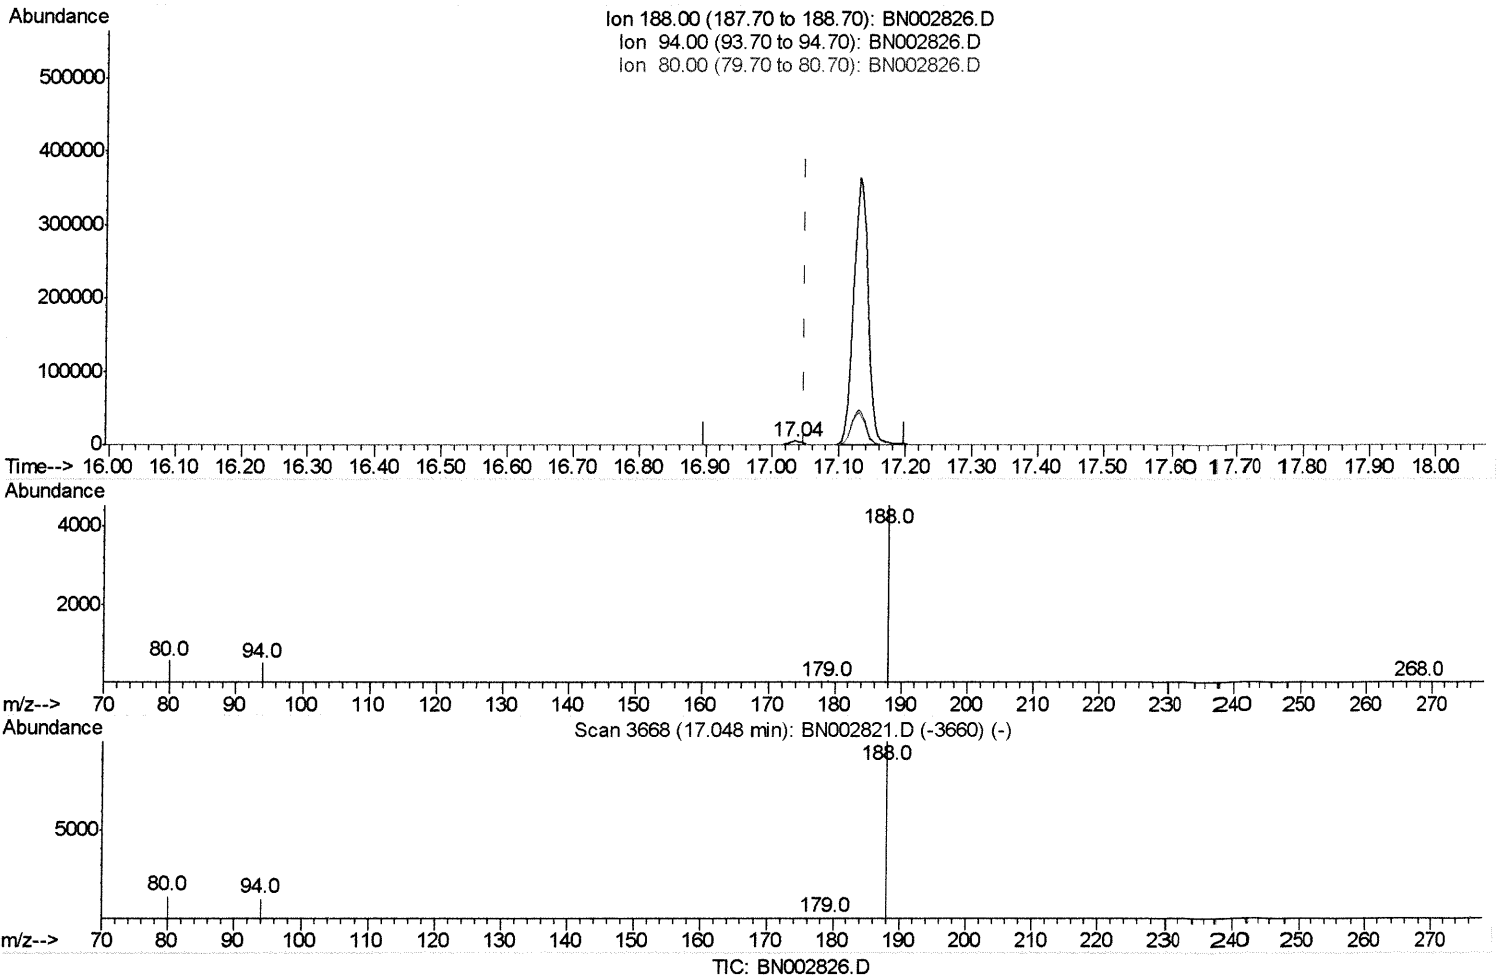

(10) Phenanthrene-d10 (I)

17.036min (-0.012) 0.40ng/ul m

SJ 9/24/18

response 6683

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.53
80.00	11.80	12.98
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:03:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

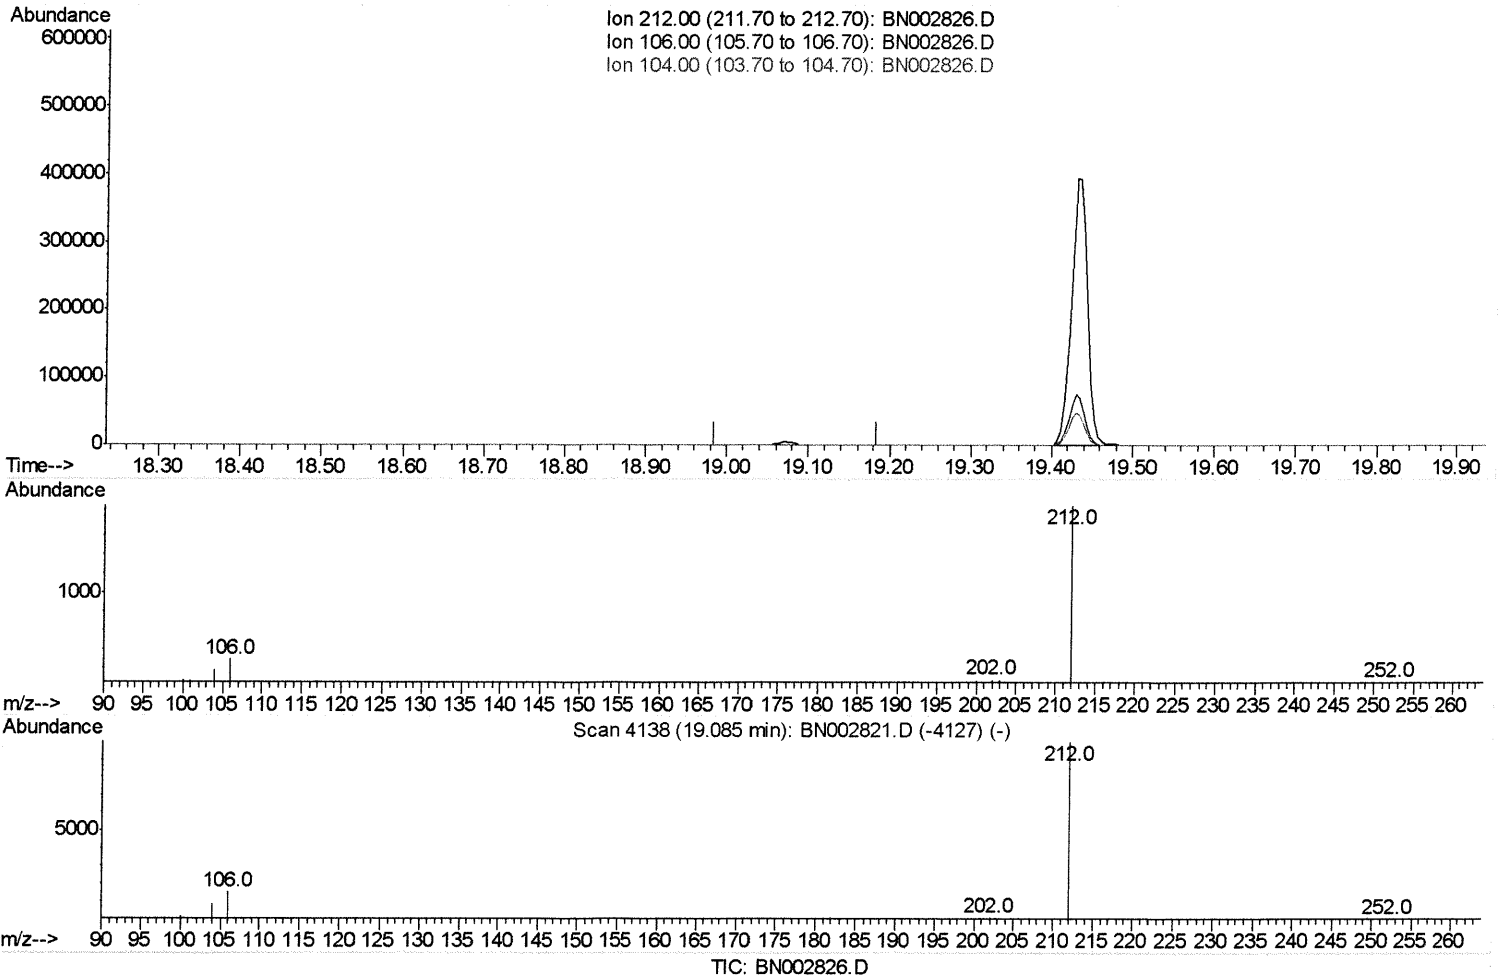

(14) Fluoranthene-d10 (SURR)

19.085min (-19.085) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:03:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

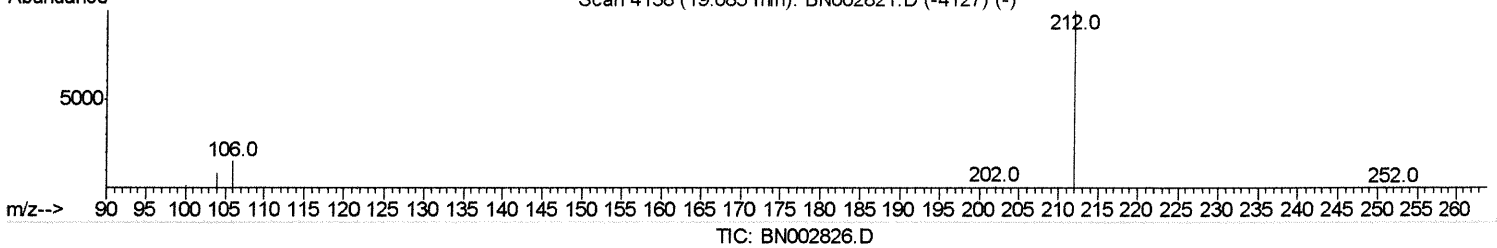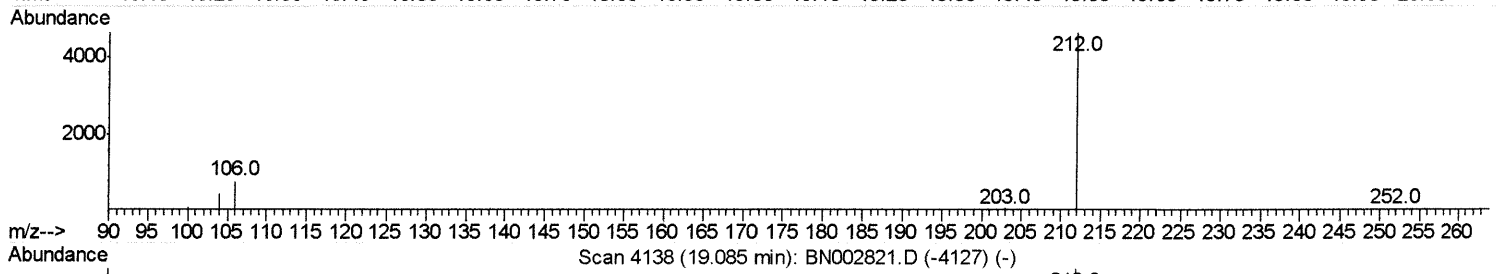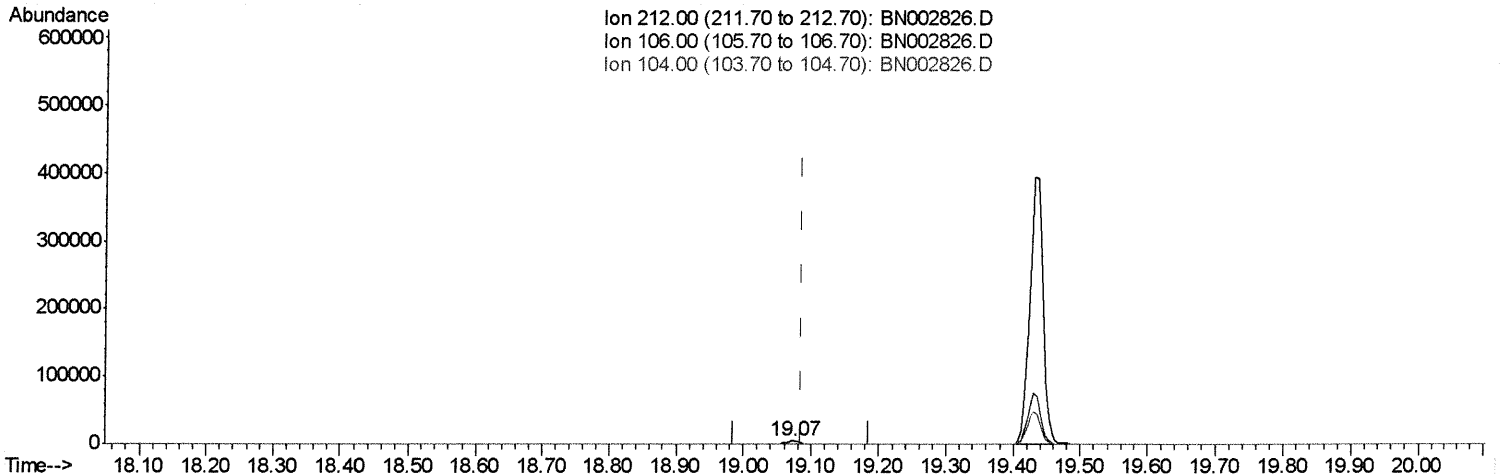

(14) Fluoranthene-d10 (SURR)

19.072min (-0.014) 0.38ng/ul m

SS 9/24/18

response 6629

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:03:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

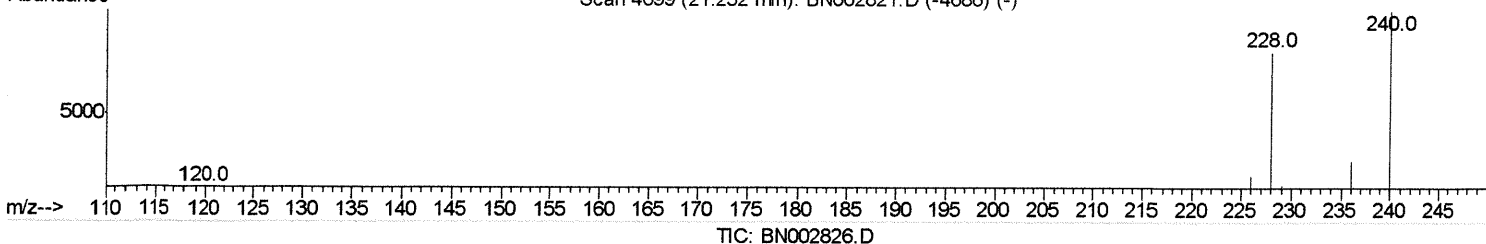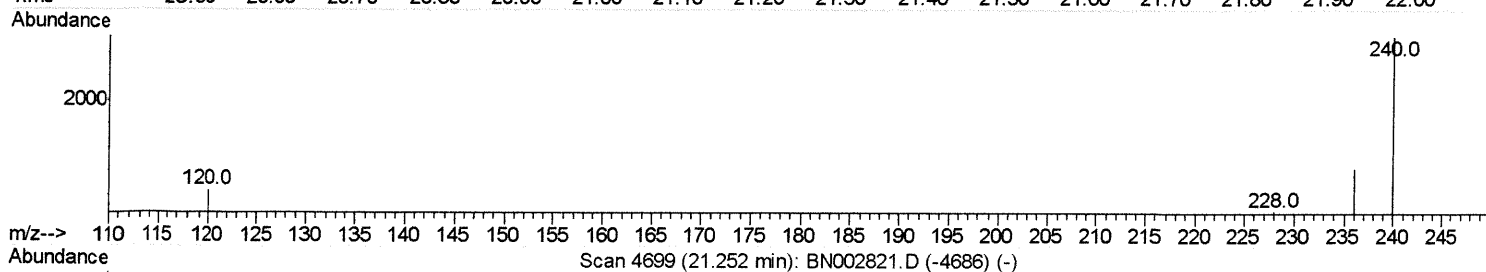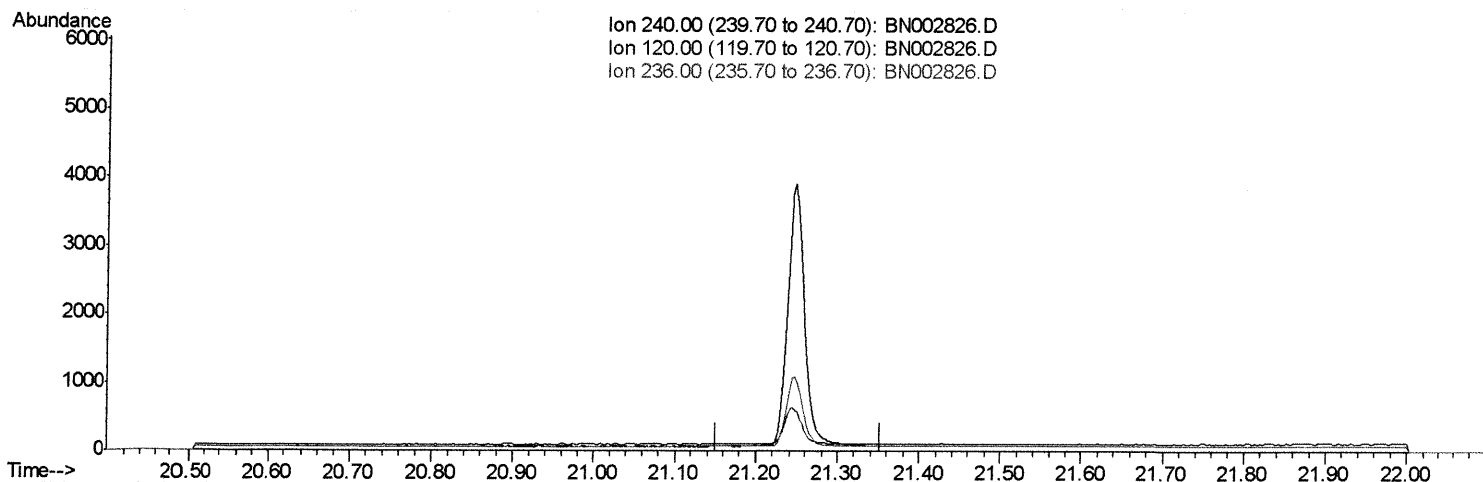

(16) Chrysene-d12 (I)

21.252min (-21.252) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:03:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

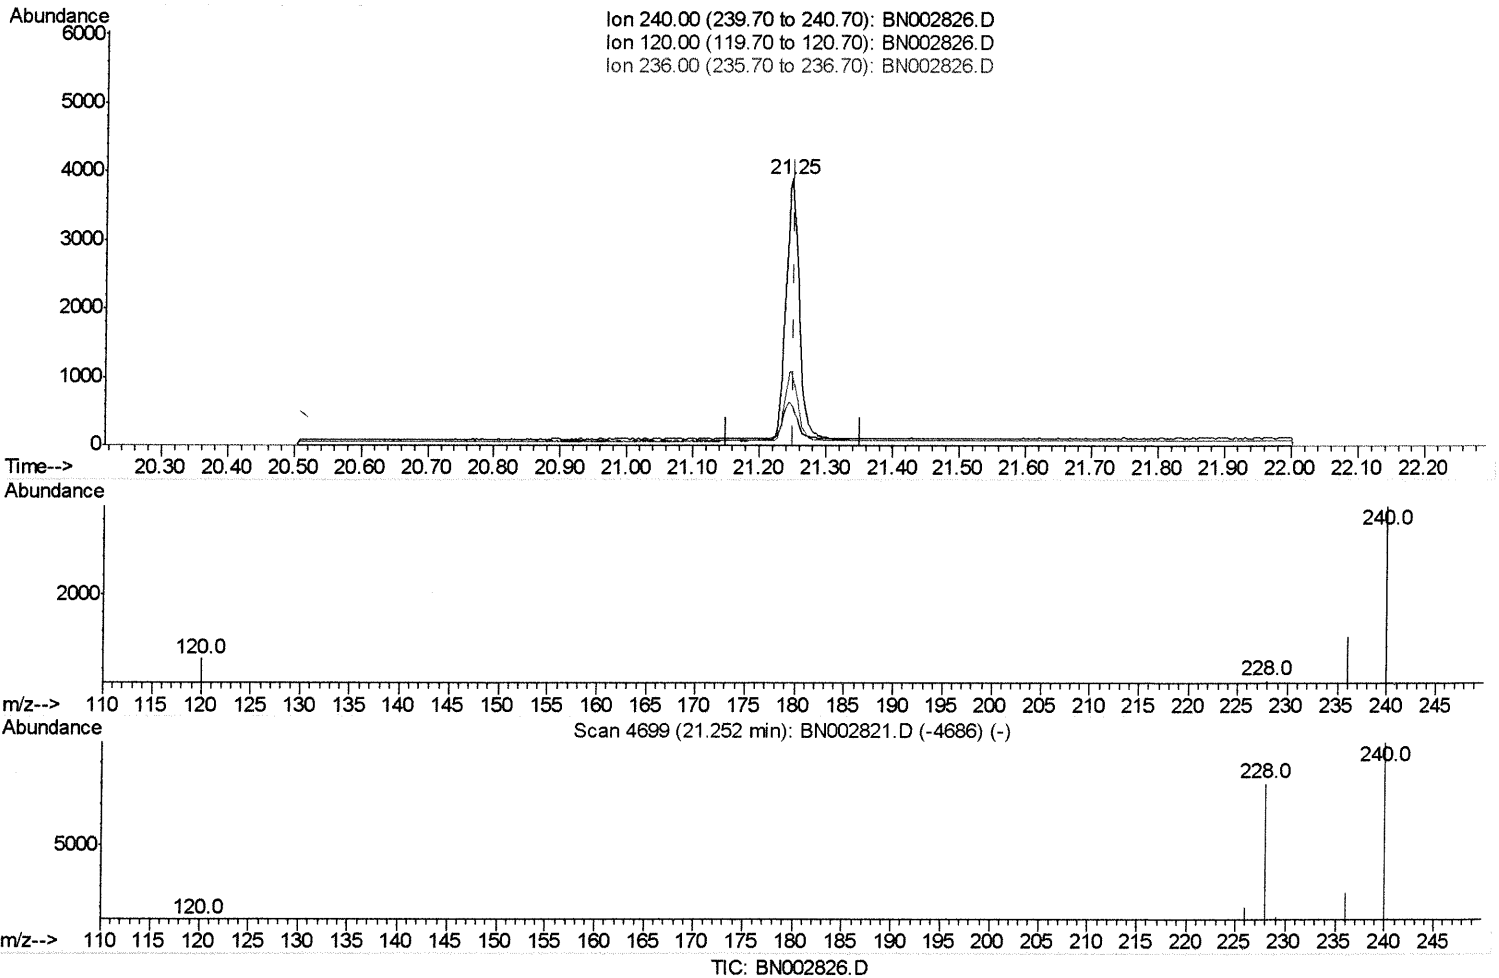

(16) Chrysene-d12 (I)

21.247min (-0.006) 0.40ng/ul m

519/24/18

response 5313

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	15.62#
236.00	34.90	27.78#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
Data File : BN002826.D
Acq On : 21 Sep 2018 19:54
Operator : JU/SJ
Sample : J4874-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A3ZC1

Manual Integrations
APPROVED

Sohil
9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:04:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 23:48:47 2018
Response via : Initial Calibration

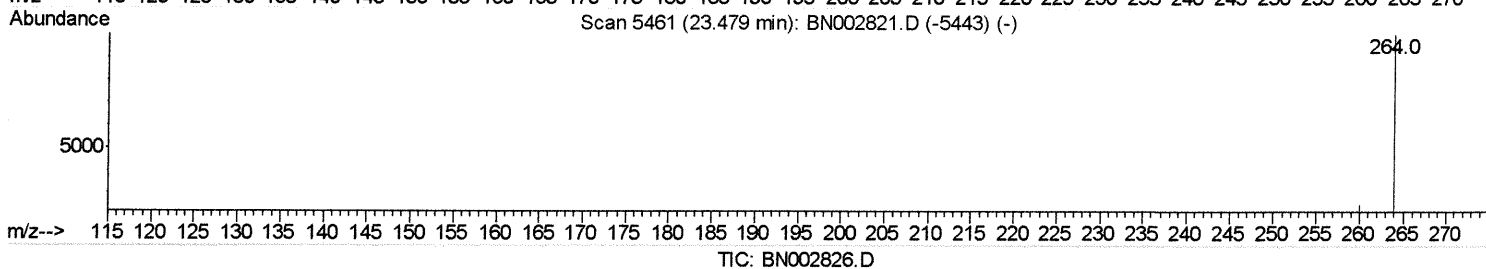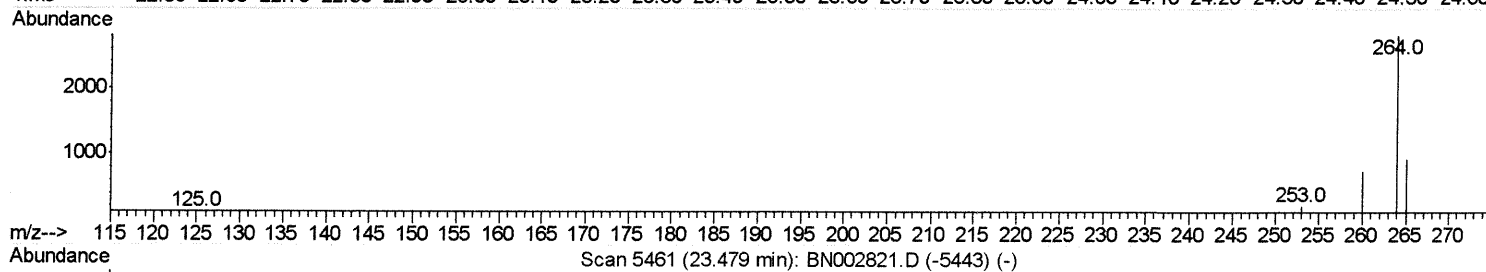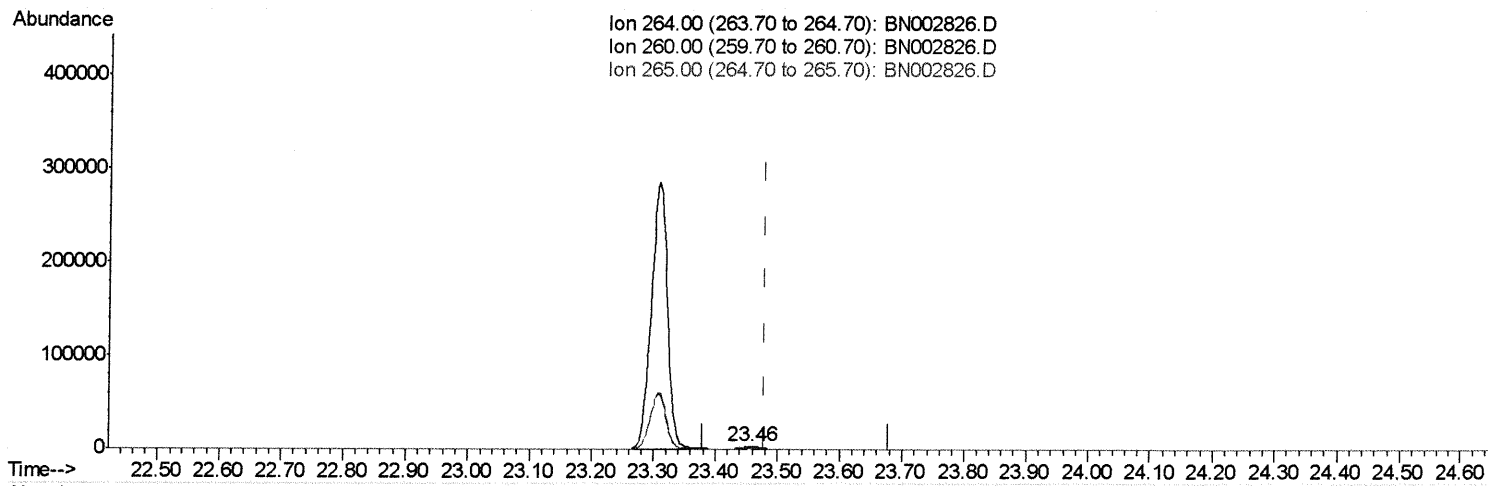

(20) Perylene-d12 (I)

23.456min (-0.023) 0.40ng/ul

response 6327

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.69
265.00	103.50	32.76#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:04:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

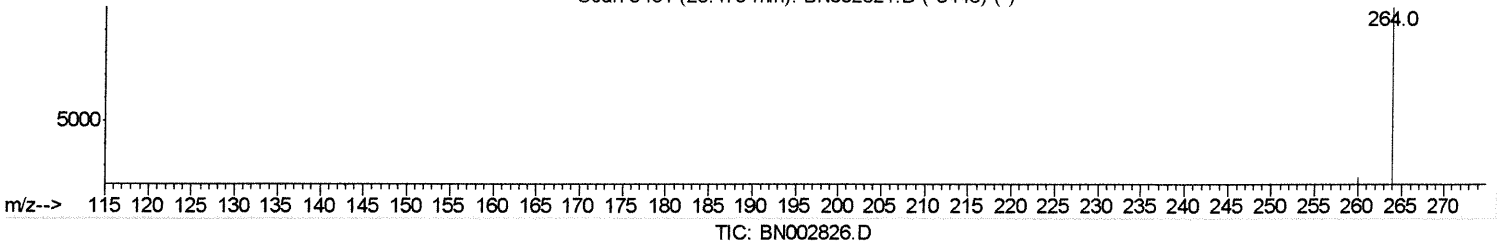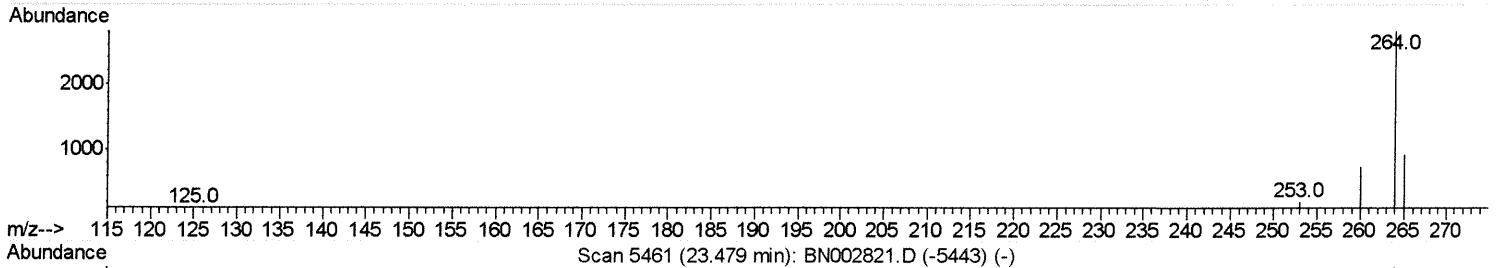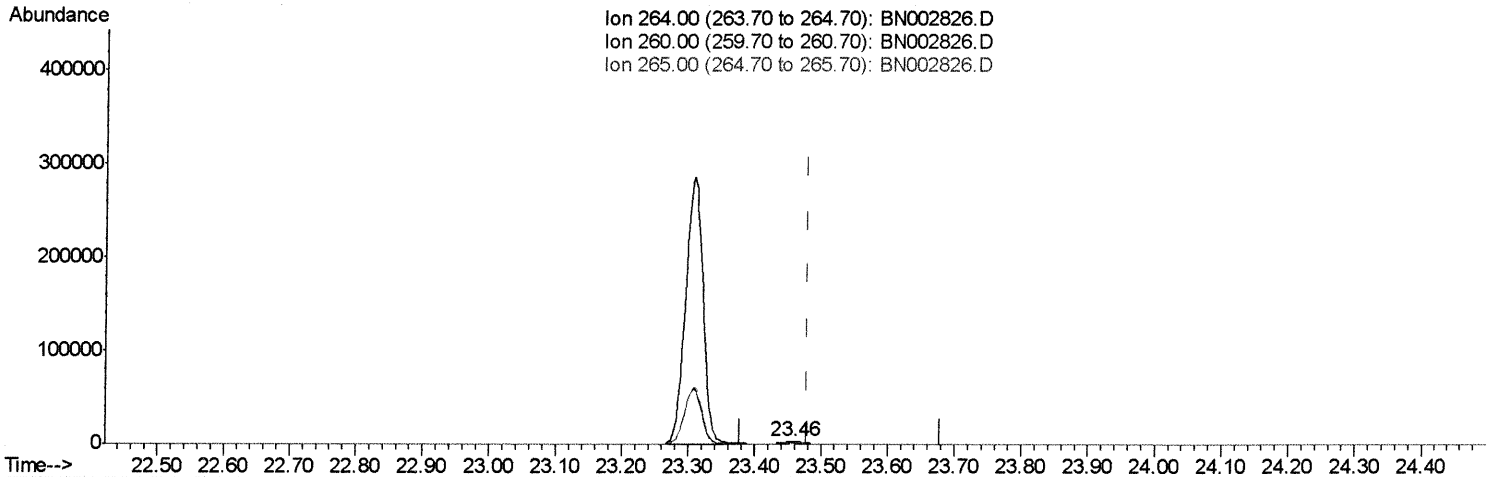

(20) Perylene-d12 (I)

23.456min (-0.023) 0.40ng/ul m

SJ 9/24/18

response 4757

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.69
265.00	103.50	32.76#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092218\
 Data File : BN002826.D
 Acq On : 21 Sep 2018 19:54
 Operator : JU/SJ
 Sample : J4874-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZC1

Manual Integrations
 APPROVED

Sohil
 9/24/2018 5:31:48 PM

Quant Time: Sep 22 00:05:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 23:48:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	1558	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	6209	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	3312	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	6683m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.25	240	5313m	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	4757m	0.40	ng/ul	-0.02

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.04	152	3406	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	6629m	0.38	ng/ul	-0.01

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SS 9/24/18
SS 9/24/18