

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
 Data File : BN027786.D
 Acq On : 21 Sep 2023 14:34
 Operator : MA/JU
 Sample : PB155450BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK450

Quant Time: Sep 22 03:59:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.008	152	4828	0.400	ng/ul	0.00
4) Naphthalene-d8	10.828	136	15746	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	9199	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	20062	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	16414	0.400	ng/ul	0.00
23) Perylene-d12	24.065	264	19039	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	35192	5.787	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.407	152	6934	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	16410	0.327	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.633	166	2581	0.063	ng/ul#	15
20) Pyrene	19.780	202	2728	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.904	252	6054	0.089	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
Data File : BN027786.D
Acq On : 21 Sep 2023 14:34
Operator : MA/JU
Sample : PB155450BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK450

Quant Time: Sep 22 03:59:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration




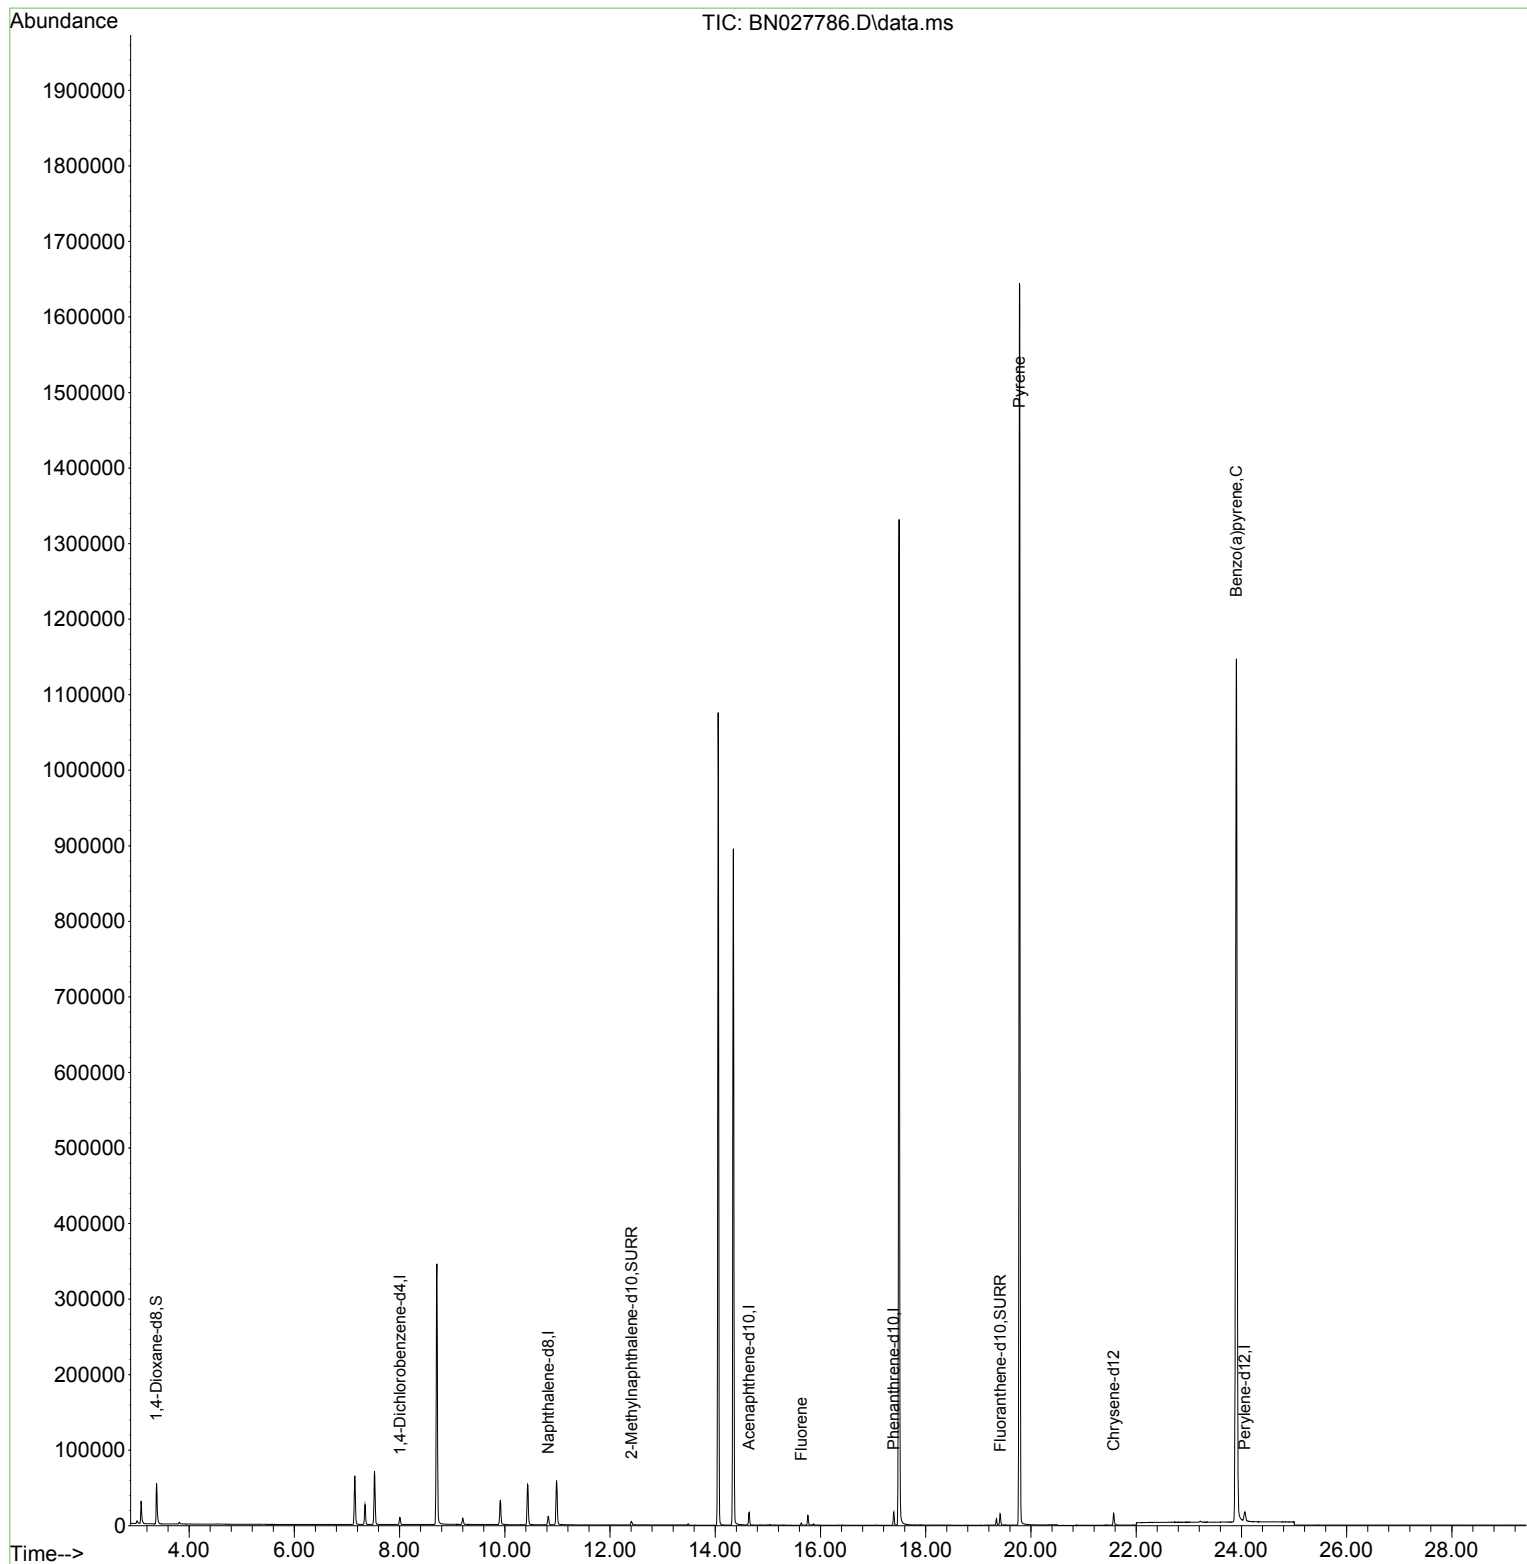


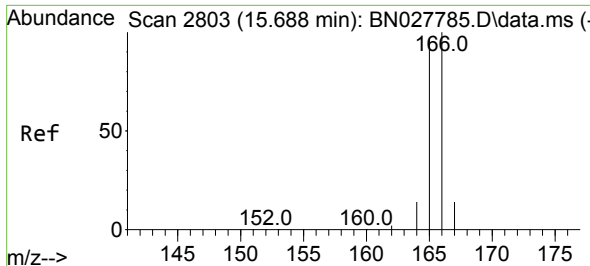

#12
 Fluorene
 Concen: 0.063 ng/ul
 RT: 15.633 min Scan# 21
 Delta R.T. -0.055 min
 Lab File: BN027786.D
 Acq: 21 Sep 2023 14:34




Instrument :
 BNA_N
 ClientSampleId :
 SBLK450


Tgt Ion:166 Resp: 2581
 Ion Ratio Lower Upper
 166 100
 165 8.4 78.0 117.0#
 167 33.7 11.4 17.2#

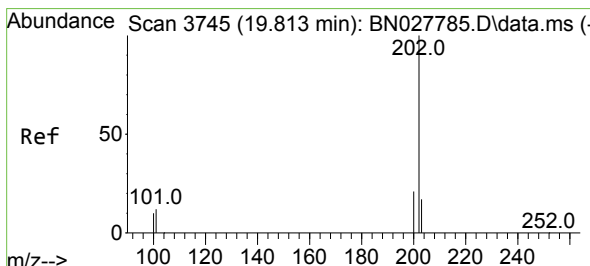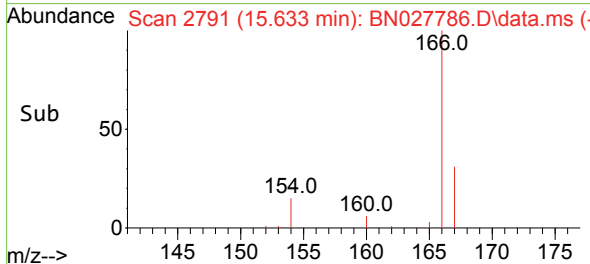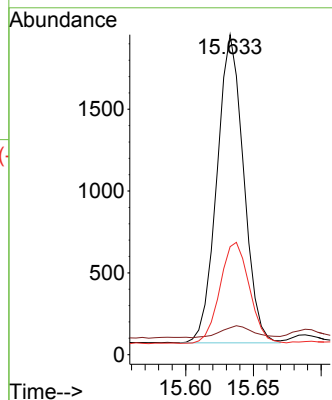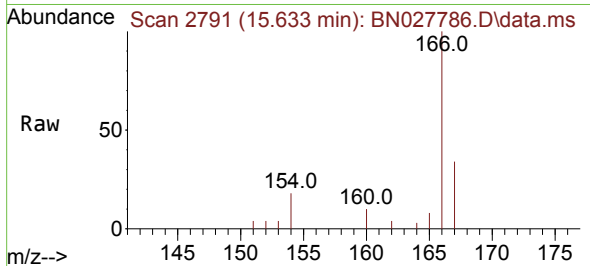

#20
 Pyrene
 Concen: 0.040 ng/ul
 RT: 19.780 min Scan# 3738
 Delta R.T. -0.032 min
 Lab File: BN027786.D
 Acq: 21 Sep 2023 14:34

Tgt Ion:202 Resp: 2728
 Ion Ratio Lower Upper
 202 100
 101 170.1 11.4 17.0#
 100 1317.7 9.1 13.7#

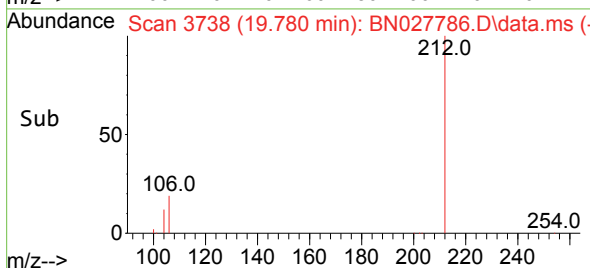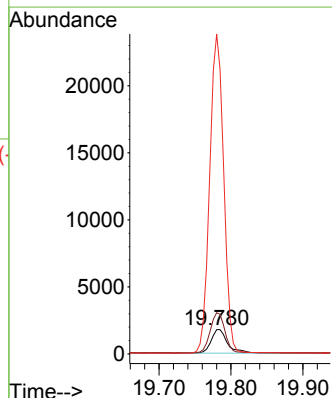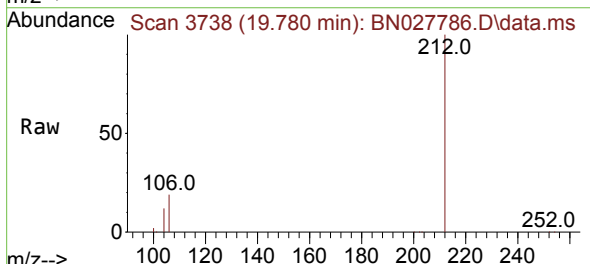

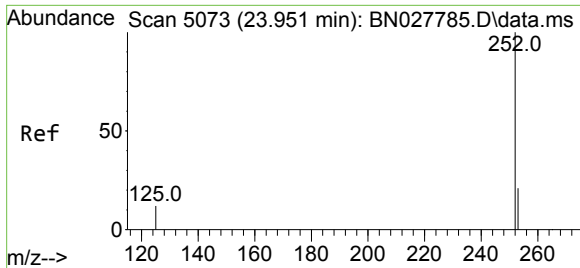

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.904 min Scan# 50
Delta R.T. -0.047 min
Lab File: BN027786.D
Acq: 21 Sep 2023 14:34

Instrument :
BNA_N
ClientSampleId :
SBLK450

Tgt Ion:252 Resp: 6054
Ion Ratio Lower Upper
252 100
253 45.9 21.9 32.9#
125 40.6 15.5 23.3#

