

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
 Data File : BN027801.D
 Acq On : 22 Sep 2023 00:20
 Operator : MA/JU
 Sample : PB155580BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK580

Quant Time: Sep 22 04:03:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	5249	0.400	ng/ul	0.00
4) Naphthalene-d8	10.823	136	18060	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	11219	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.388	188	24115	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	20687	0.400	ng/ul	0.00
23) Perylene-d12	24.062	264	20272	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	34660	5.242	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.407	152	7921	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	20169	0.319	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.633	166	2802	0.056	ng/ul#	16
20) Pyrene	19.780	202	2947	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.898	252	5378	0.074	ng/ul#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
Data File : BN027801.D
Acq On : 22 Sep 2023 00:20
Operator : MA/JU
Sample : PB155580BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Quant Time: Sep 22 04:03:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration

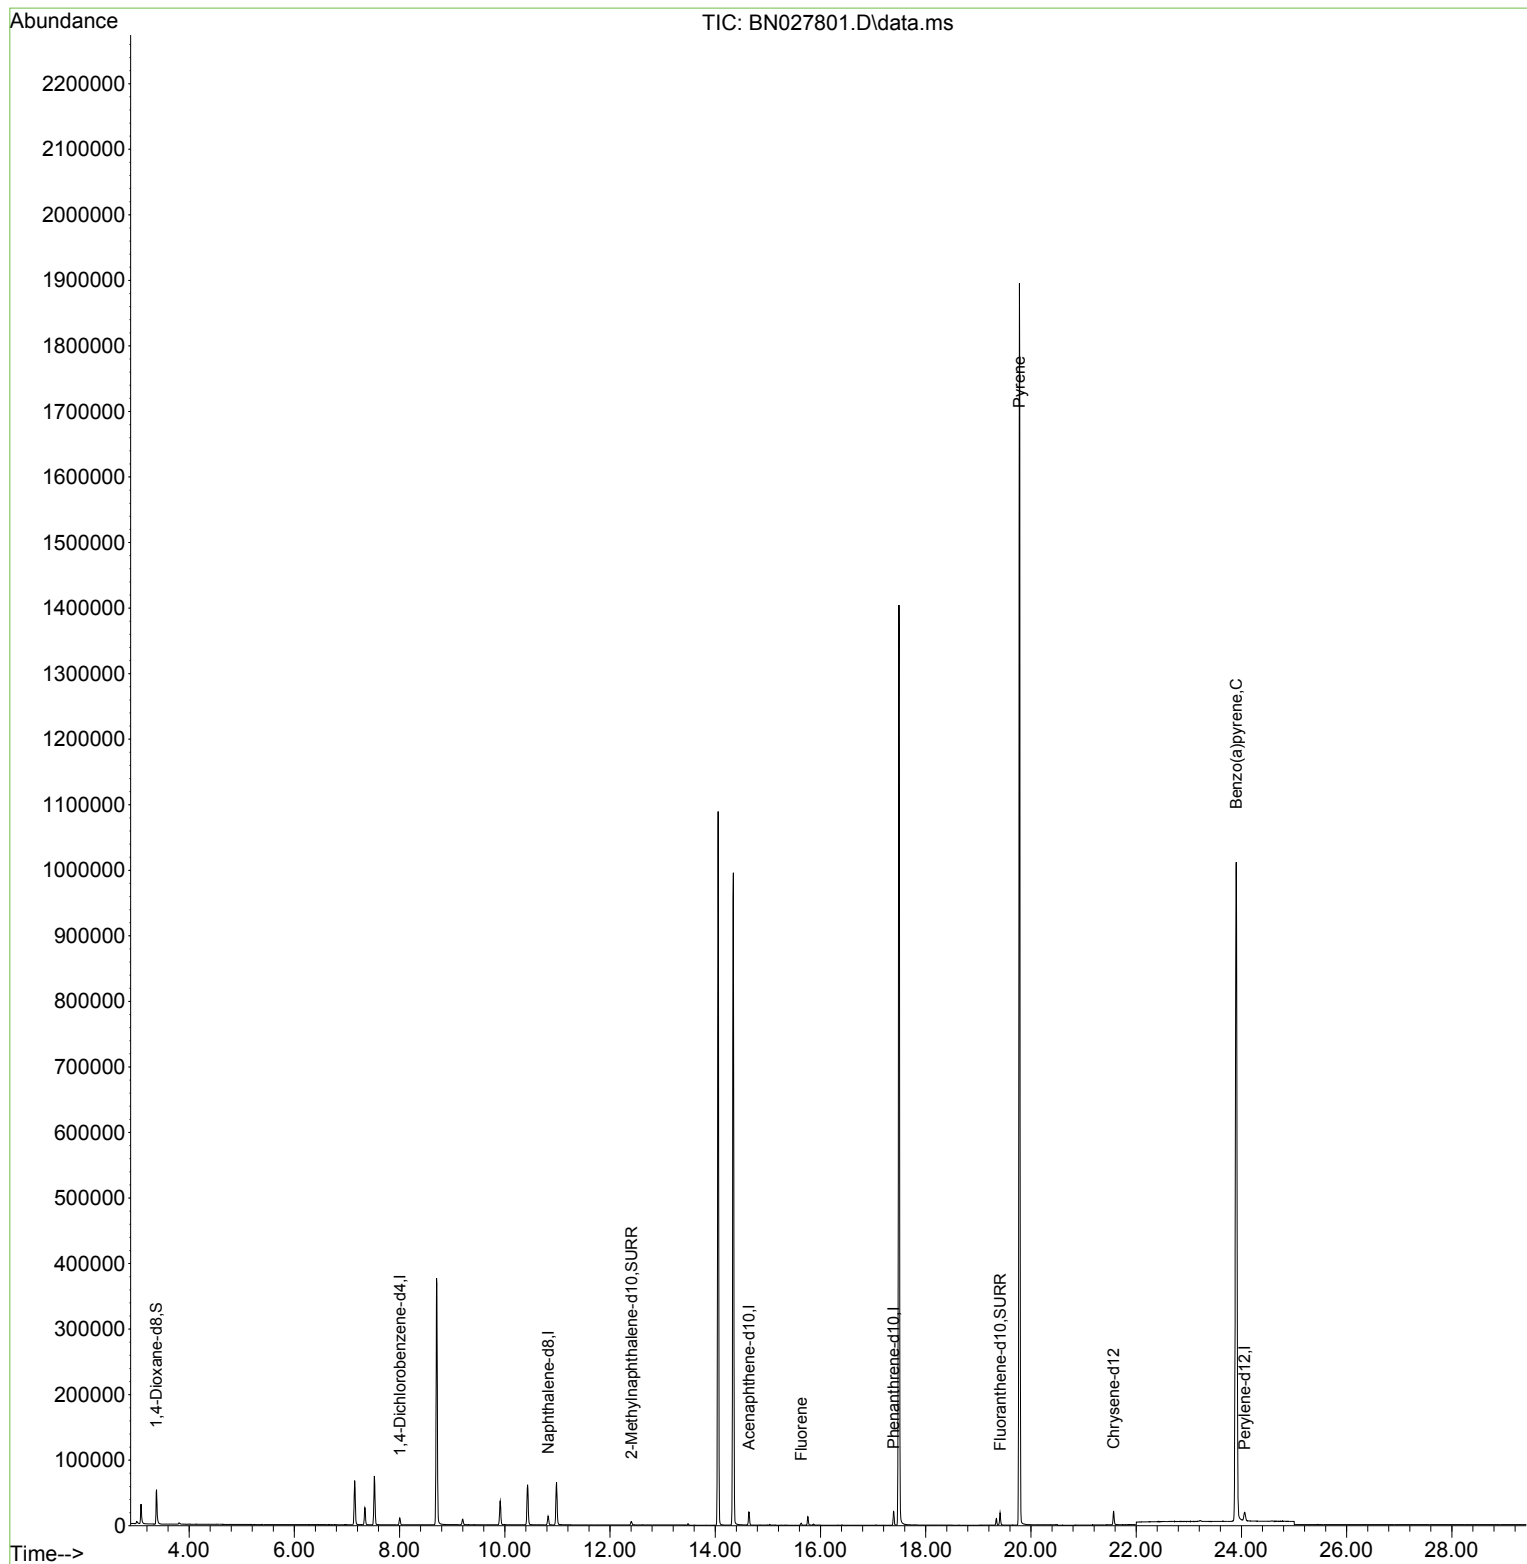




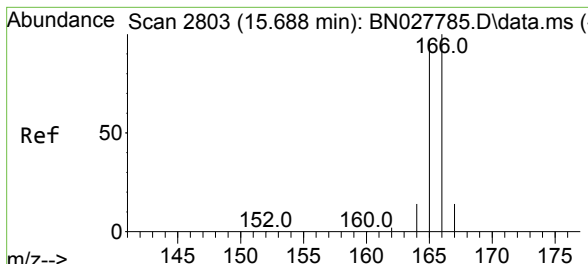


#12
 Fluorene
 Concen: 0.056 ng/ul
 RT: 15.633 min Scan# 21
 Delta R.T. -0.055 min
 Lab File: BN027801.D
 Acq: 22 Sep 2023 00:20

Instrument :
 BNA_N
 ClientSampleId :
 SBLK580

Tgt Ion:166 Resp: 2802




Ion	Ratio	Lower	Upper
166	100		
165	9.9	78.0	117.0#
167	36.2	11.4	17.2#

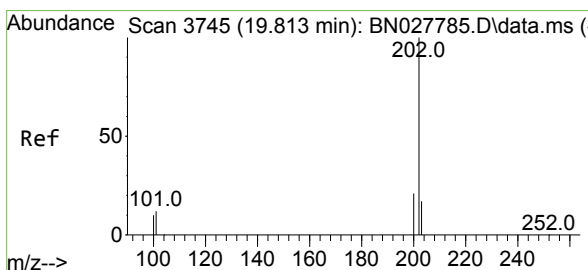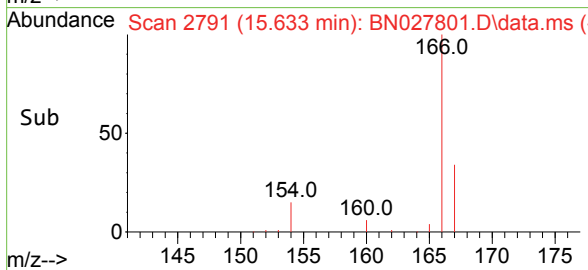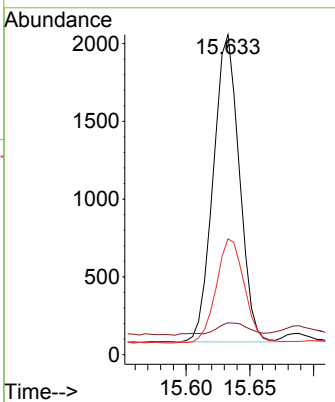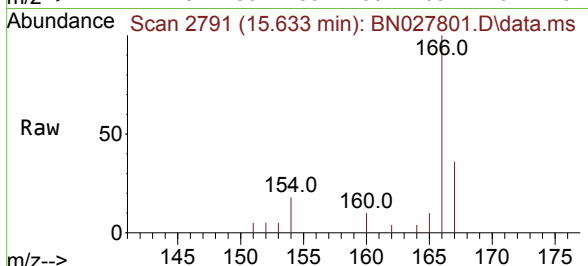


#20
 Pyrene
 Concen: 0.034 ng/ul
 RT: 19.780 min Scan# 3738
 Delta R.T. -0.032 min
 Lab File: BN027801.D
 Acq: 22 Sep 2023 00:20

Tgt Ion:202 Resp: 2947


Ion	Ratio	Lower	Upper
202	100		
101	160.5	11.4	17.0#
100	1202.9	9.1	13.7#

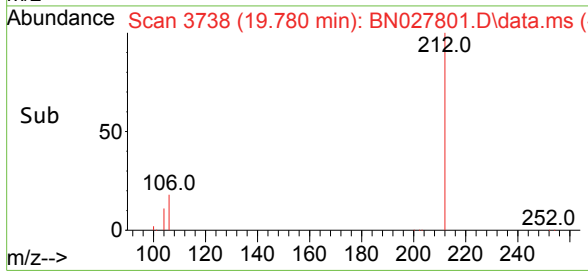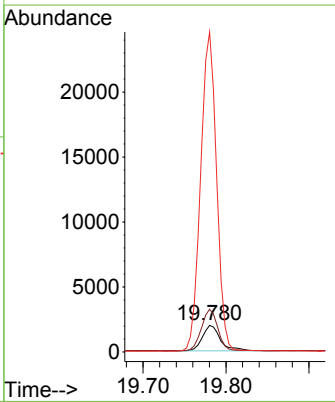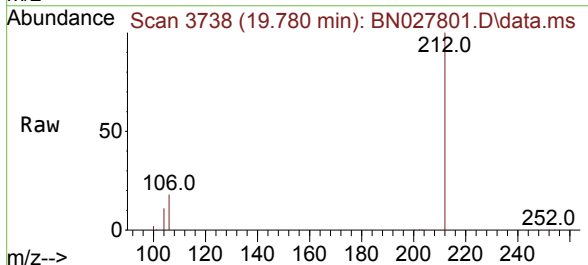

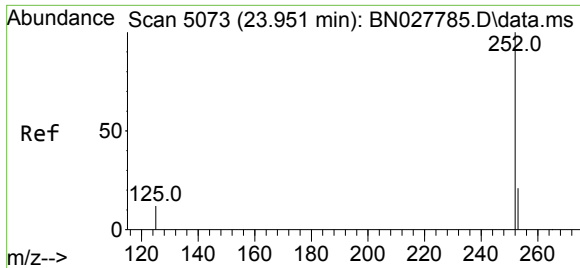

#26
 Benzo(a)pyrene
 Concen: 0.074 ng/ul
 RT: 23.898 min Scan# 50
 Delta R.T. -0.052 min
 Lab File: BN027801.D
 Acq: 22 Sep 2023 00:20

Instrument :
 BNA_N
 ClientSampleId :
 SBLK580

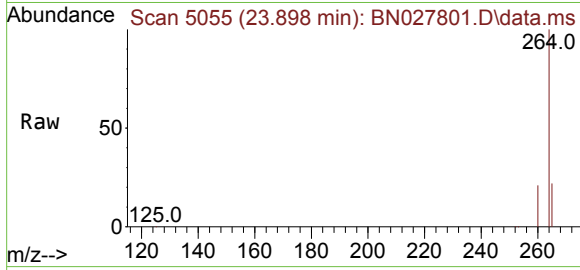

Tgt Ion:	252	Resp:	5378
Ion	Ratio	Lower	Upper
252	100		
253	56.2	21.9	32.9#
125	54.2	15.5	23.3#

