

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
 Data File : BN027838.D
 Acq On : 22 Sep 2023 23:22
 Operator : MA/JU
 Sample : 04387-12
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF3

Quant Time: Sep 23 03:50:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	5307	0.400	ng/ul	0.00
4) Naphthalene-d8	10.823	136	19611	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	12363	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	27874	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	22186	0.400	ng/ul	# 0.00
23) Perylene-d12	24.070	264	19982	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	26481	3.961	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	9969	0.335	ng/ul	0.00
18) Fluoranthene-d10	19.417	212	26243	0.387	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	279	0.040	ng/ul#	1
20) Pyrene	19.785	202	4034	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.907	252	5589	0.078	ng/ul#	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
Data File : BN027838.D
Acq On : 22 Sep 2023 23:22
Operator : MA/JU
Sample : 04387-12
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF3

Quant Time: Sep 23 03:50:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration




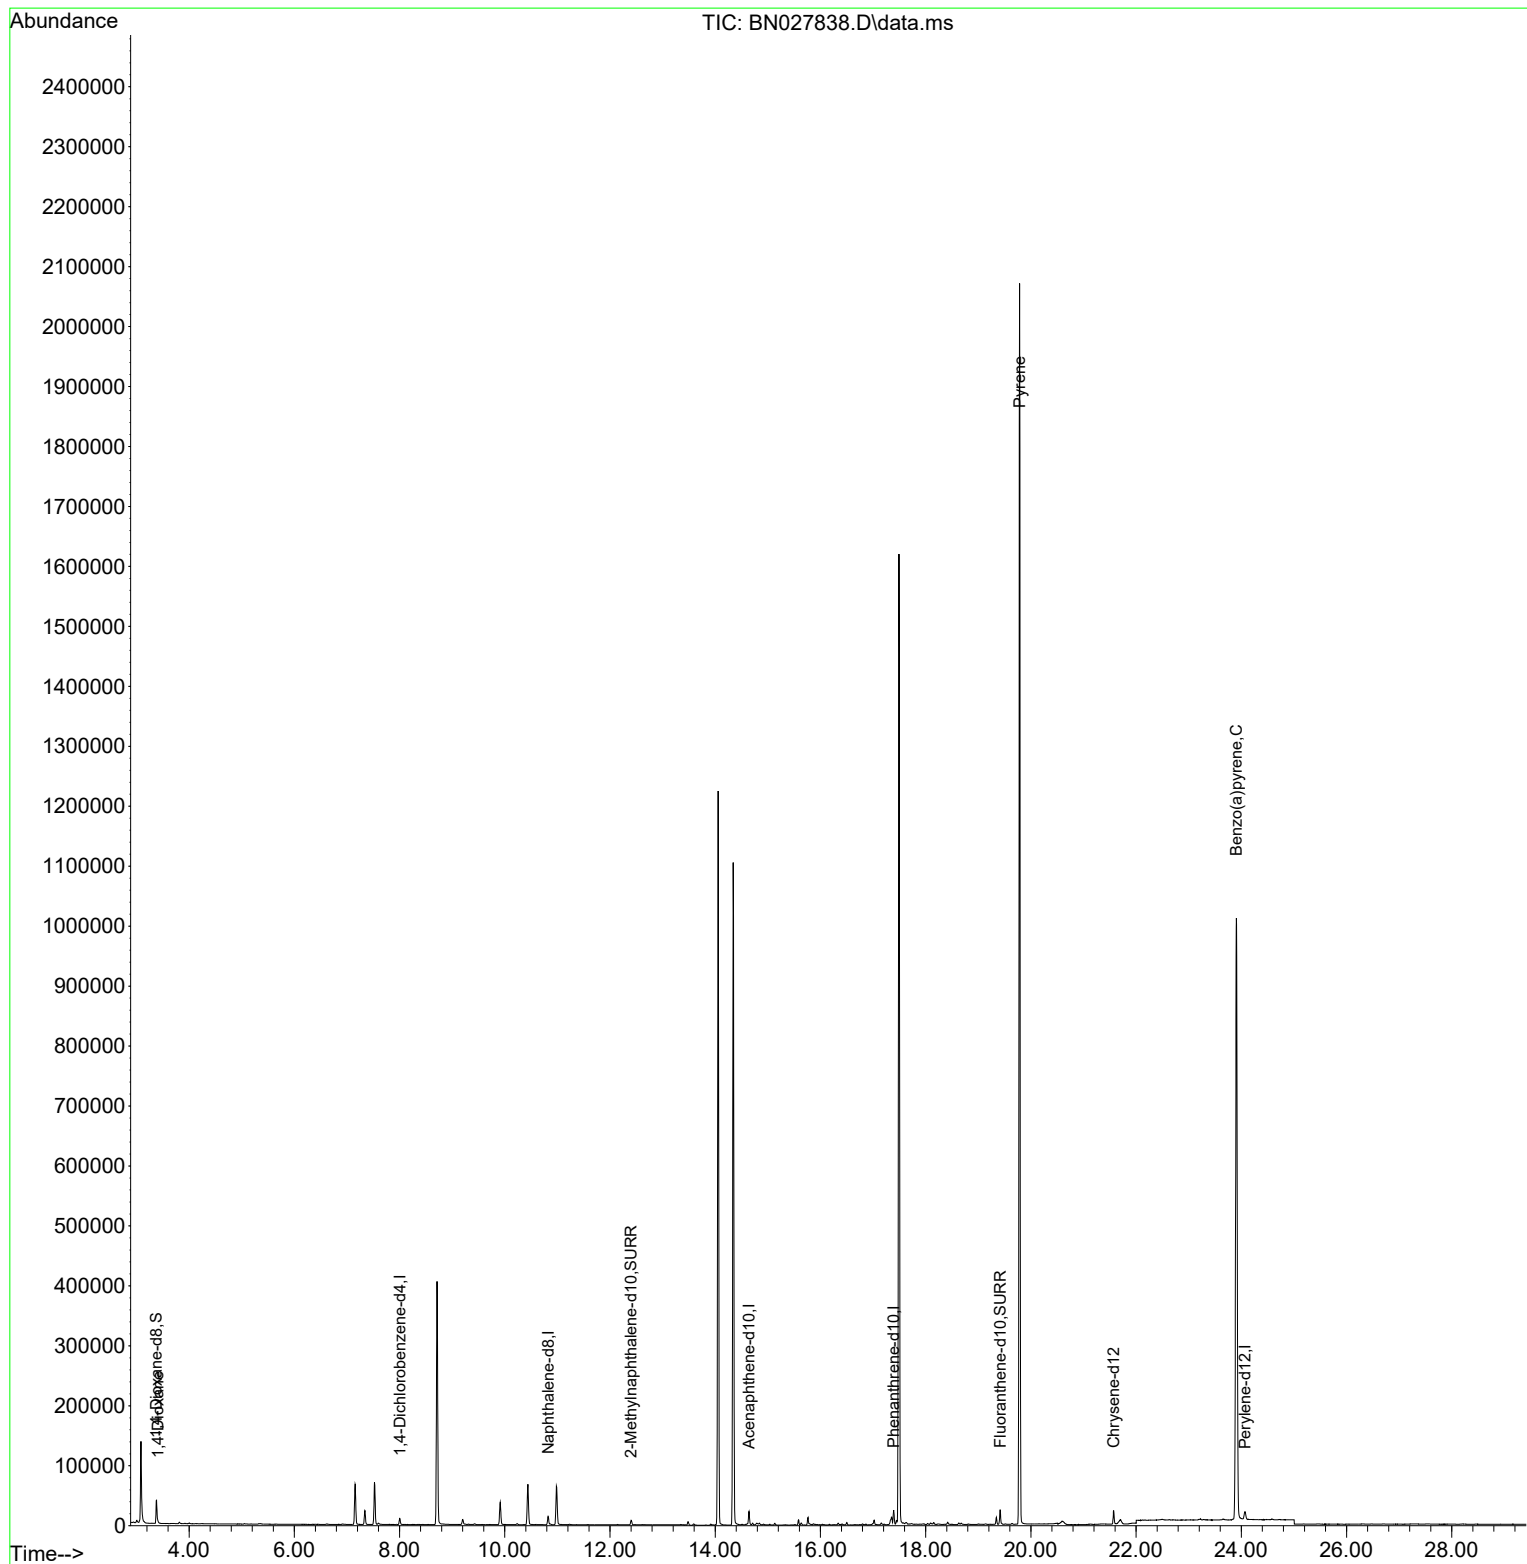


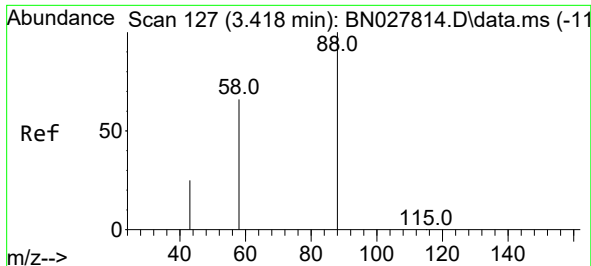

#2
1,4-Dioxane
Concen: 0.040 ng/ul
RT: 3.406 min Scan# 11
Delta R.T. -0.017 min
Lab File: BN027838.D
Acq: 22 Sep 2023 23:22




Instrument :
BNA_N
ClientSampleId :
C0AF3


Tgt Ion: 88 Resp: 279
Ion Ratio Lower Upper
88 100
43 384.6 39.6 59.4#
58 33.0 48.3 72.5#

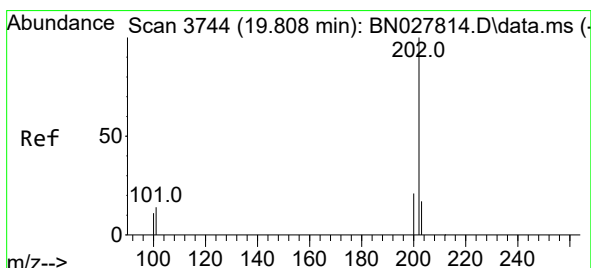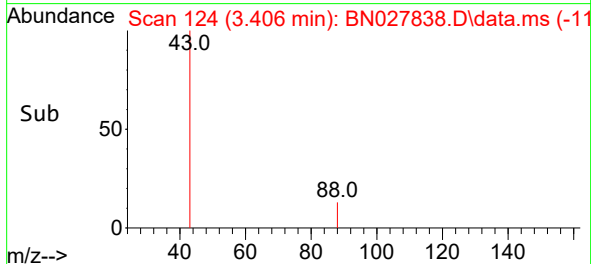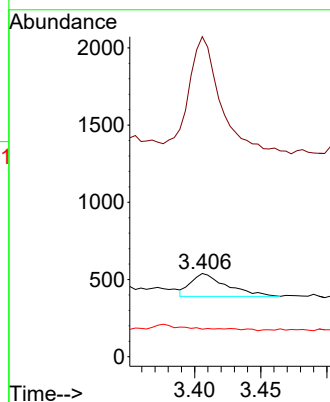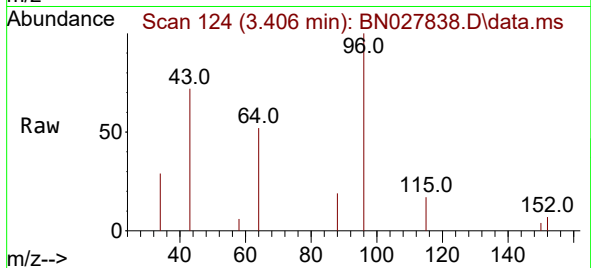

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.785 min Scan# 3739
Delta R.T. -0.028 min
Lab File: BN027838.D
Acq: 22 Sep 2023 23:22


Tgt Ion: 202 Resp: 4034
Ion Ratio Lower Upper
202 100
101 150.4 11.4 17.0#
100 1063.0 9.1 13.7#

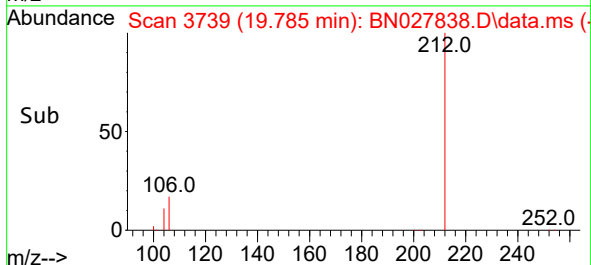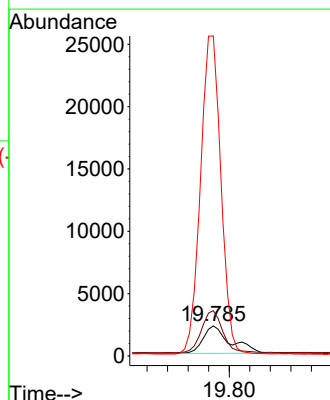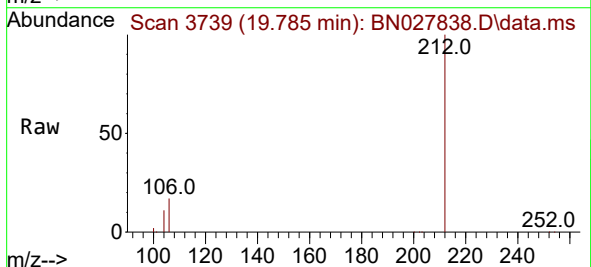

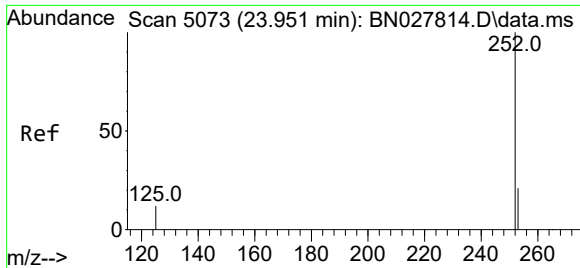

#26
 Benzo(a)pyrene
 Concen: 0.078 ng/ul
 RT: 23.907 min Scan# 50
 Delta R.T. -0.044 min
 Lab File: BN027838.D
 Acq: 22 Sep 2023 23:22

Instrument :
 BNA_N
 ClientSampleId :
 C0AF3

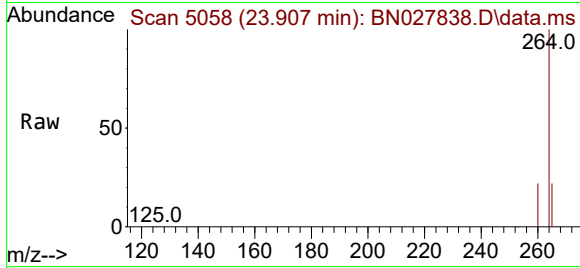

Tgt Ion:	252	Resp:	5589
Ion	Ratio	Lower	Upper
252	100		
253	69.3	21.9	32.9#
125	72.0	15.5	23.3#

