

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
 Data File : BN027809.D
 Acq On : 22 Sep 2023 05:09
 Operator : MA/JU
 Sample : 04332-20
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG8

Quant Time: Sep 22 06:27:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	5631	0.400	ng/ul	0.00
4) Naphthalene-d8	10.823	136	19383	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	12194	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	27326	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	22587	0.400	ng/ul	# 0.00
23) Perylene-d12	24.064	264	21373	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	30634	4.319	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	7642	0.260	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	19300	0.280	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.445	202	1988	0.022	ng/ul#	Qvalue 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092223\
Data File : BN027809.D
Acq On : 22 Sep 2023 05:09
Operator : MA/JU
Sample : 04332-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Quant Time: Sep 22 06:27:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration

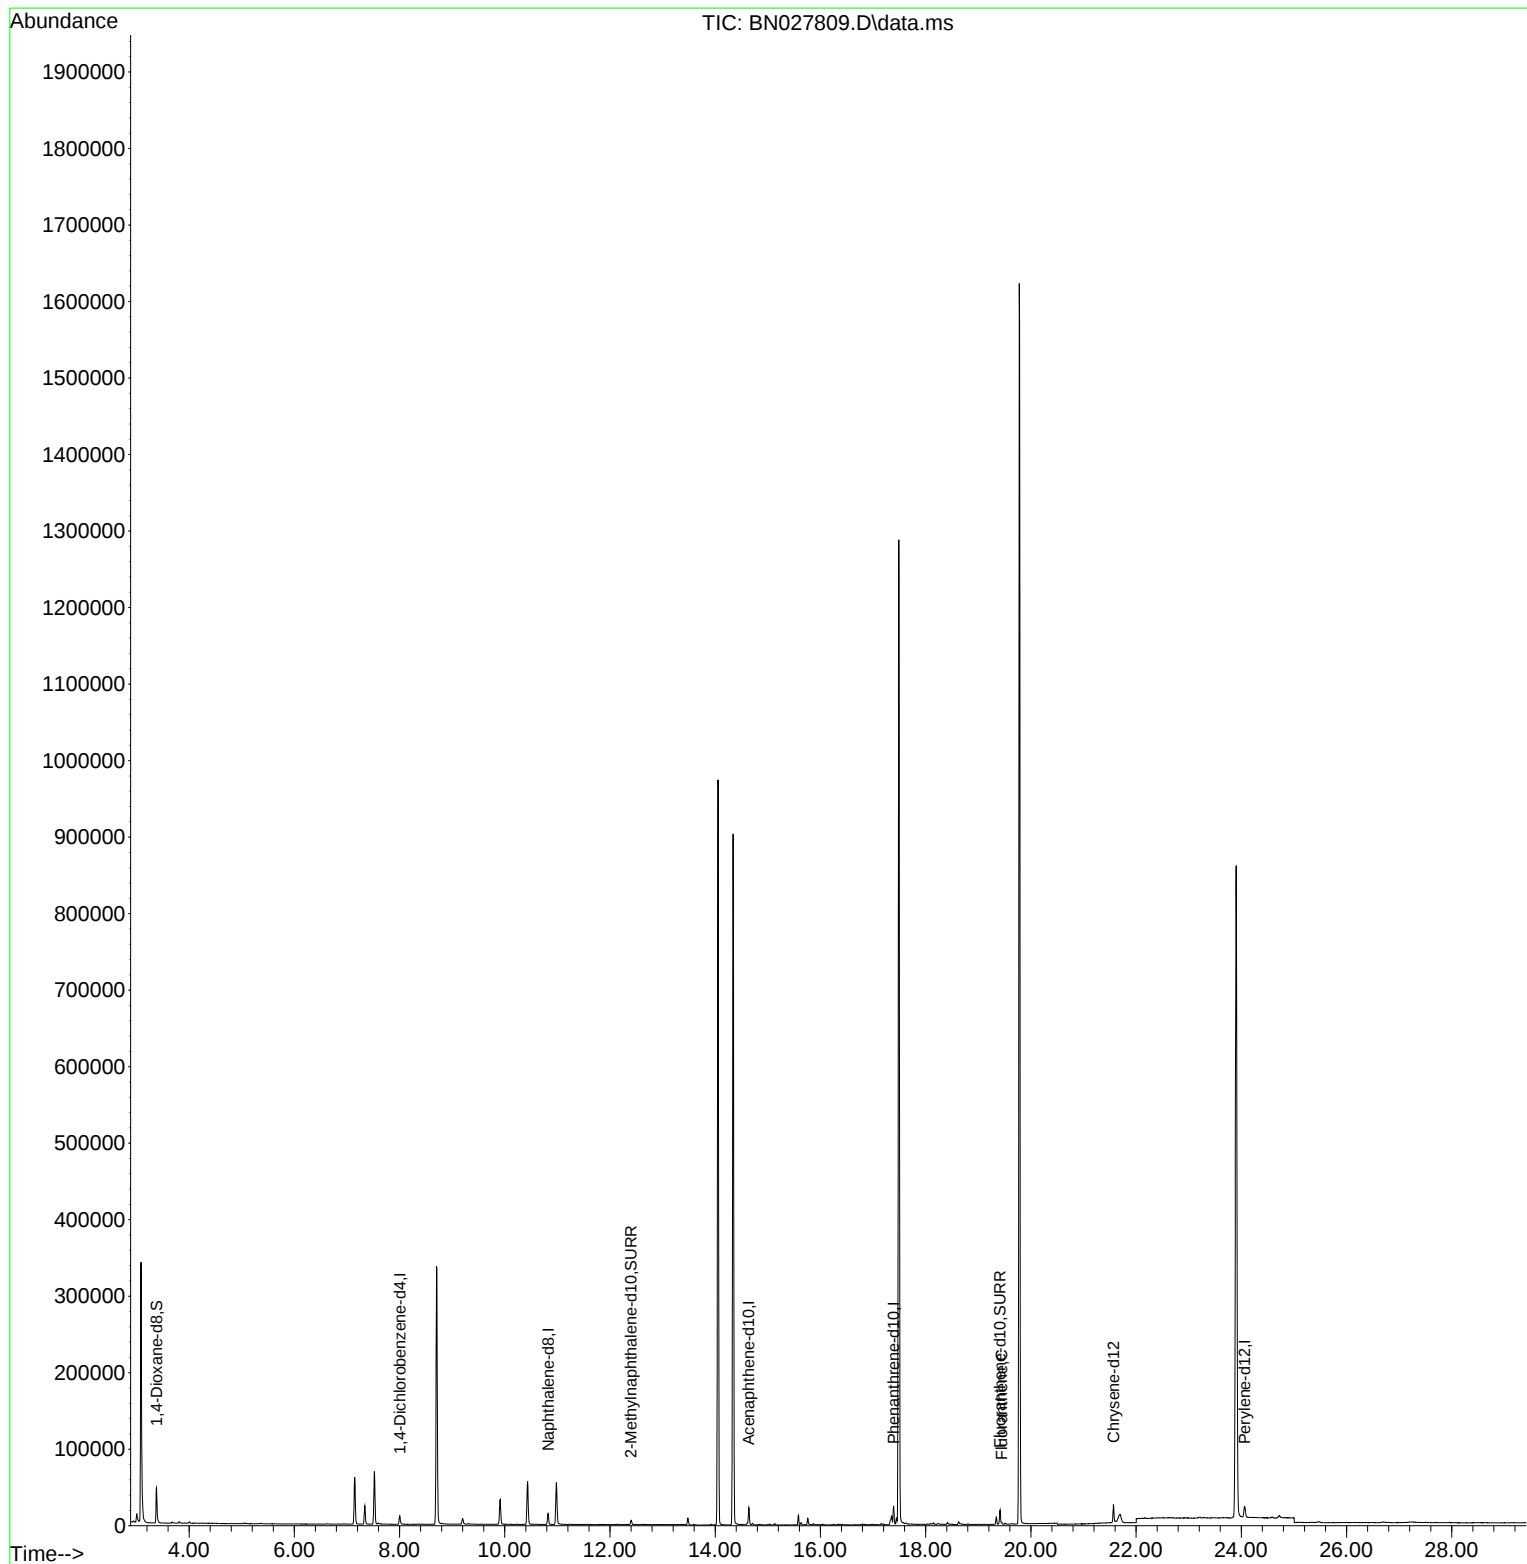

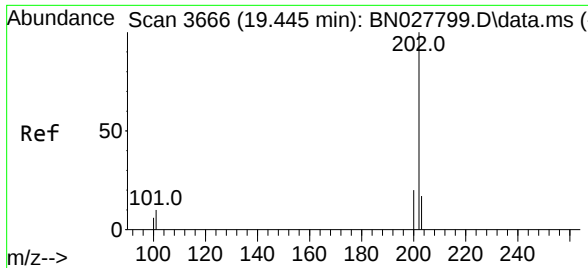

#19
 Fluoranthene
 Concen: 0.022 ng/ul
 RT: 19.445 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN027809.D
 Acq: 22 Sep 2023 05:09

Instrument :
 BNA_N
 ClientSampleId :
 C0AG8

Tgt Ion:	202	Resp:	1988
Ion	Ratio	Lower	Upper
202	100		
101	20.6	9.3	13.9#
100	14.2	7.0	10.4#

