

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092319\
 Data File : BN007825.D
 Acq On : 24 Sep 2019 05:53
 Operator : HP/JU
 Sample : PB123271BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	15	18	20	rBV2	50919	58078	0.68%	0.142%
2	3.140	24	26	29	rVV2	36002	34157	0.40%	0.083%
3	3.181	29	33	38	rVB	575020	624940	7.32%	1.524%
4	3.505	85	88	96	rVB3	40883	57174	0.67%	0.139%
5	3.958	162	165	170	rVB	35083	45480	0.53%	0.111%
6	4.593	270	273	277	rVB4	13797	16822	0.20%	0.041%
7	4.869	319	320	327	rVB4	9120	15346	0.18%	0.037%
8	7.069	691	694	698	rBV4	6718	10076	0.12%	0.025%
9	7.687	791	799	812	rBV	2453078	3816766	44.70%	9.306%
10	10.457	1262	1270	1287	rBV	3032344	5048829	59.14%	12.309%
11	14.316	1919	1926	1941	rBV	4519335	6586084	77.14%	16.057%
12	15.316	2091	2096	2098	rBV3	8789	13924	0.16%	0.034%
13	16.845	2349	2356	2361	rBV4	16143	25402	0.30%	0.062%
14	17.057	2385	2392	2404	rBV2	5365692	7919143	92.75%	19.307%
15	17.157	2404	2409	2415	rVB4	18613	37180	0.44%	0.091%
16	18.027	2555	2557	2564	rVB4	6748	12610	0.15%	0.031%
17	20.398	2956	2960	2964	rBV6	30709	47385	0.56%	0.116%
18	21.257	3100	3106	3117	rBV	6607235	8537753	100.00%	20.816%
19	21.368	3122	3125	3132	rBV2	98196	175062	2.05%	0.427%
20	23.468	3475	3482	3497	rVB	4440592	7933747	92.93%	19.343%


Sum of corrected areas: 41015958

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092319\
Data File : BN007825.D
Acq On : 24 Sep 2019 05:53
Operator : HP/JU
Sample : PB123271BL
Misc : GCMS CONFIRMATION
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK71

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

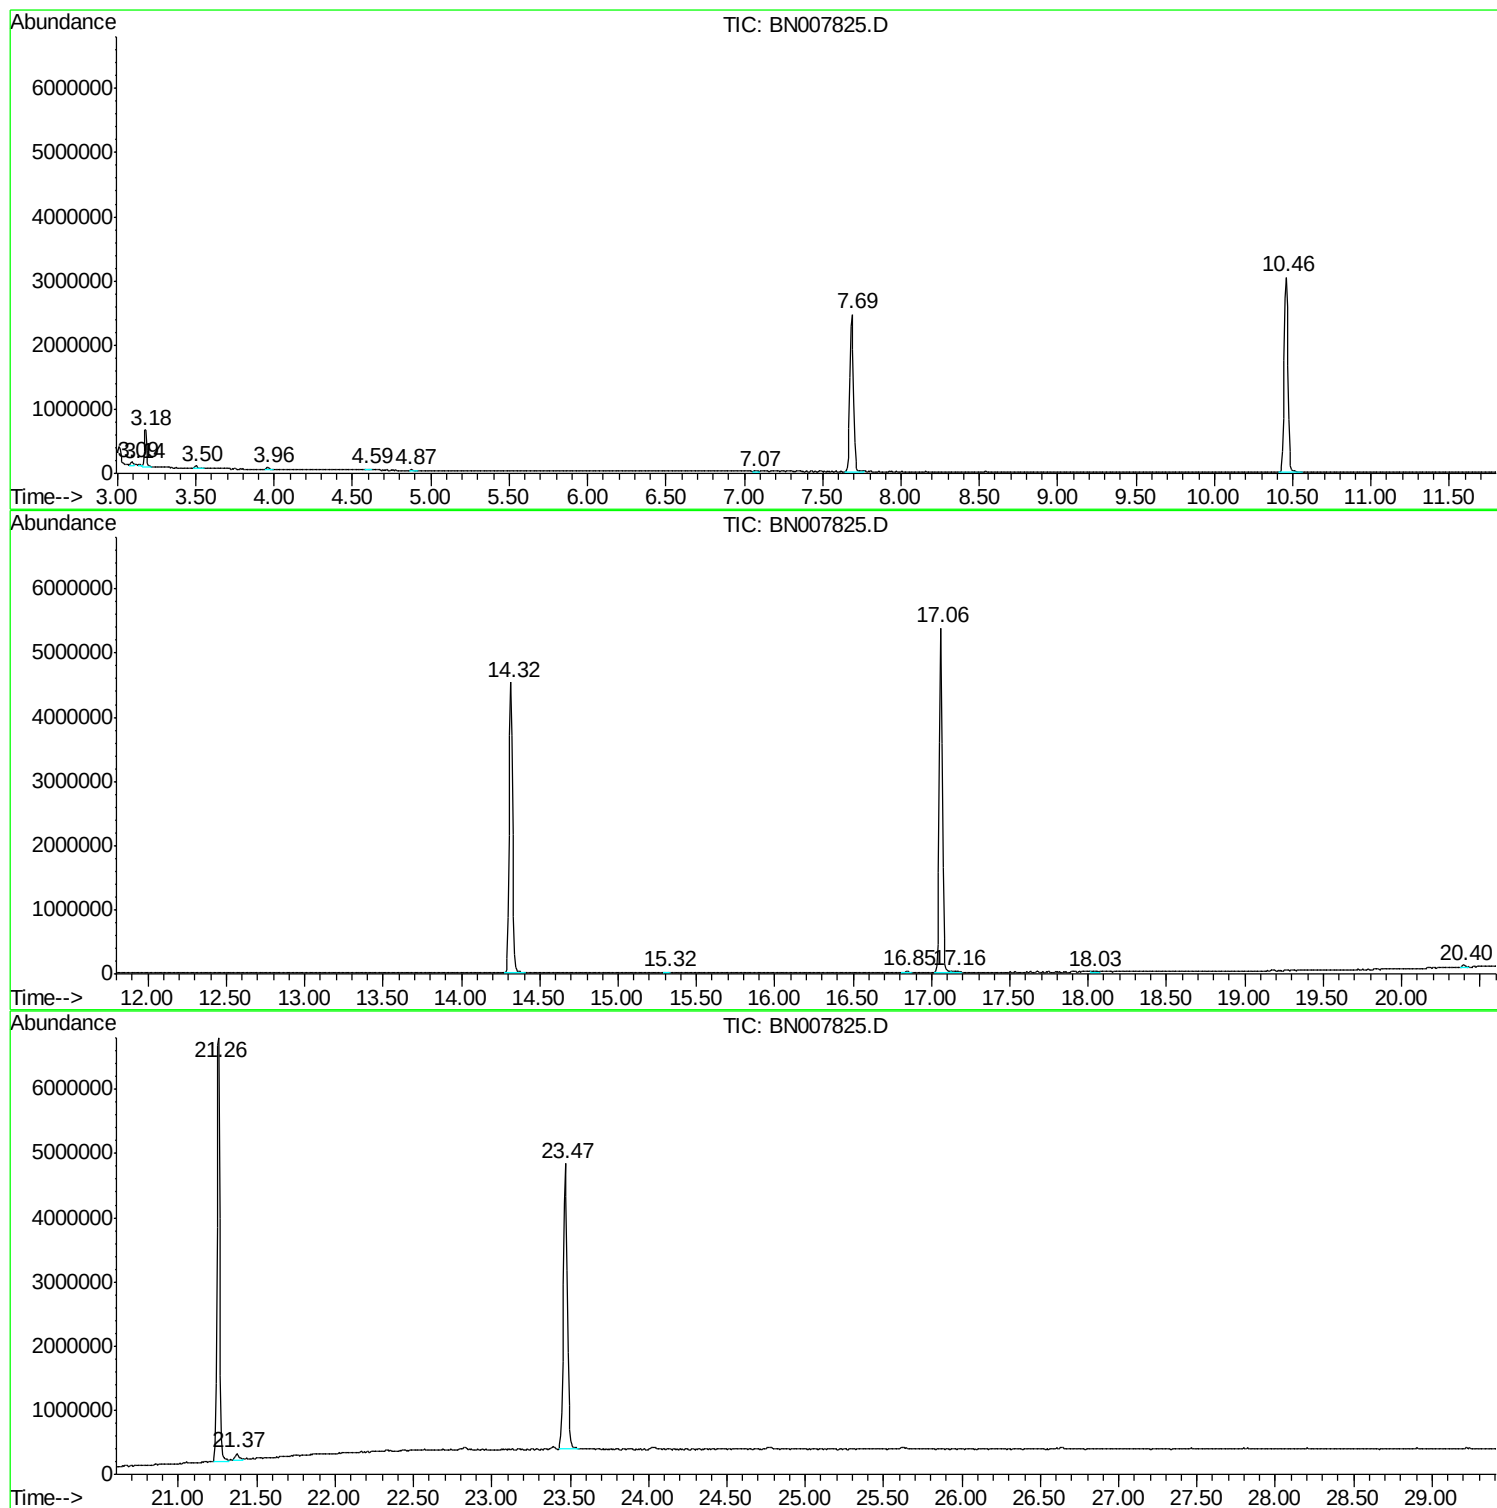

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092319\
Data File : BN007825.D
Acq On : 24 Sep 2019 05:53
Operator : HP/JU
Sample : PB123271BL
Misc : GCMS CONFIRMATION
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK71










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.18	3.27 ng/ul	624940	1,4-Dichlorobenzene-d4	7.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	91
2		Heptane	100	C7H16	000142-82-5	91
3		Heptane	100	C7H16	000142-82-5	91
4		Heptane	100	C7H16	000142-82-5	90
5		2-Bromononane	206	C9H19Br	002216-35-5	59

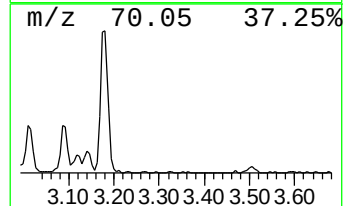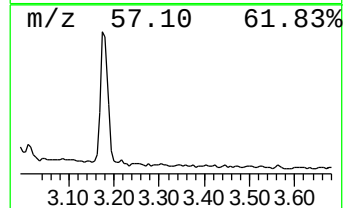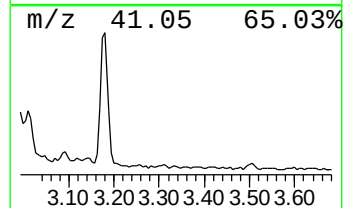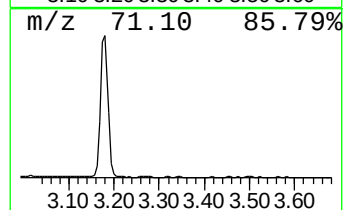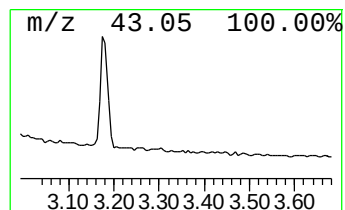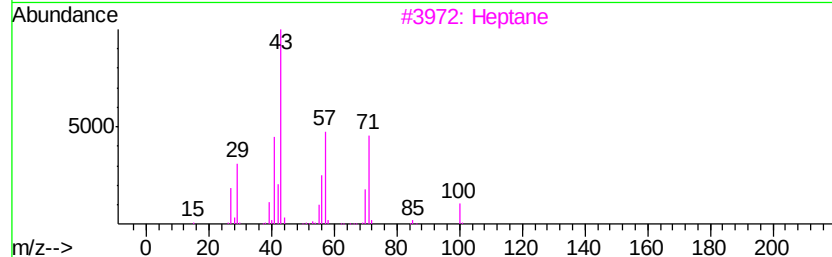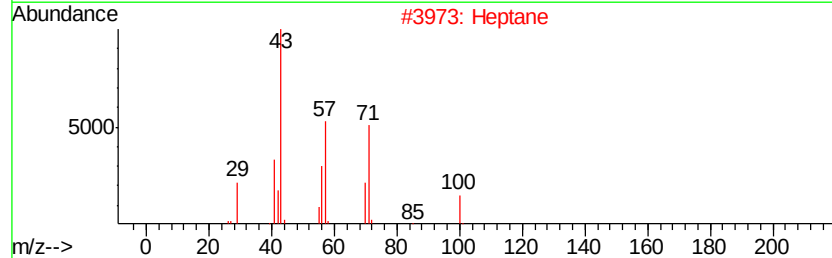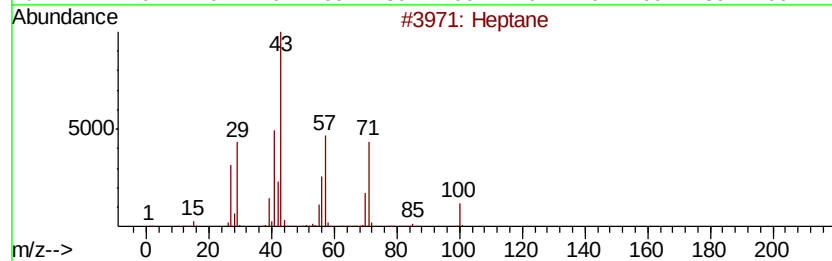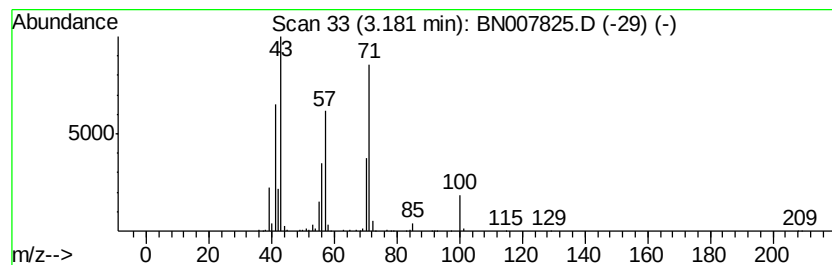

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092319\
Data File : BN007825.D
Acq On : 24 Sep 2019 05:53
Operator : HP/JU
Sample : PB123271BL
Misc : GCMS CONFIRMATION
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK71

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.18	3.3	ng/ul	624940	1	7.69	3816770	20.0