
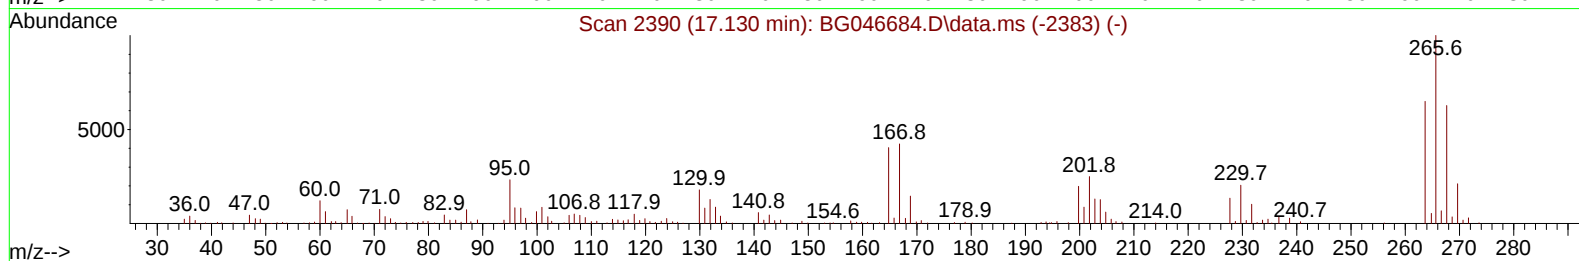
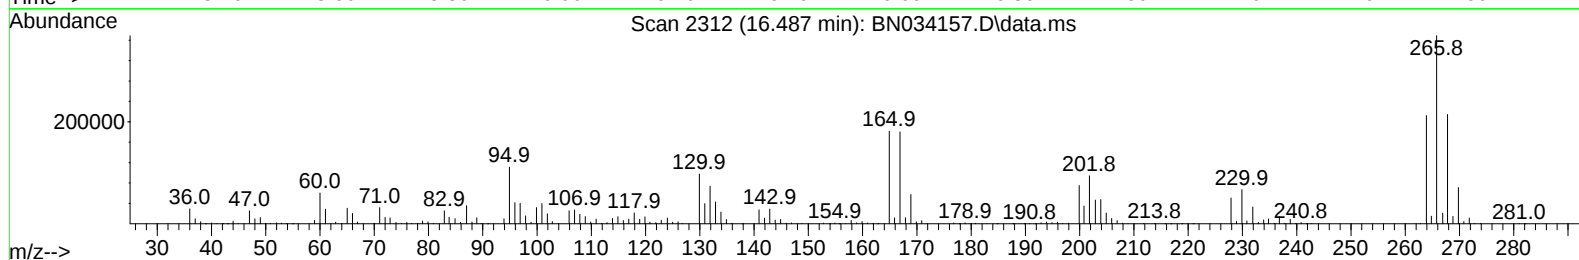


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092324\
Data File : BN034157.D
Acq On : 23 Sep 2024 09:27
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 13:22:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

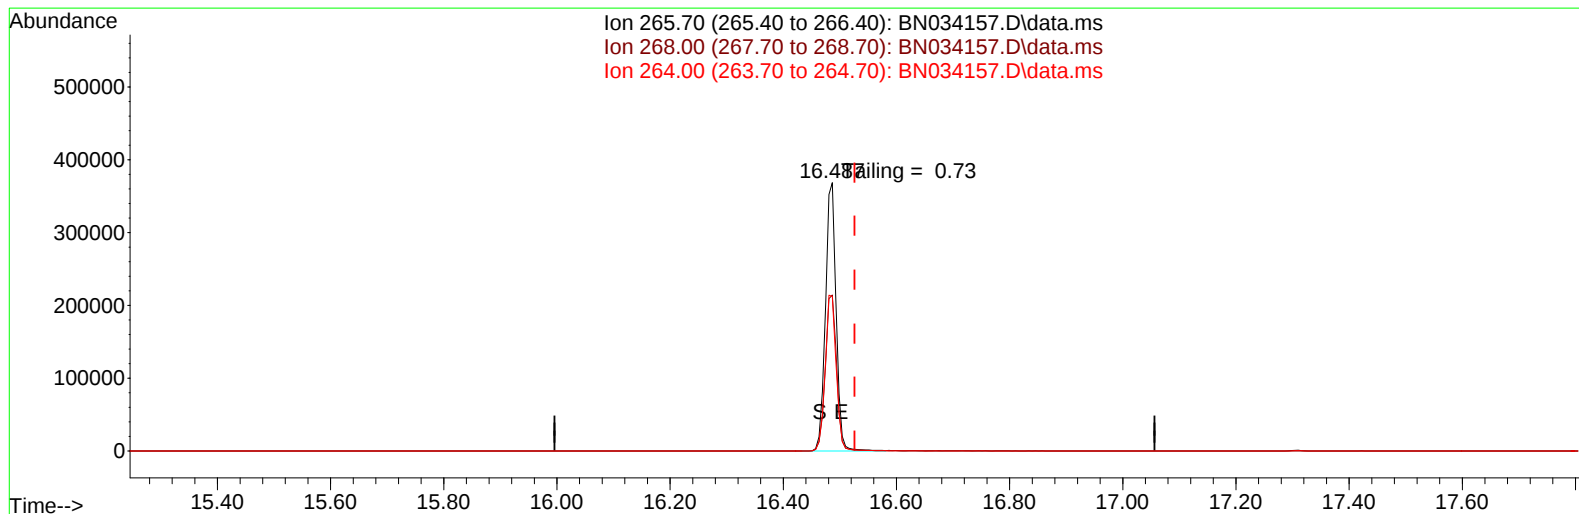

TIC: BN034157.D\data.ms

(70) Pentachlorophenol (C)




16.487min (-0.039) 19362.70 ng

response 484276

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.16
264.00	61.60	57.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092324\
Data File : BN034157.D
Acq On : 23 Sep 2024 09:27
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 13:22:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

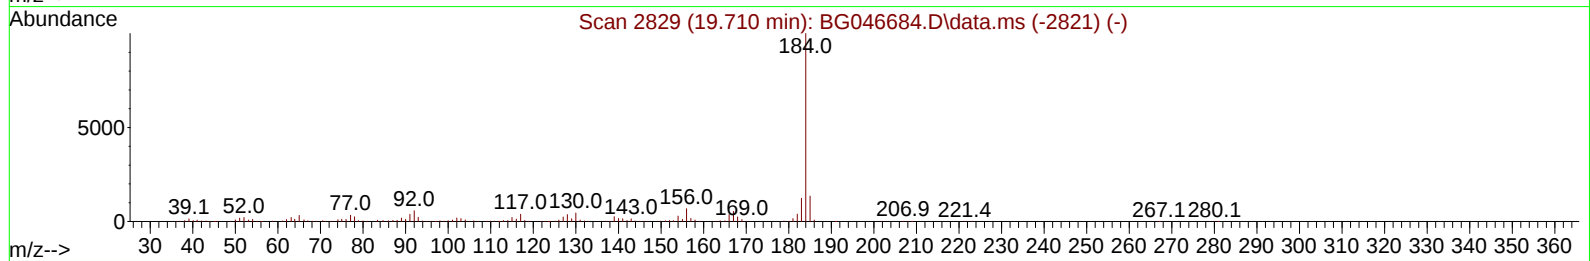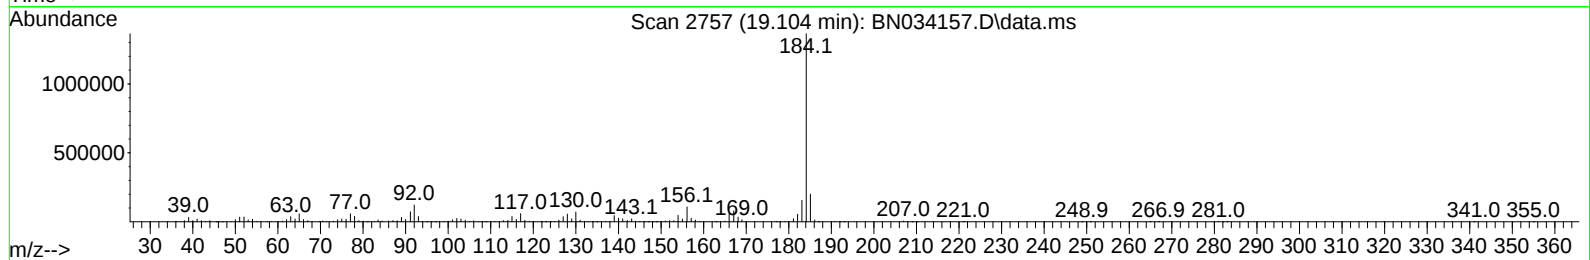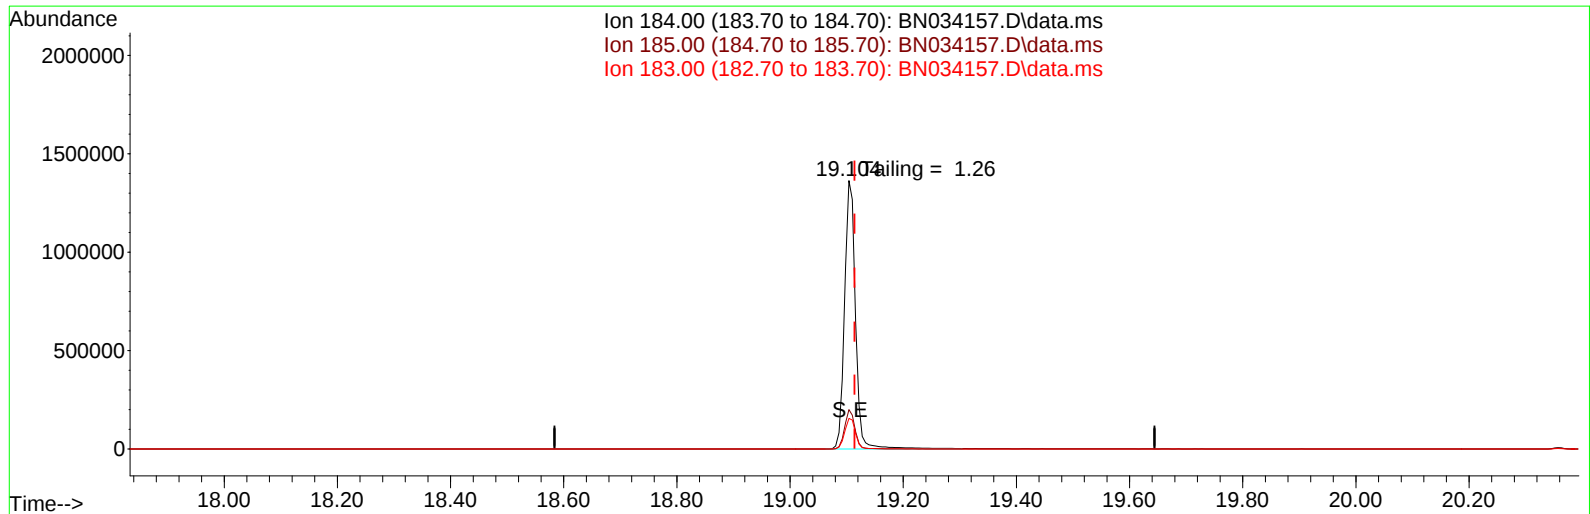

TIC: BN034157.D\data.ms

(77) Benzidine

19.104min (-0.010) 0.00 ng

response 1828086

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.71
183.00	13.20	11.40
0.00	0.00	0.00