


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092324\
Data File : BN034157.D
Acq On : 23 Sep 2024 09:27
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 18 16:09:28 2024

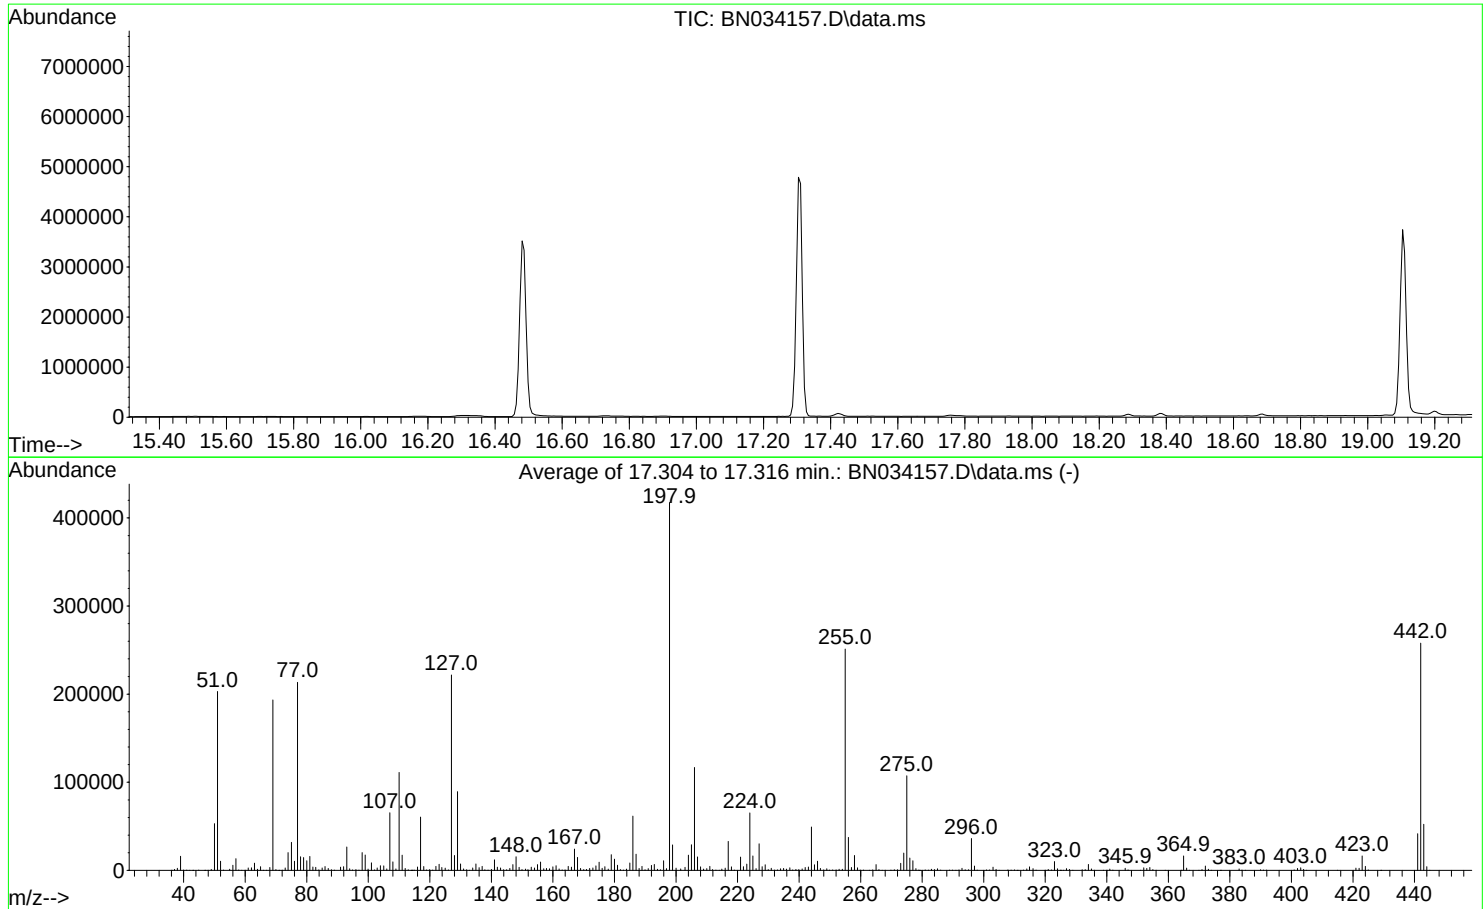




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	202983	PASS
68	69	0.00	2	1.7	3275	PASS
69	198	0.00	100	46.3	193336	PASS
70	69	0.00	2	0.5	967	PASS
127	198	10	80	53.1	221717	PASS
197	198	0.00	2	0.5	2035	PASS
198	198	100	100	100.0	417536	PASS
199	198	5	9	6.9	28947	PASS
275	198	10	60	25.7	107387	PASS
365	198	1	100	3.9	16285	PASS
441	198	0.01	100	10.0	41576	PASS
442	442	50	100	100.0	257835	PASS
443	442	15	24	20.3	52360	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092324\
Data File : BN034157.D
Acq On : 23 Sep 2024 09:27
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 23 13:22:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

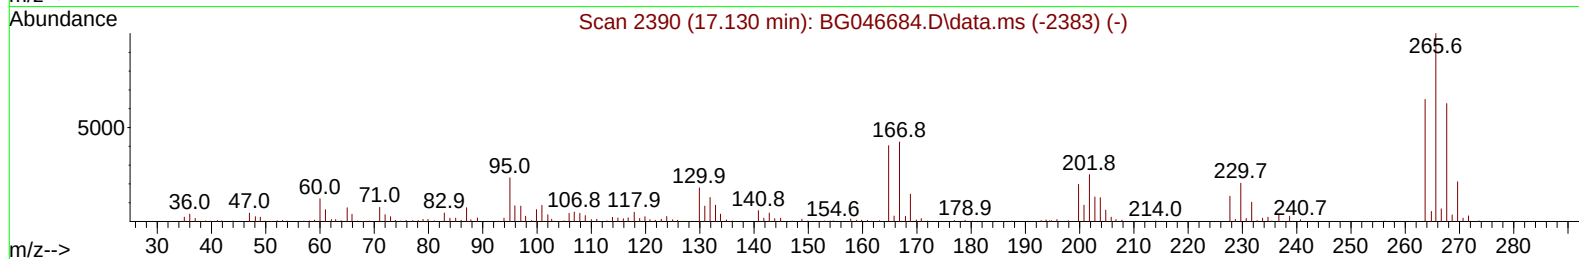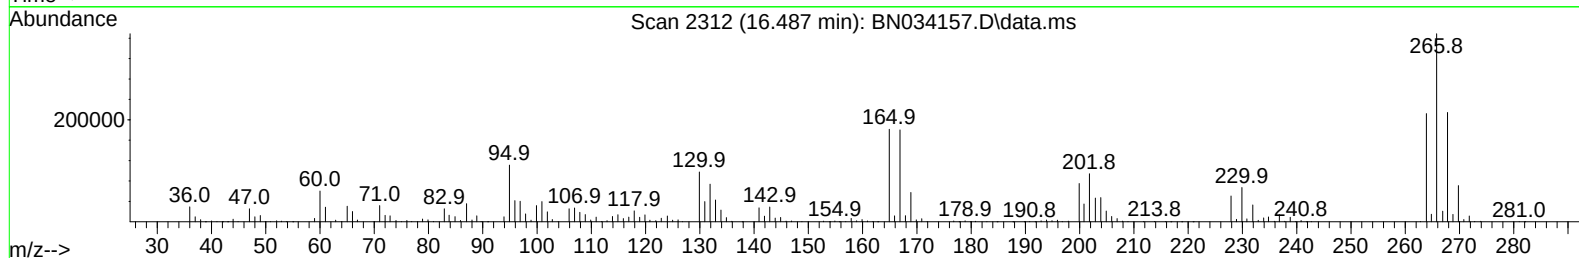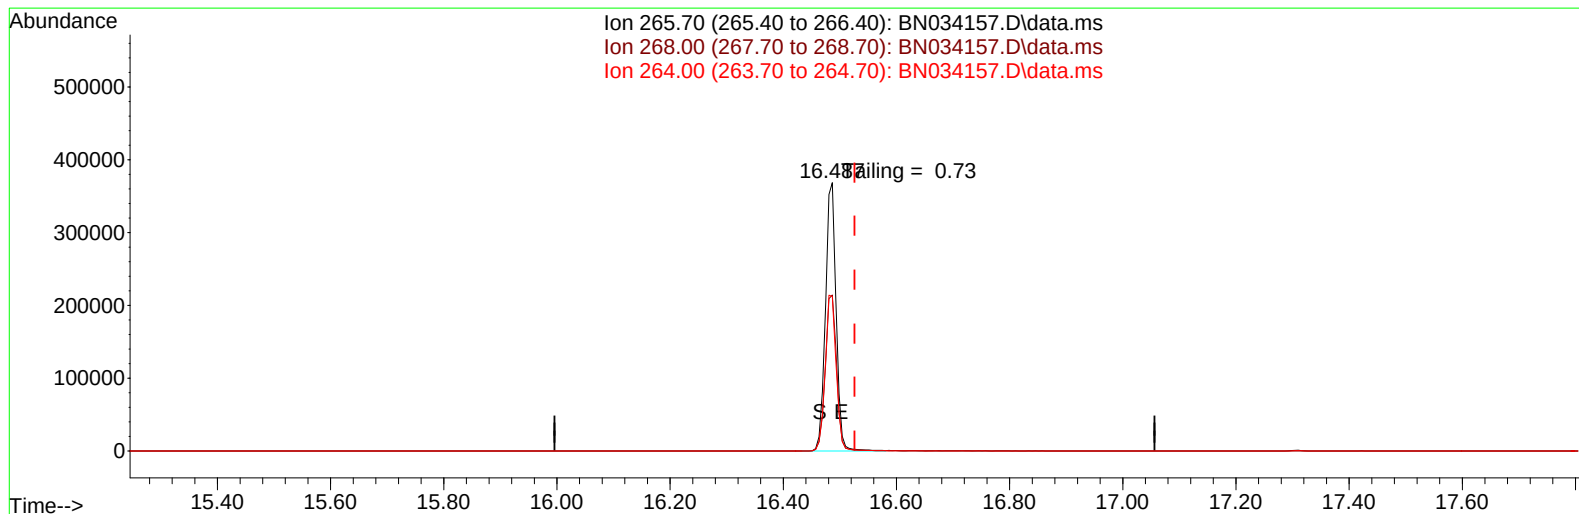

TIC: BN034157.D\data.ms

(70) Pentachlorophenol (C)

16.487min (-0.039) 19362.70 ng




response 484276

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.16
264.00	61.60	57.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092324\
Data File : BN034157.D
Acq On : 23 Sep 2024 09:27
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 23 13:22:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

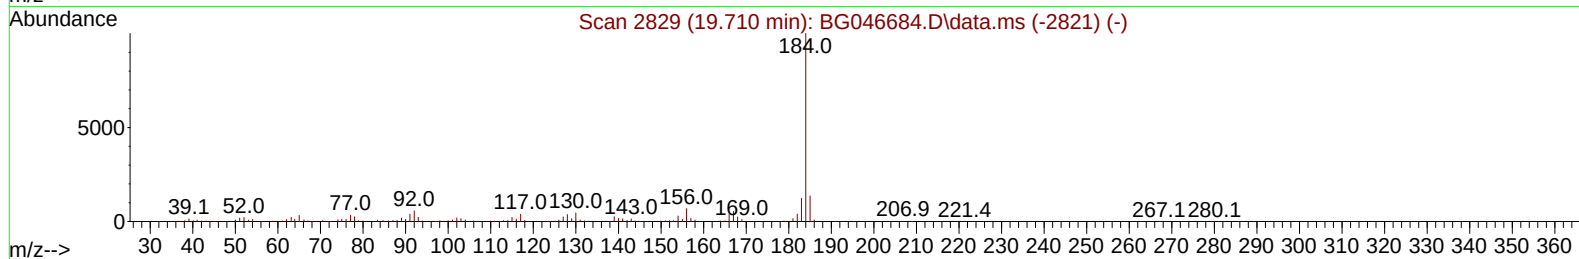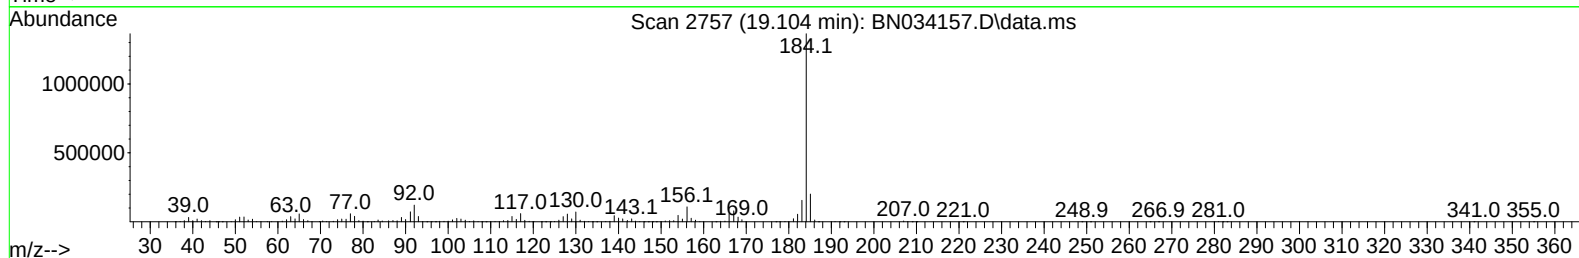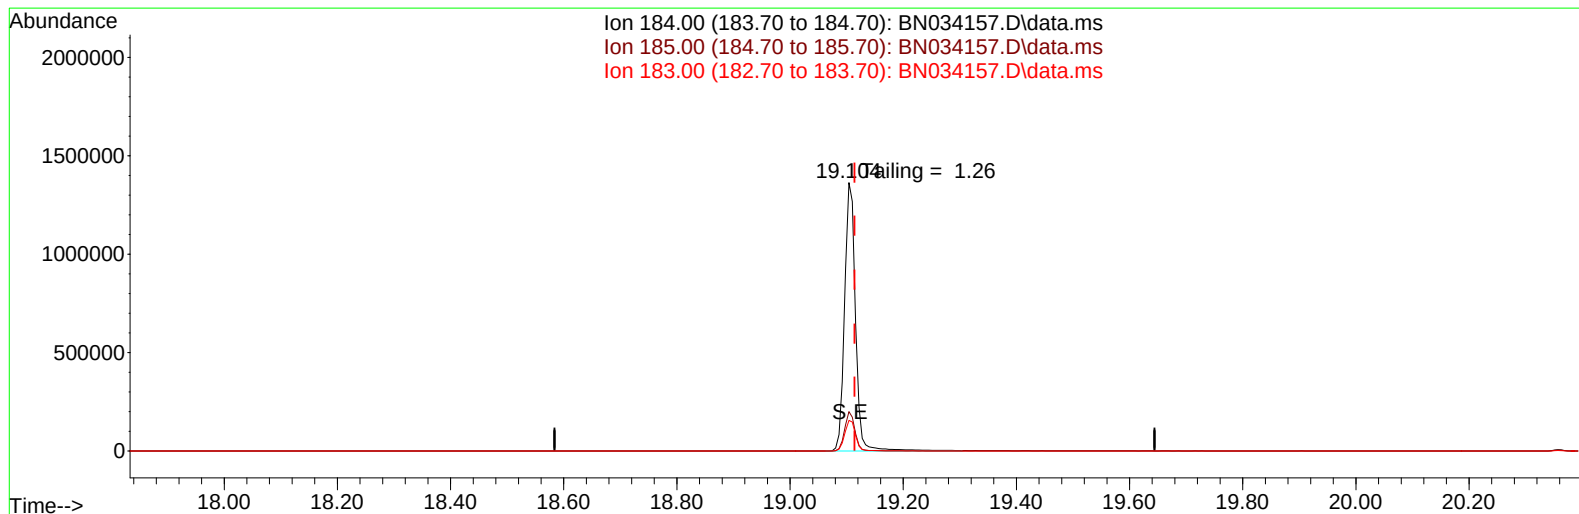

TIC: BN034157.D\data.ms

(77) Benzidine

19.104min (-0.010) 0.00 ng

response 1828086

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.71
183.00	13.20	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2024	BNA_N	<u>BN034157.D</u>
Compound Name	Response	Retention Time
DDT	1466882	20.357
DDD	18006	19.963
DDE	915	19.398
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18921	1485803	1.27

Instrument :
BNA_N
ClientSampleId :
DFTPP