

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
 Data File : BN007835.D
 Acq On : 24 Sep 2019 14:23
 Operator : JU
 Sample : K4985-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETJR7

Quant Time: Sep 24 15:36:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:15:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	525310	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	2170664	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	1405458	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	3071018	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	3216123	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	3481556	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	3755670	271.71	ng/uL	-0.03
5) Phenol-d5	6.86	99	254002	5.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	722532	25.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	718142	20.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	303305	7.96	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	447968	28.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	442777	29.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	870525	24.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	67781	1.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	3494238	31.24	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	3783505	29.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	102306	5.14	ng/ul	0.00
57) Fluorene-d10	15.31	176	2900322	29.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	399881	24.13	ng/ul	0.00
70) Anthracene-d10	17.16	188	4359918	28.52	ng/ul	0.00
78) Pyrene-d10	19.46	212	5513750	31.83	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	5928895	32.73	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.78	163	189754	1.665	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092419\
Data File : BN007835.D
Acq On : 24 Sep 2019 14:23
Operator : JU
Sample : K4985-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETJR7

Quant Time: Sep 24 15:36:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:15:33 2019
Response via : Initial Calibration

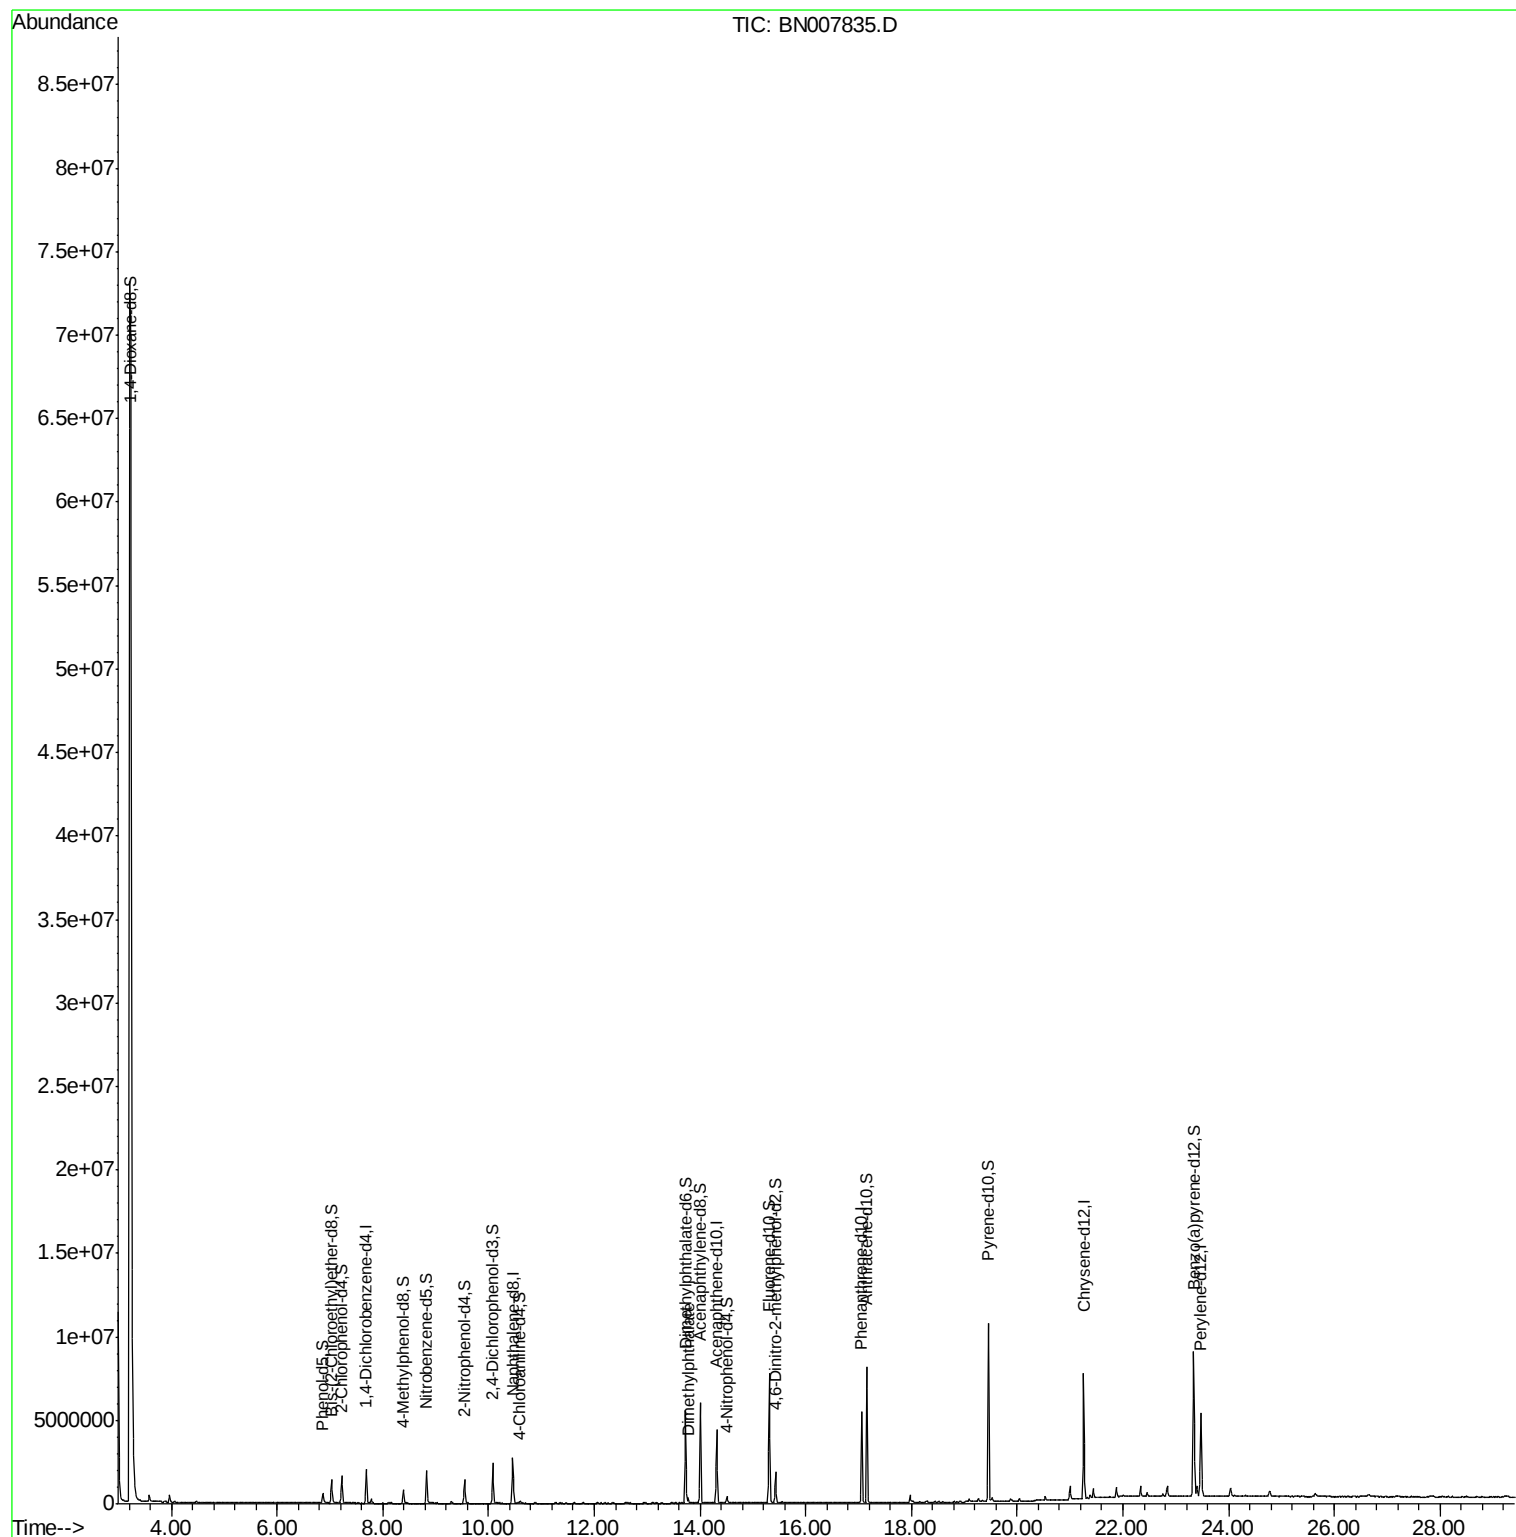

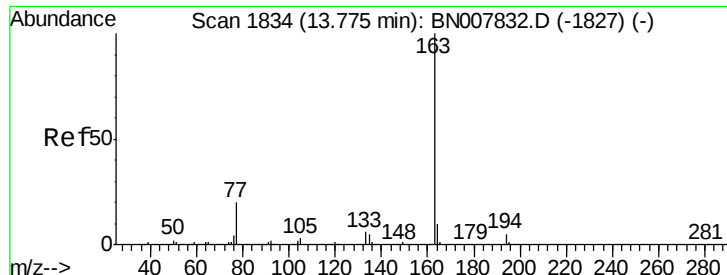

#44

Dimethylphthalate

Concen: 1.665 ng/ul

RT: 13.78 min Scan# 1834

Delta R.T. 0.00 min

Lab File: BN007835.D

Acq: 24 Sep 2019 14:23

Instrument :

BNA_N

ClientSampleId :

ETJR7


Tot Ion:163 Resp: 189754

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.2

164 10.1 8.4 12.6

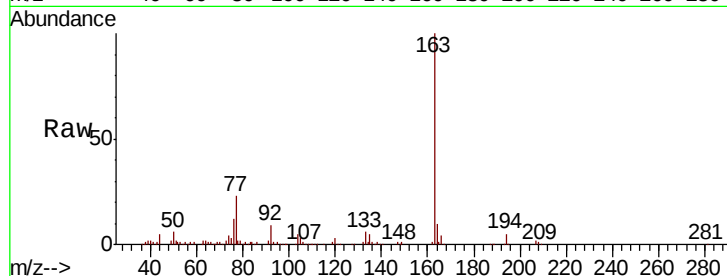

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

