

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
 Data File : BN007836.D
 Acq On : 24 Sep 2019 14:59
 Operator : JU
 Sample : K4985-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETJR8

Quant Time: Sep 24 15:38:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:15:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	534259	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	2160637	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	1389537	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	2989697	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	3138104	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	3448915	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	56233	4.00	ng/uL	0.00
5) Phenol-d5	6.86	99	260307	5.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	716226	24.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	741504	20.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	471327	12.16	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	440628	27.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	438944	29.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	860162	24.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	103980	2.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	3145284	28.45	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	3517067	27.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	76713	3.90	ng/ul	0.00
57) Fluorene-d10	15.31	176	2730169	28.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	352377	21.84	ng/ul	0.00
70) Anthracene-d10	17.16	188	4657624	31.30	ng/ul	0.00
78) Pyrene-d10	19.46	212	5641735	33.38	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	5980706	33.33	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.77	163	256347	2.274	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
Data File : BN007836.D
Acq On : 24 Sep 2019 14:59
Operator : JU
Sample : K4985-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETJR8

Quant Time: Sep 24 15:38:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:15:33 2019
Response via : Initial Calibration

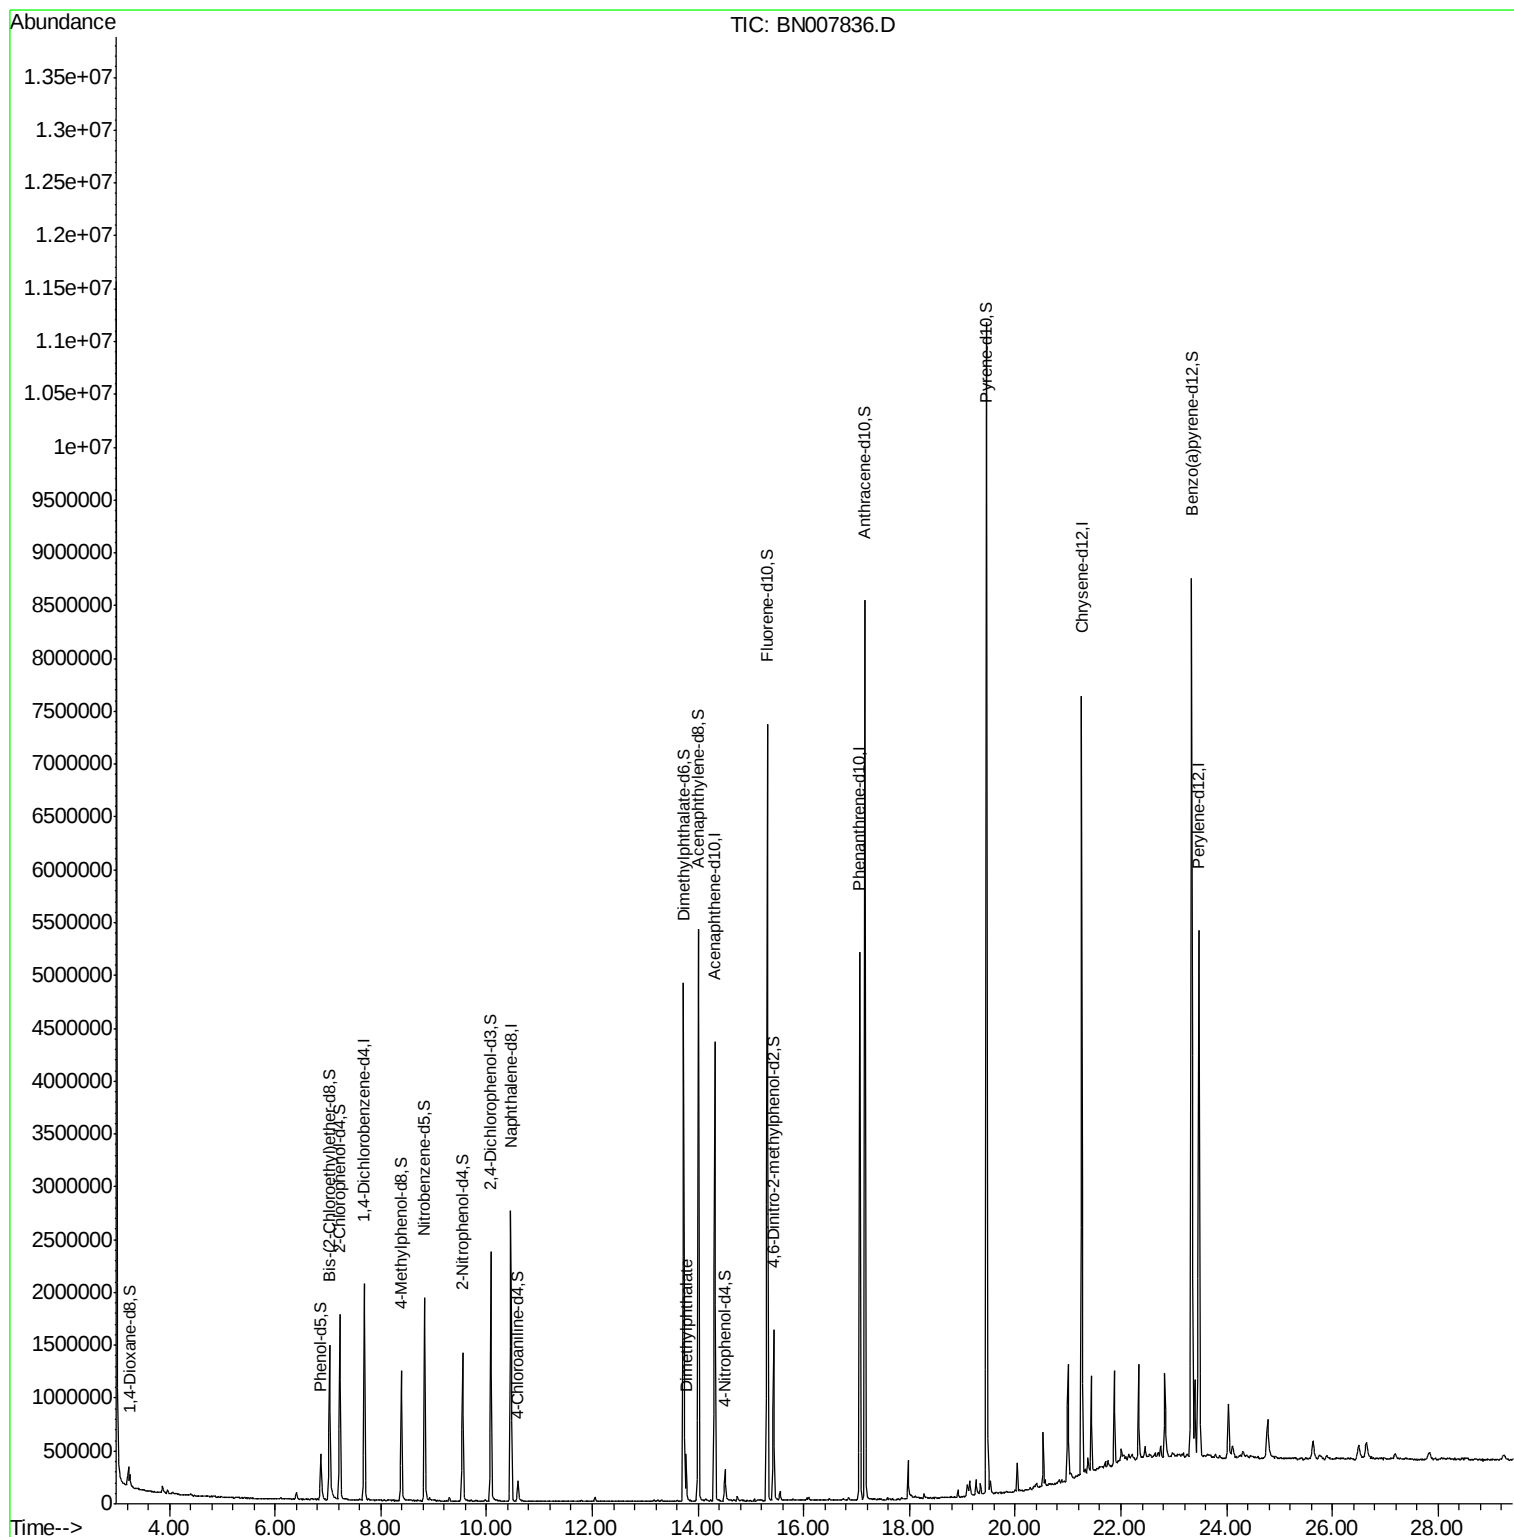

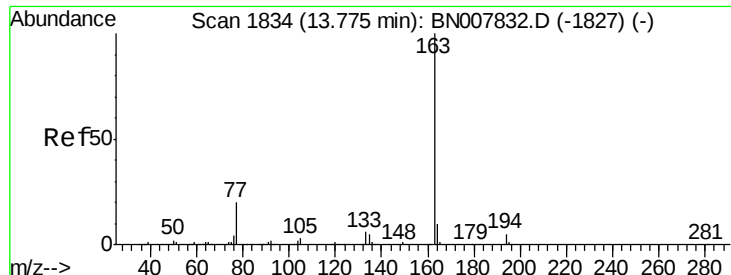

#44

Dimethylphthalate

Concen: 2.274 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.00 min

Lab File: BN007836.D

Acq: 24 Sep 2019 14:59

Instrument :

BNA_N

ClientSampleId :

ETJR8

Tot Ion:163 Resp: 256347

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.2 8.4 12.6

