

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092419\
 Data File : BN007837.D
 Acq On : 24 Sep 2019 15:35
 Operator : JU
 Sample : K4985-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETJR9

Quant Time: Sep 24 16:14:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:15:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	610515	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	2471899	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	1595122	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	3402011	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	3608789	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	3972609	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	63778	3.97	ng/uL	0.00
5) Phenol-d5	6.86	99	343704	5.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	831923	25.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	899122	22.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	600762	13.56	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	522623	28.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	528000	30.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	1028068	25.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	103843	1.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	3839108	30.25	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	4152028	28.56	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	126316	5.59	ng/ul	0.00
57) Fluorene-d10	15.31	176	3215846	29.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	479533	26.12	ng/ul	0.00
70) Anthracene-d10	17.16	188	5512964	32.55	ng/ul	0.00
78) Pyrene-d10	19.46	212	6652568	34.23	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	7102397	34.36	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.77	163	196735	1.521	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
Data File : BN007837.D
Acq On : 24 Sep 2019 15:35
Operator : JU
Sample : K4985-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETJR9

Quant Time: Sep 24 16:14:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:15:33 2019
Response via : Initial Calibration

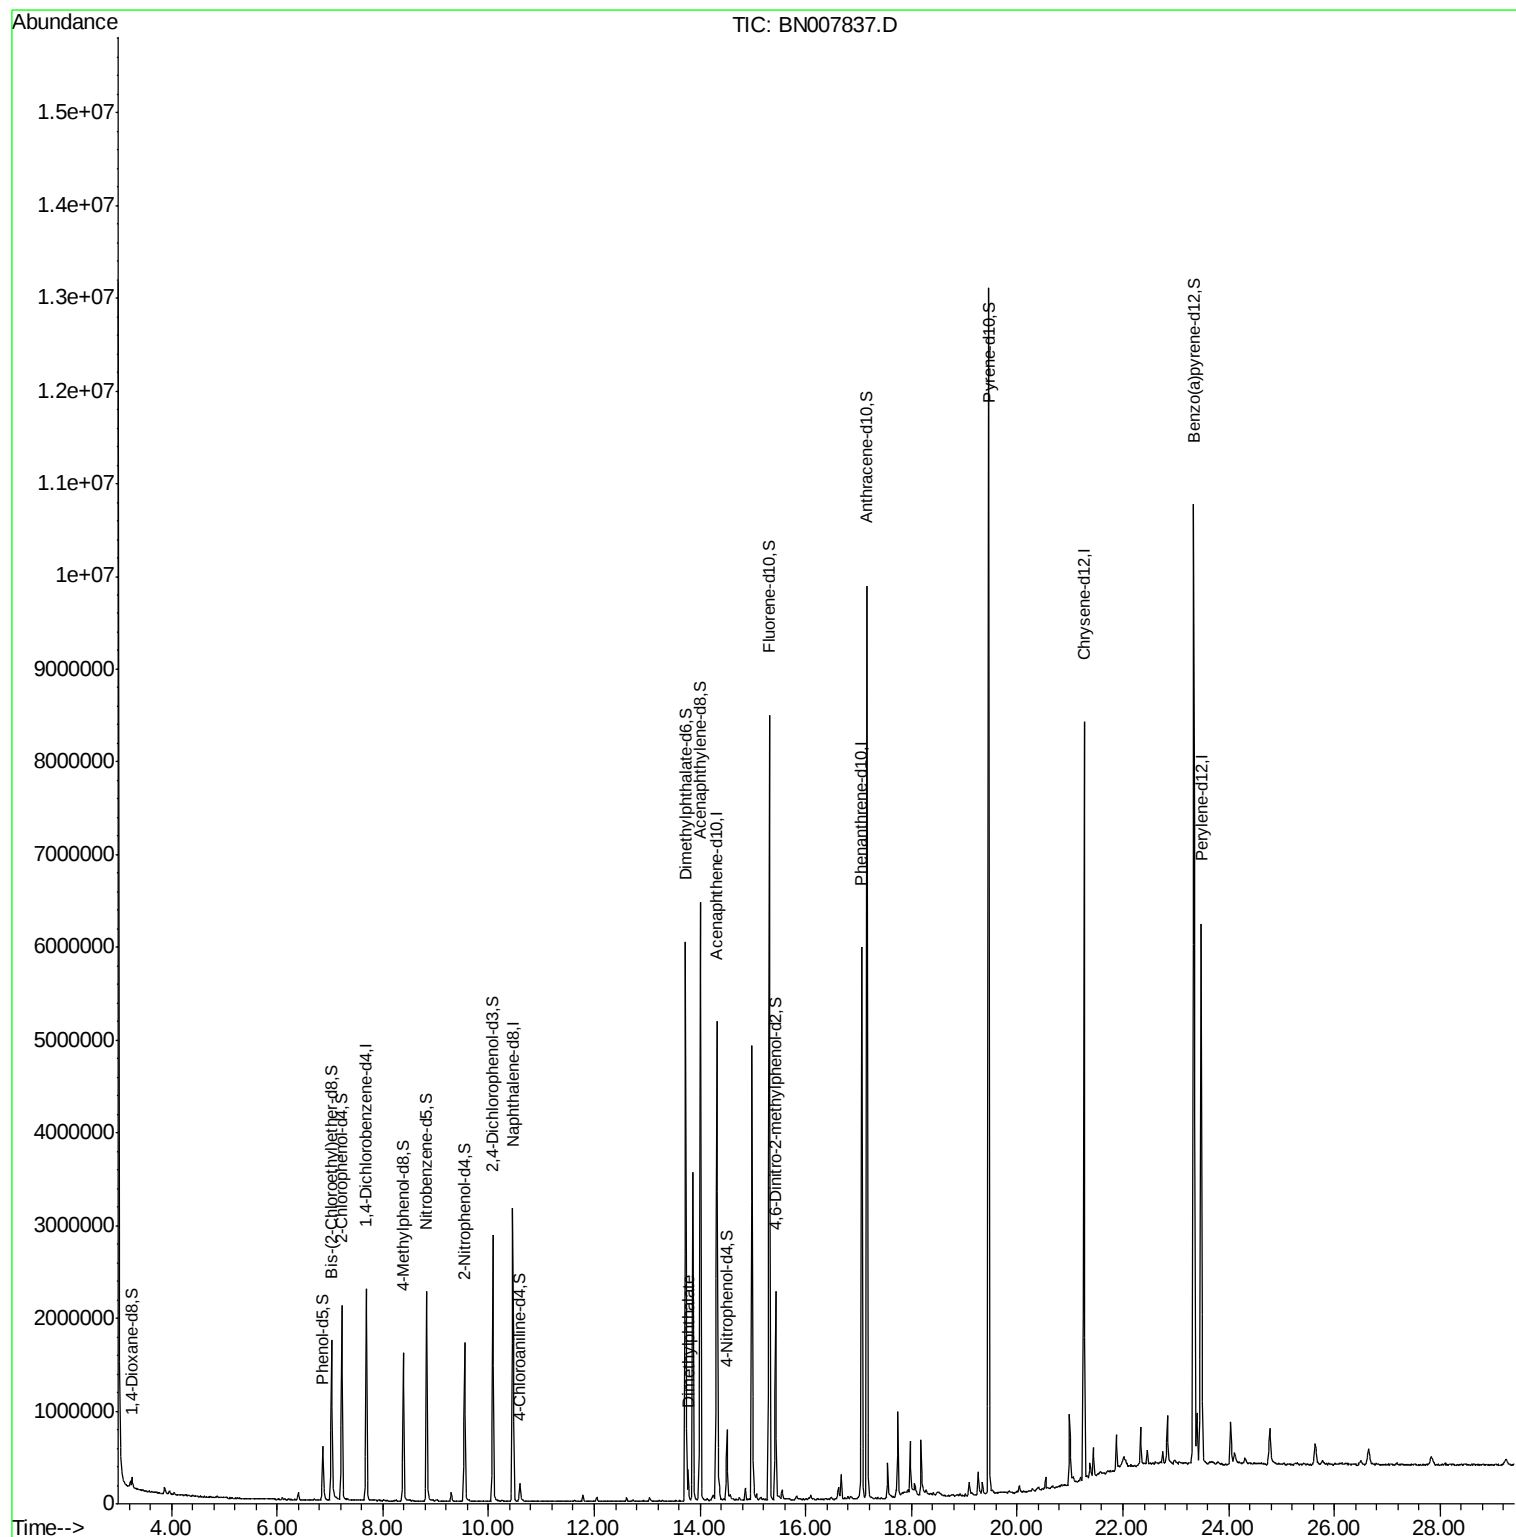

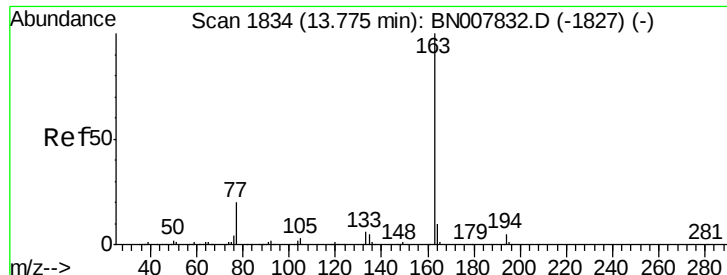

#44

Dimethylphthalate

Concen: 1.521 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. 0.00 min

Lab File: BN007837.D

Acq: 24 Sep 2019 15:35

Instrument :

BNA_N

ClientSampleId :

ETJR9


Tot Ion:163 Resp: 196735

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 9.7 8.4 12.6

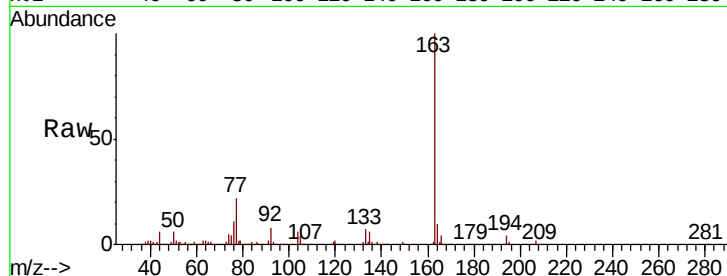

Abundance Ion 163.00 (162.70 to 163.70): E

200000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

