

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092419\
 Data File : BN007838.D
 Acq On : 24 Sep 2019 16:11
 Operator : JU
 Sample : K4985-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETJS0

Quant Time: Sep 24 16:54:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:15:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	557417	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	2279708	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	1488112	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	3152090	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	3336766	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	3608496	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	64632	4.41	ng/uL	0.00
5) Phenol-d5	6.86	99	314309	5.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	786706	26.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	828289	22.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	564321	13.95	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	484102	29.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	495481	31.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	943680	25.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	1305597	27.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	3410462	28.80	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	3805141	28.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	76041	3.61	ng/ul	0.00
57) Fluorene-d10	15.31	176	2973589	28.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	267367	15.72	ng/ul	0.00
70) Anthracene-d10	17.16	188	5247067	33.44	ng/ul	0.00
78) Pyrene-d10	19.46	212	6227272	34.65	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	6581599	35.06	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.77	163	156635	1.298	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
Data File : BN007838.D
Acq On : 24 Sep 2019 16:11
Operator : JU
Sample : K4985-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETJS0

Quant Time: Sep 24 16:54:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:15:33 2019
Response via : Initial Calibration

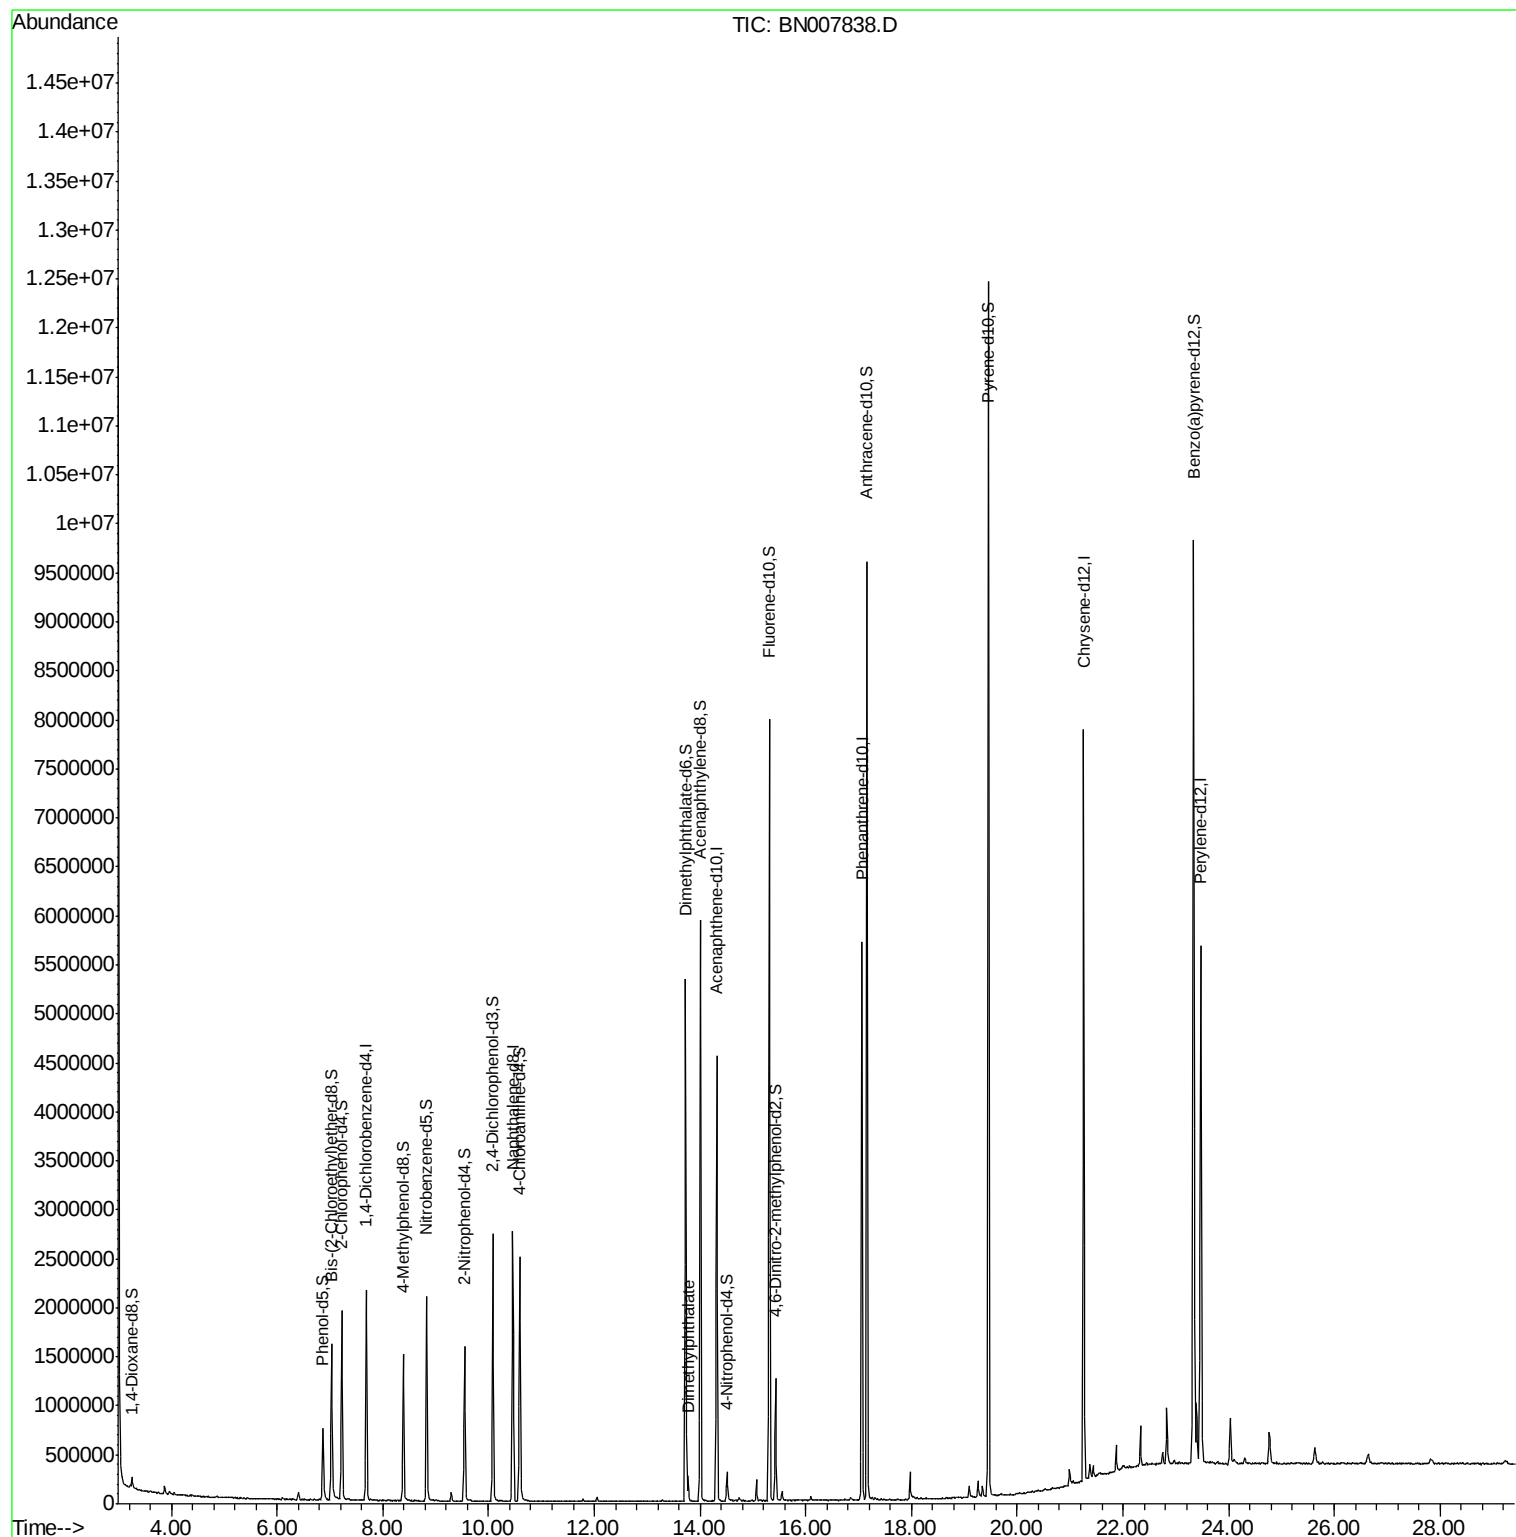

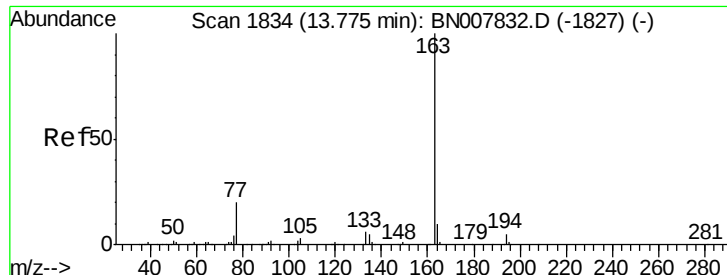

#44

Dimethylphthalate

Concen: 1.298 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.00 min

Lab File: BN007838.D

Acq: 24 Sep 2019 16:11

Instrument :

BNA_N

ClientSampleId :

ETJS0


Tot Ion:163 Resp: 156635

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 9.4 8.4 12.6

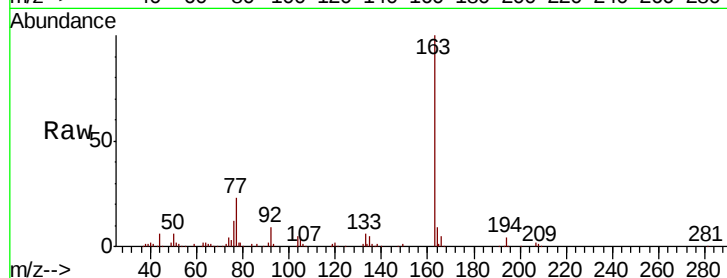

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

