

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
 Data File : BN007839.D
 Acq On : 24 Sep 2019 16:47
 Operator : JU
 Sample : K4985-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETJS1

Quant Time: Sep 24 17:32:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:15:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	488225	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1973143	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	1269522	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	2730470	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	2851789	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	3091427	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	59252	4.61	ng/uL	0.00
5) Phenol-d5	6.86	99	270807	5.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	733534	27.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	754479	23.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	503470	14.21	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	451220	31.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	451143	33.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	881063	27.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	1188444	28.55	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	3274585	32.42	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	3569037	30.85	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	77760	4.33	ng/ul	0.00
57) Fluorene-d10	15.31	176	2809272	32.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	348024	23.62	ng/ul	0.00
70) Anthracene-d10	17.16	188	4689035	34.50	ng/ul	0.00
78) Pyrene-d10	19.46	212	5588181	36.38	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	5755395	35.78	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.77	163	273778	2.659	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
Data File : BN007839.D
Acq On : 24 Sep 2019 16:47
Operator : JU
Sample : K4985-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETJS1

Quant Time: Sep 24 17:32:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:15:33 2019
Response via : Initial Calibration

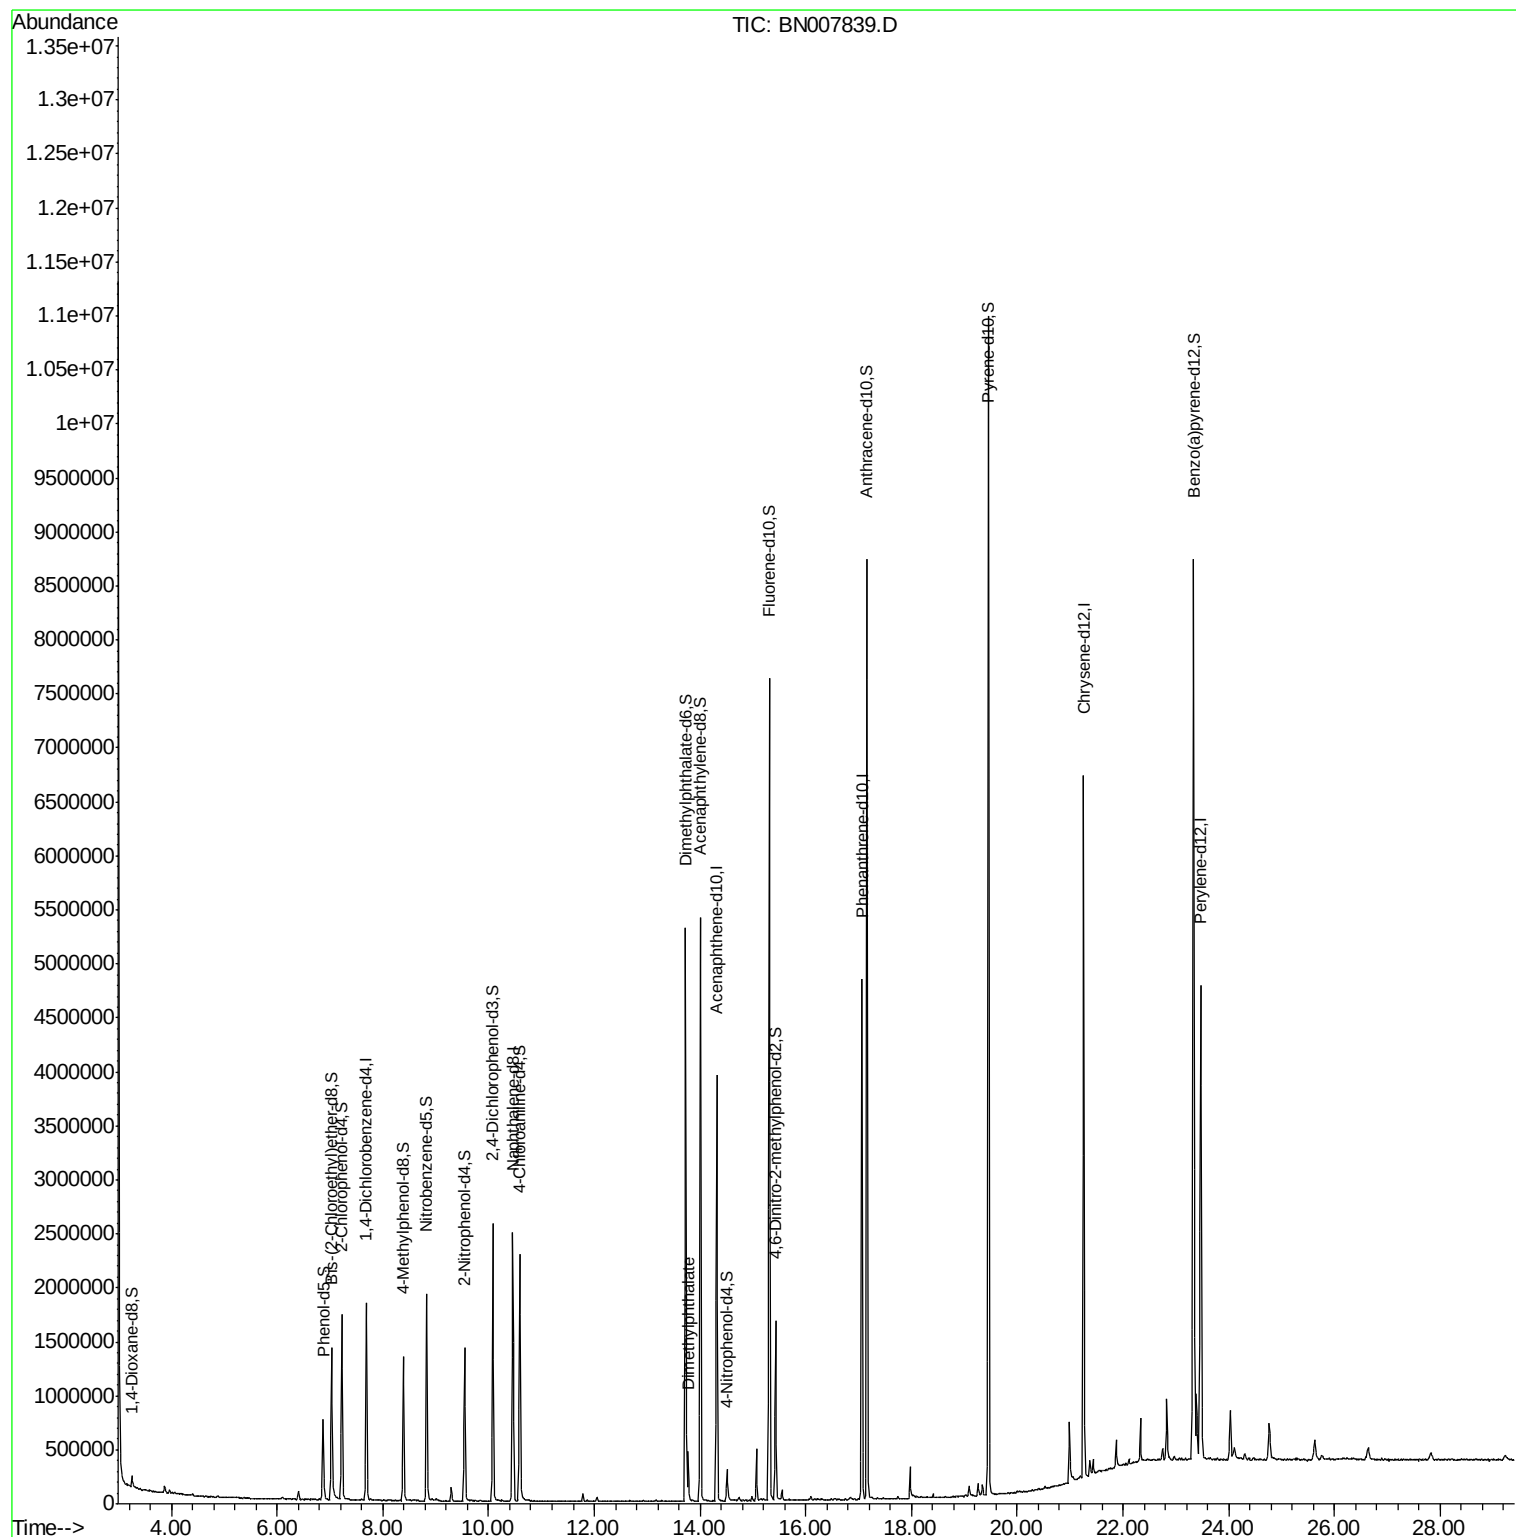

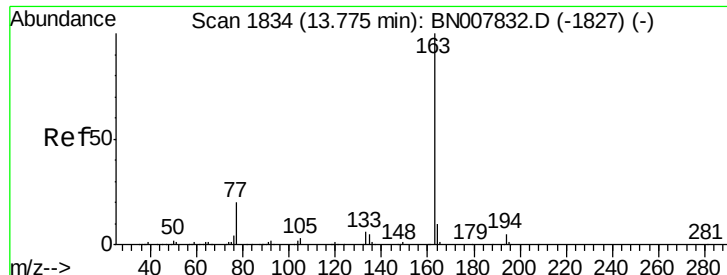

#44

Dimethylphthalate

Concen: 2.659 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.00 min

Lab File: BN007839.D

Acq: 24 Sep 2019 16:47

Instrument :

BNA_N

ClientSampleId :

ETJS1


Tot Ion:163 Resp: 273778

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 10.4 8.4 12.6

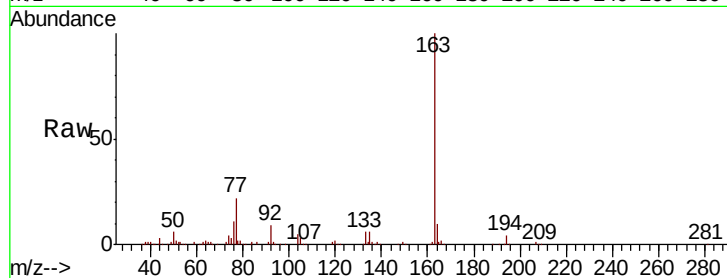

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

