

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
 Data File : BN007841.D
 Acq On : 24 Sep 2019 17:58
 Operator : JU
 Sample : K4985-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETJS3

Quant Time: Sep 24 18:34:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:15:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	574366	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	2358868	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	1530043	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	3250793	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	3350787	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	3625461	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	71149	4.71	ng/uL	0.00
5) Phenol-d5	6.86	99	398296	7.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	912820	29.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	973141	25.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	686693	16.48	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	561101	32.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	588556	36.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	1125286	29.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	99955	2.01	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	3839771	31.54	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	4321572	30.99	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	131926	6.09	ng/ul	0.00
57) Fluorene-d10	15.31	176	3313883	31.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	486339	27.72	ng/ul	0.00
70) Anthracene-d10	17.16	188	5332466	32.95	ng/ul	0.00
78) Pyrene-d10	19.46	212	6347405	35.17	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	6569039	34.82	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.78	163	179494	1.446	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092419\
Data File : BN007841.D
Acq On : 24 Sep 2019 17:58
Operator : JU
Sample : K4985-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETJS3

Quant Time: Sep 24 18:34:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:15:33 2019
Response via : Initial Calibration

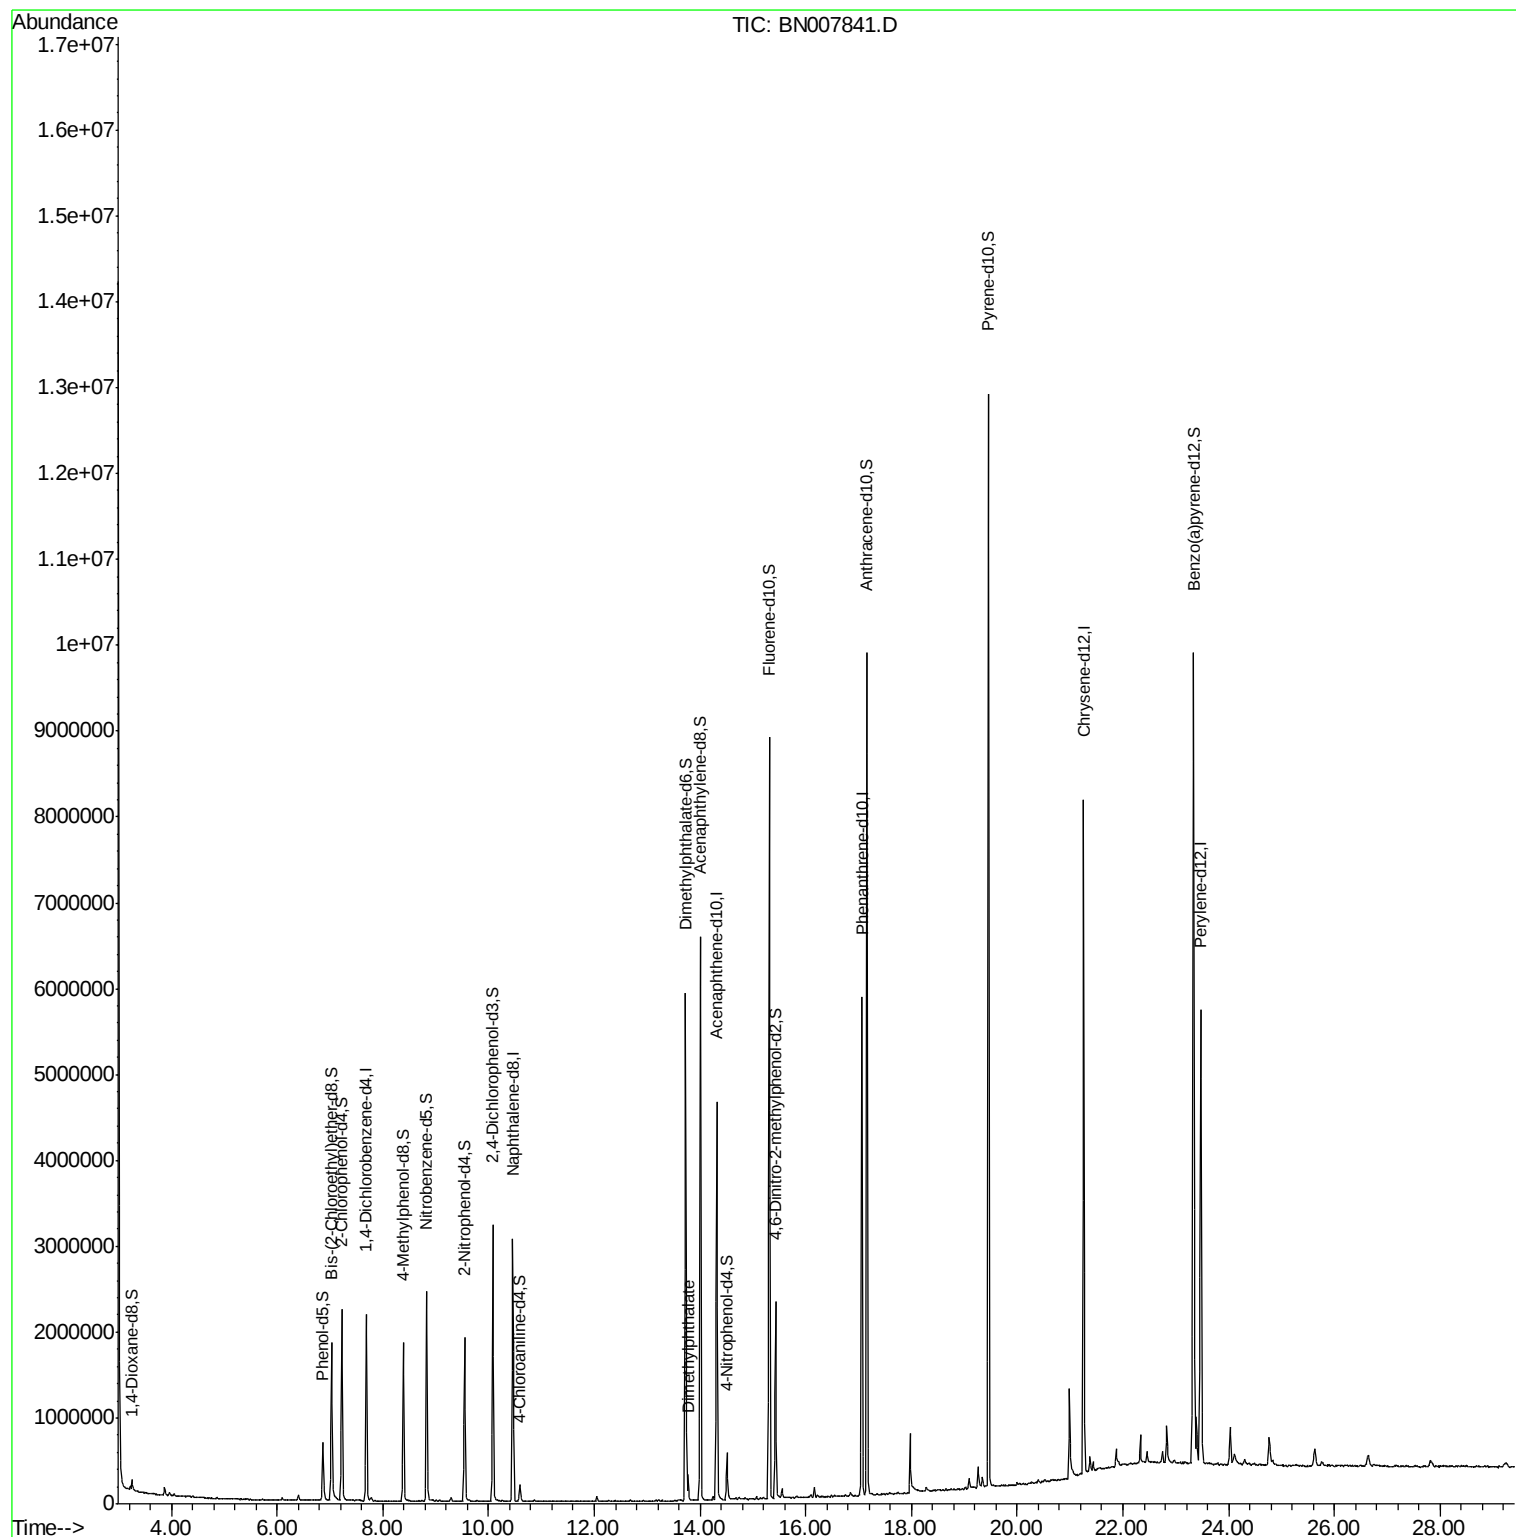

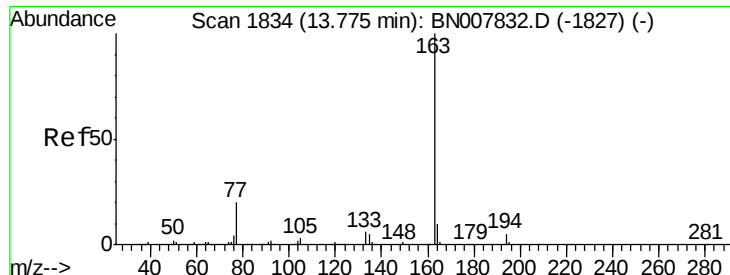

#44

Dimethylphthalate

Concen: 1.446 ng/ul

RT: 13.78 min Scan# 1834

Delta R.T. 0.00 min

Lab File: BN007841.D

Acq: 24 Sep 2019 17:58

Instrument :

BNA_N

ClientSampleId :

ETJS3


Tot Ion:163 Resp: 179494

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 10.9 8.4 12.6

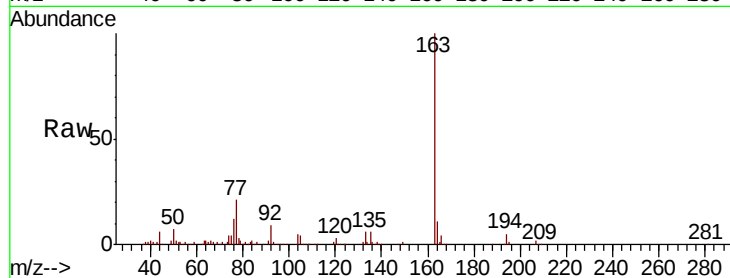

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

