

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
 Data File : BN016420.D
 Acq On : 23 Sep 2021 13:31
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Sep 23 16:03:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 16:03:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.670	152	22284	0.400	ng	0.00
7) Naphthalene-d8	10.432	136	94648	0.400	ng	#-0.01
13) Acenaphthene-d10	14.294	164	48152	0.400	ng	0.00
19) Phenanthrene-d10	17.042	188	90625	0.400	ng	# 0.00
29) Chrysene-d12	21.259	240	86698	0.400	ng	0.01
35) Perylene-d12	23.522	264	73299	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.282	112	19051	0.341	ng	0.00
5) Phenol-d6	6.849	99	22237	0.328	ng	0.00
8) Nitrobenzene-d5	8.810	82	22722	0.404	ng	0.00
11) 2-Methylnaphthalene-d10	12.034	152	52387	0.351	ng	0.00
14) 2,4,6-Tribromophenol	15.791	330	4372	0.309	ng	0.00
15) 2-Fluorobiphenyl	12.924	172	74319	0.394	ng	0.00
27) Fluoranthene-d10	19.088	212	91178	0.348	ng	0.00
31) Terphenyl-d14	19.703	244	79064	0.394	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	4403	0.475	ng	# 88
3) n-Nitrosodimethylamine	3.622	42	8519	0.402	ng	# 71
6) bis(2-Chloroethyl)ether	7.108	93	23300	0.386	ng	93
9) Naphthalene	10.483	128	94868	0.372	ng	99
10) Hexachlorobutadiene	10.774	225	18728	0.386	ng	# 99
12) 2-Methylnaphthalene	12.105	142	60629	0.359	ng	98
16) Acenaphthylene	14.015	152	68416	0.305	ng	99
17) Acenaphthene	14.358	154	50669	0.365	ng	99
18) Fluorene	15.347	166	60733	0.352	ng	99
20) 4,6-Dinitro-2-methylph...	15.436	198	2371	0.626	ng	# 65
21) 4-Bromophenyl-phenylether	16.251	248	19000	0.358	ng	99
22) Hexachlorobenzene	16.348	284	19490	0.389	ng	# 90
23) Atrazine	16.531	200	12056	0.248	ng	97
24) Pentachlorophenol	16.701	266	5553	0.329	ng	99
25) Phenanthrene	17.091	178	98774	0.386	ng	99
26) Anthracene	17.176	178	78478	0.316	ng	99
28) Fluoranthene	19.118	202	110859	0.376	ng	99
30) Pyrene	19.485	202	107865	0.393	ng	99
32) Benzo(a)anthracene	21.238	228	96173	0.345	ng	99
33) Chrysene	21.291	228	107273	0.398	ng	99
34) Bis(2-ethylhexyl)phtha...	21.196	149	27850	0.185	ng	98
36) Indeno(1,2,3-cd)pyrene	25.819	276	92472	0.391	ng	99
37) Benzo(b)fluoranthene	22.841	252	96803	0.416	ng	98
38) Benzo(k)fluoranthene	22.885	252	94127	0.420	ng	99
39) Benzo(a)pyrene	23.423	252	76560	0.364	ng	97
40) Dibenzo(a,h)anthracene	25.843	278	79632	0.396	ng	94
41) Benzo(g,h,i)perylene	26.521	276	81674	0.408	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
Data File : BN016420.D
Acq On : 23 Sep 2021 13:31
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Sep 23 16:03:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 16:03:09 2021
Response via : Initial Calibration

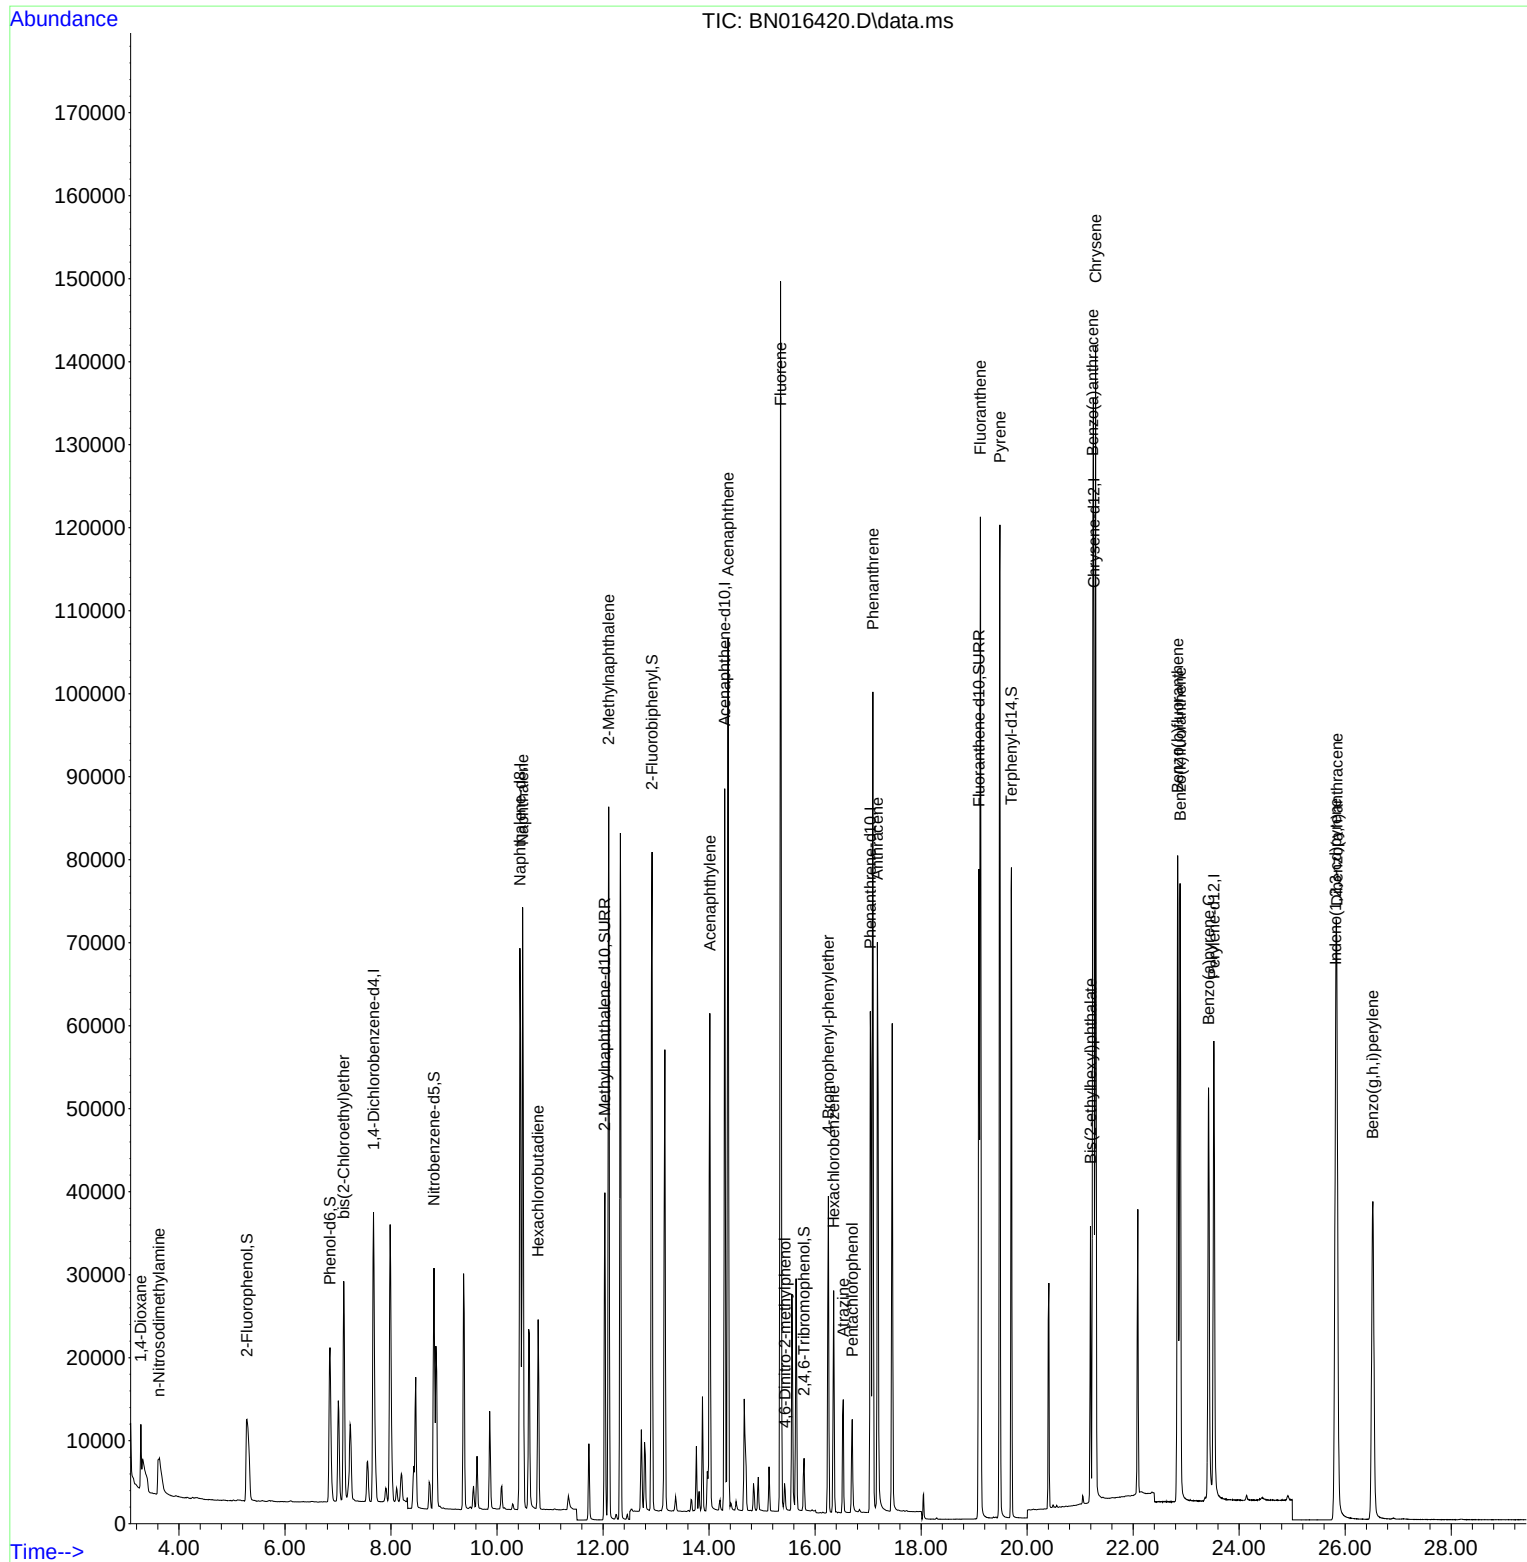







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.670 min Scan# 498
 Delta R.T. 0.000 min
 Lab File: BN016420.D
 Acq: 23 Sep 2021 13:31

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:152 Resp: 22284




Ion	Ratio	Lower	Upper
152	100		
150	154.5	125.6	188.4
115	57.0	50.2	75.2

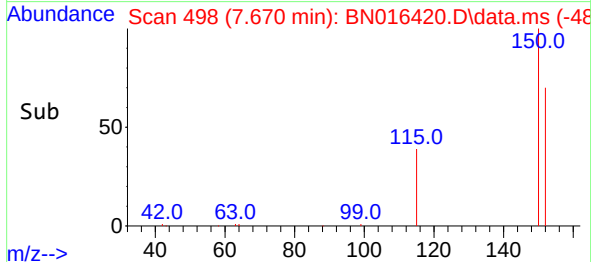


#2
 1,4-Dioxane
 Concen: 0.475 ng
 RT: 3.281 min Scan# 22
 Delta R.T. 0.000 min
 Lab File: BN016420.D
 Acq: 23 Sep 2021 13:31

Tgt Ion: 88 Resp: 4403

Ion	Ratio	Lower	Upper
88	100		
43	42.9	20.3	30.5
58	81.9	69.9	104.9


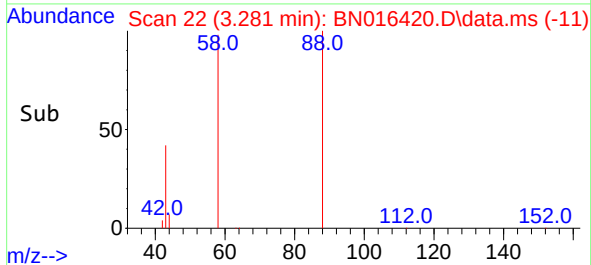

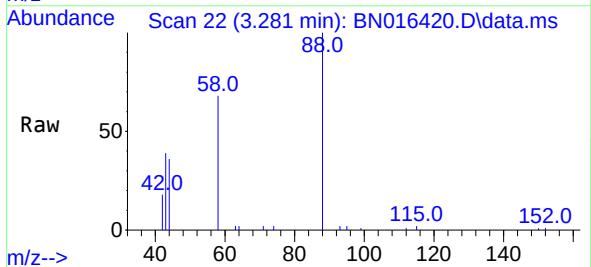


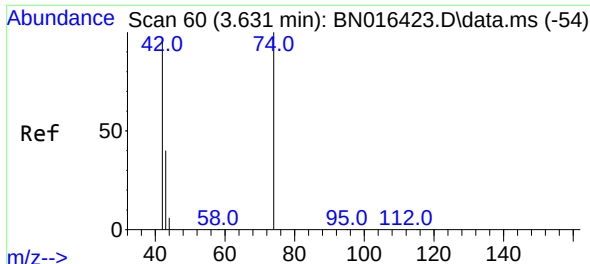

#3
n-Nitrosodimethylamine
Concen: 0.402 ng
RT: 3.622 min Scan# 59
Delta R.T. -0.009 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 8519
Ion Ratio Lower Upper
42 100
74 107.0 113.6 170.4#
44 5.5 0.0 0.0#



#4
2-Fluorophenol
Concen: 0.341 ng
RT: 5.282 min Scan# 239
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion: 112 Resp: 19051
Ion Ratio Lower Upper
112 100
64 62.6 47.3 70.9
63 32.7 23.4 35.0


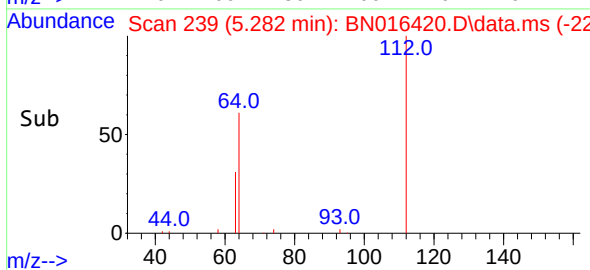

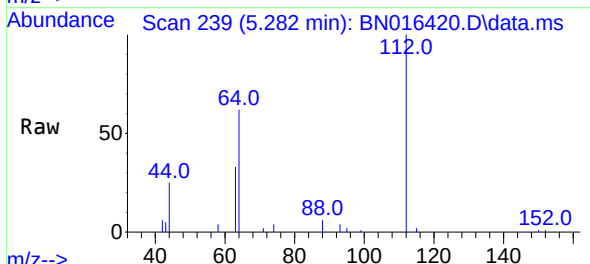




#5
Phenol-d6
Concen: 0.328 ng
RT: 6.849 min Scan# 409
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 22237
Ion Ratio Lower Upper
99 100
42 24.5 14.0 21.0#
71 31.3 23.8 35.6

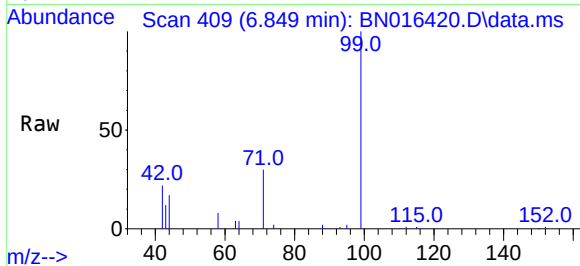

#6
bis(2-Chloroethyl)ether
Concen: 0.386 ng
RT: 7.108 min Scan# 437
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion: 93 Resp: 23300
Ion Ratio Lower Upper
93 100
63 87.3 63.4 95.0
95 32.9 26.8 40.2


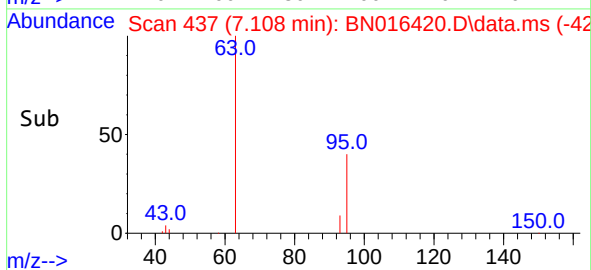

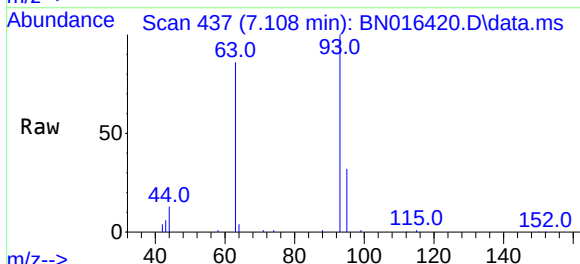




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.432 min Scan# 735
Delta R.T. -0.012 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	94648
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.8	13.2
54	11.5	5.3	7.9#
68	6.9	3.9	5.9#

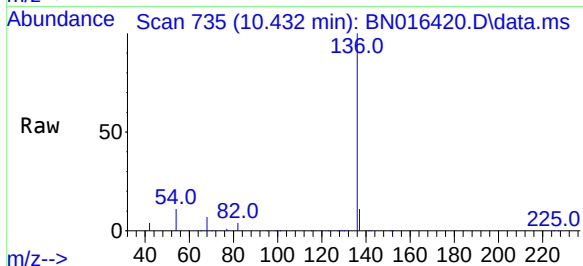

#8
Nitrobenzene-d5
Concen: 0.404 ng
RT: 8.810 min Scan# 607
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:	82	Resp:	22722
Ion Ratio	Lower	Upper	
82	100		
128	40.0	31.7	47.5
54	65.1	46.4	69.6




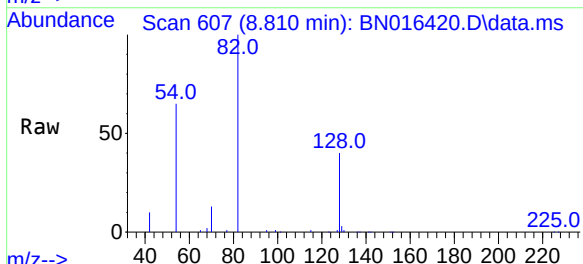




#9
Naphthalene
Concen: 0.372 ng
RT: 10.483 min Scan# 739
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	128	Resp:	94868
Ion	Ratio	Lower	Upper
128	100		
129	11.1	8.9	13.3
127	13.2	10.1	15.1

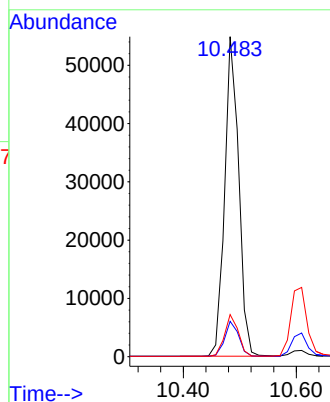

#10
Hexachlorobutadiene
Concen: 0.386 ng
RT: 10.774 min Scan# 762
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:	225	Resp:	18728
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.6	51.5	77.3


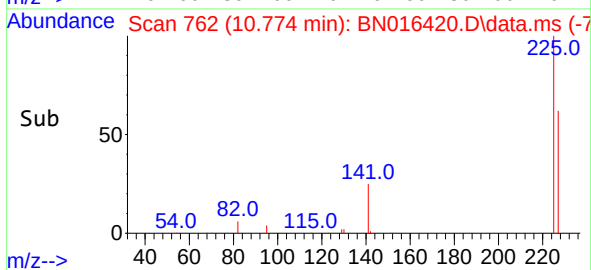
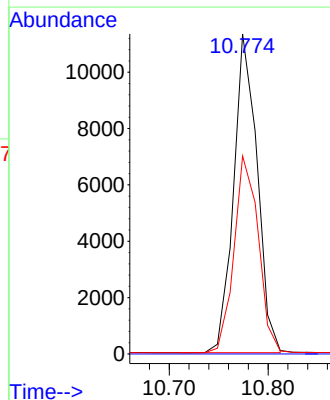



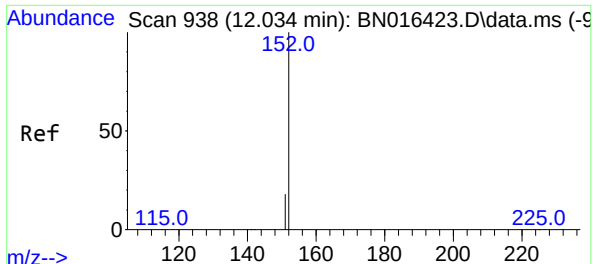

#11
2-Methylnaphthalene-d10
Concen: 0.351 ng
RT: 12.034 min Scan# 938
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 52387
Ion Ratio Lower Upper
152 100
151 20.3 16.1 24.1

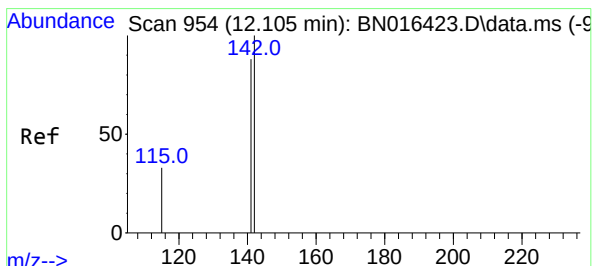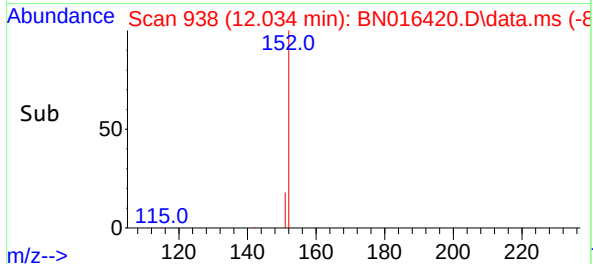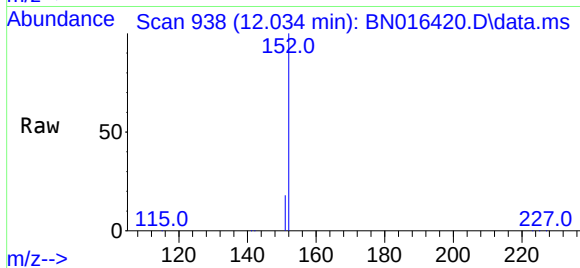

#12
2-Methylnaphthalene
Concen: 0.359 ng
RT: 12.105 min Scan# 954
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:142 Resp: 60629
Ion Ratio Lower Upper
142 100
141 88.4 69.8 104.8
115 33.4 24.4 36.6


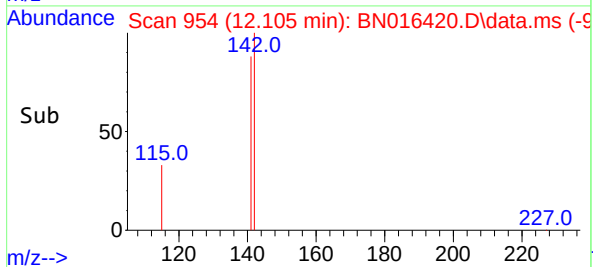

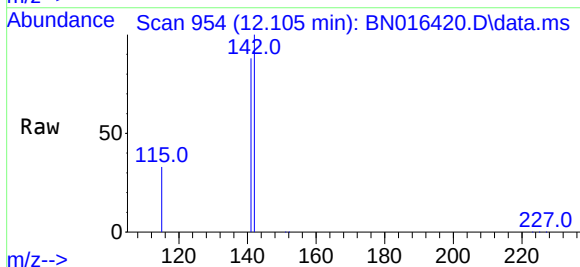




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.294 min Scan# 1185
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 48152
Ion Ratio Lower Upper
164 100
162 101.3 79.0 118.4
160 46.0 34.1 51.1

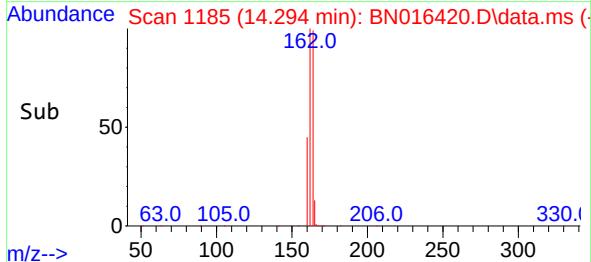

#14
2,4,6-Tribromophenol
Concen: 0.309 ng
RT: 15.791 min Scan# 1303
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:330 Resp: 4372
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 42.9 25.0 37.4#


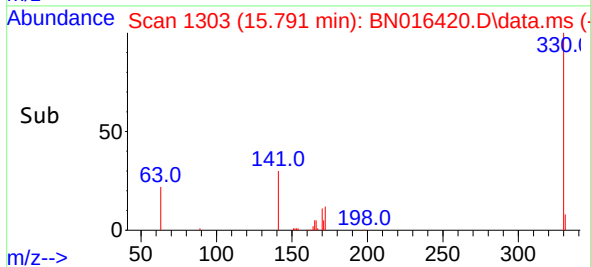

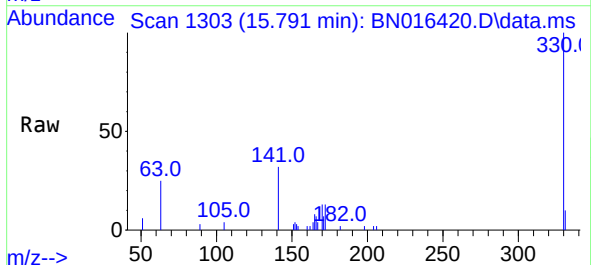




#15
2-Fluorobiphenyl
Concen: 0.394 ng
RT: 12.924 min Scan# 1077
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 74319
Ion Ratio Lower Upper
172 100
171 33.4 27.8 41.6
170 21.5 18.2 27.2

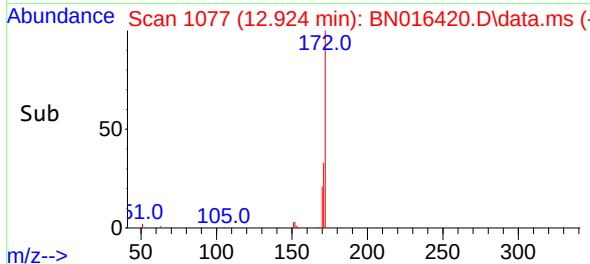

#16
Acenaphthylene
Concen: 0.305 ng
RT: 14.015 min Scan# 1163
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:152 Resp: 68416
Ion Ratio Lower Upper
152 100
151 19.4 15.2 22.8
153 13.0 10.5 15.7


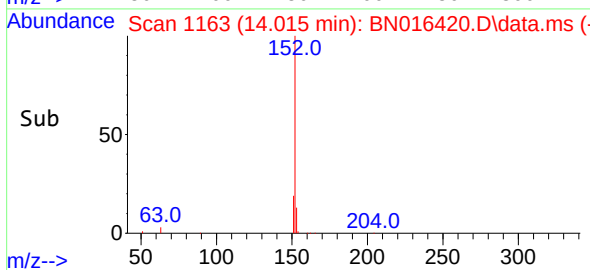

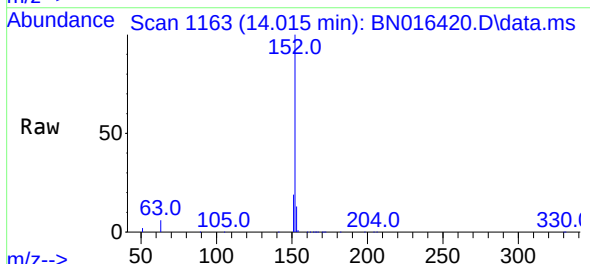




#17
Acenaphthene
Concen: 0.365 ng
RT: 14.358 min Scan# 1190
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 50669
Ion Ratio Lower Upper
154 100
153 111.6 89.3 133.9
152 54.5 42.2 63.4

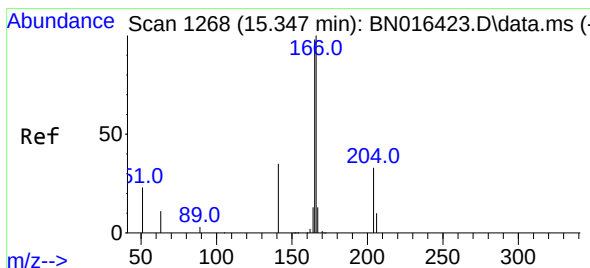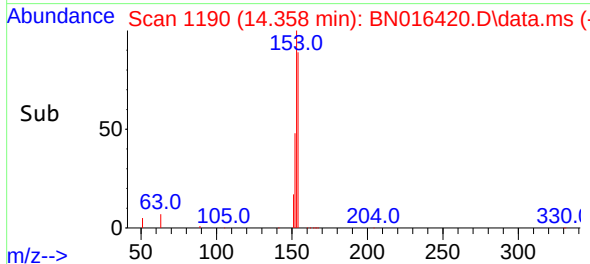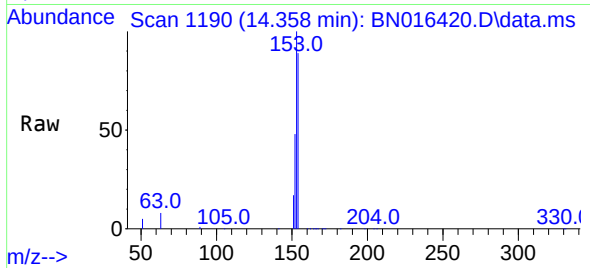

#18
Fluorene
Concen: 0.352 ng
RT: 15.347 min Scan# 1268
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:166 Resp: 60733
Ion Ratio Lower Upper
166 100
165 96.9 76.7 115.1
167 13.5 10.9 16.3


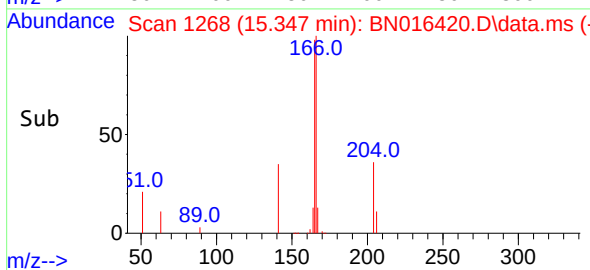

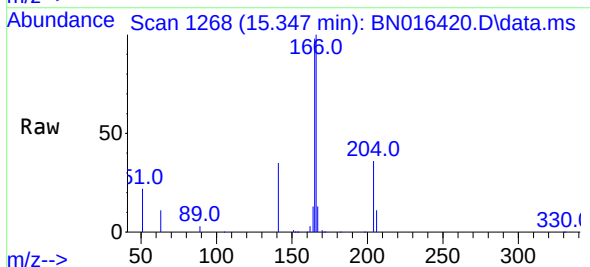




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.042 min Scan# 1405
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 90625
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.3 7.0 10.6#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.626 ng
RT: 15.436 min Scan# 1275
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:198 Resp: 2371
Ion Ratio Lower Upper
198 100
182 13.2 26.6 39.8#
77 0.0 0.0 0.0



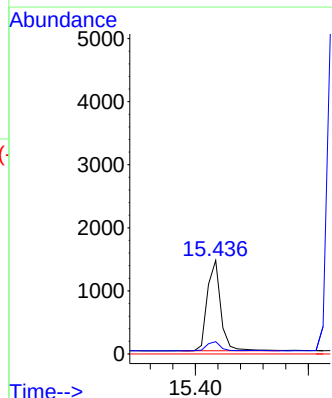





#21
4-Bromophenyl-phenylether
Concen: 0.358 ng
RT: 16.251 min Scan# 1340
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	248	Resp:	19000
Ion	Ratio	Lower	Upper
248	100		
250	100.0	80.5	120.7
141	45.5	34.8	52.2



#22
Hexachlorobenzene
Concen: 0.389 ng
RT: 16.348 min Scan# 1348
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:	284	Resp:	19490
Ion	Ratio	Lower	Upper
284	100		
142	37.0	22.6	34.0#
249	32.2	24.4	36.6


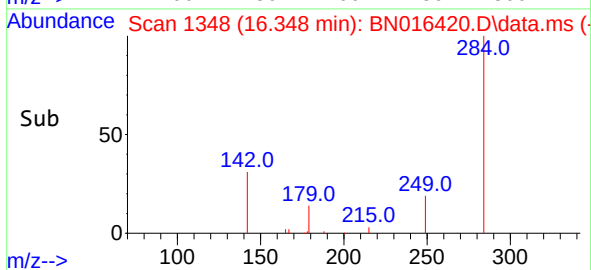






#23
Atrazine
Concen: 0.248 ng
RT: 16.531 min Scan# 1363
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 12056
Ion Ratio Lower Upper
200 100
173 20.9 18.7 28.1
215 50.8 41.6 62.4

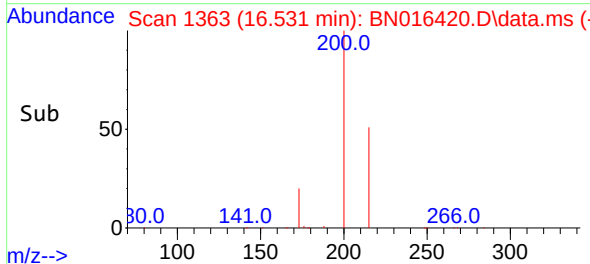

#24
Pentachlorophenol
Concen: 0.329 ng
RT: 16.701 min Scan# 1377
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:266 Resp: 5553
Ion Ratio Lower Upper
266 100
264 63.7 50.6 75.8
268 64.7 52.6 79.0


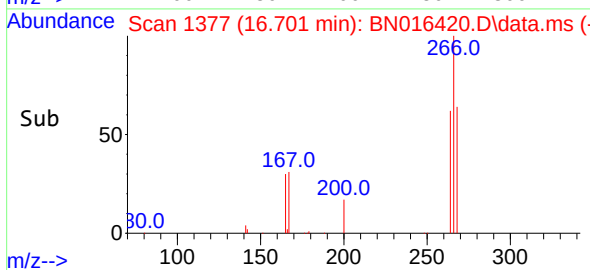

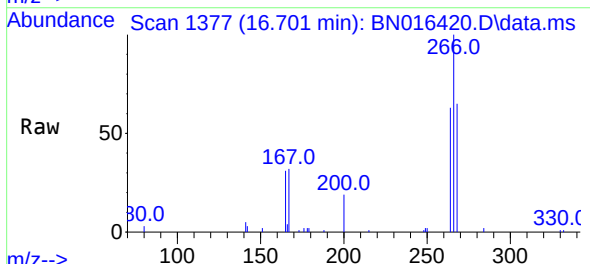




#25
Phenanthrene
Concen: 0.386 ng
RT: 17.091 min Scan# 1409
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 98774
Ion Ratio Lower Upper
178 100
176 18.7 14.4 21.6
179 15.5 12.2 18.4

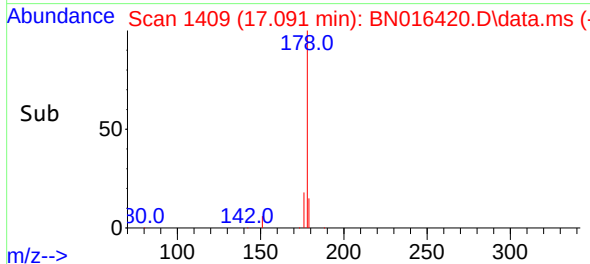

#26
Anthracene
Concen: 0.316 ng
RT: 17.176 min Scan# 1416
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:178 Resp: 78478
Ion Ratio Lower Upper
178 100
176 18.2 13.9 20.9
179 15.2 12.2 18.4


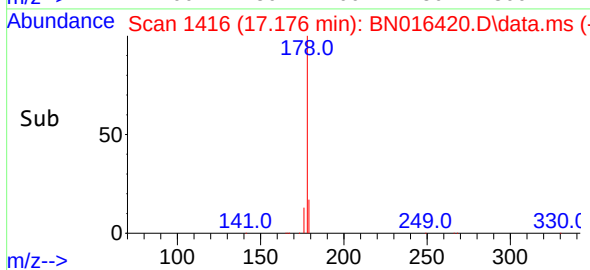

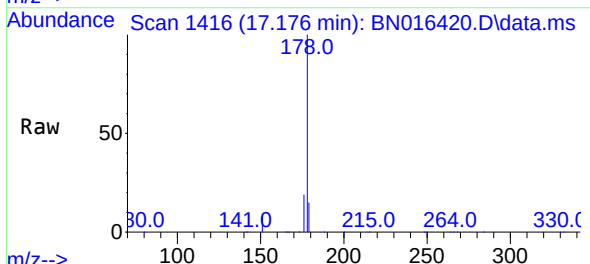




#27
Fluoranthene-d10
Concen: 0.348 ng
RT: 19.088 min Scan# 1701
Delta R.T. -0.005 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 91178
Ion Ratio Lower Upper
212 100
106 11.1 9.8 14.6
104 6.2 5.4 8.2

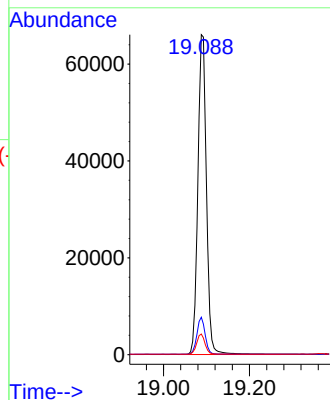

#28
Fluoranthene
Concen: 0.376 ng
RT: 19.118 min Scan# 1707
Delta R.T. -0.005 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:202 Resp: 110859
Ion Ratio Lower Upper
202 100
101 9.8 8.5 12.7
203 17.3 13.8 20.8



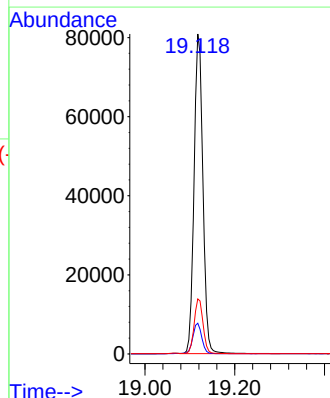





#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.259 min Scan# 2004
Delta R.T. 0.011 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 86698
Ion Ratio Lower Upper
240 100
120 5.7 5.3 7.9
236 25.6 19.8 29.8



#30
Pyrene
Concen: 0.393 ng
RT: 19.485 min Scan# 1781
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:202 Resp: 107865
Ion Ratio Lower Upper
202 100
200 20.5 15.8 23.6
203 17.4 13.9 20.9


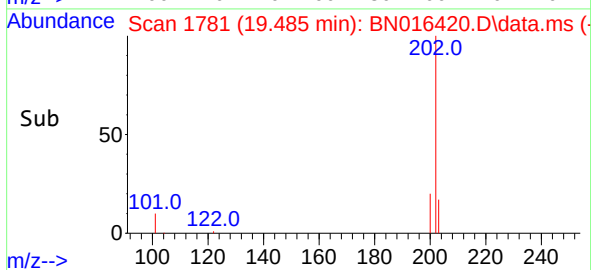




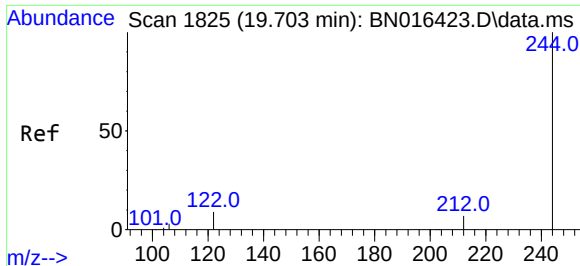

#31
Terphenyl-d14
Concen: 0.394 ng
RT: 19.703 min Scan# 1825
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 79064
Ion Ratio Lower Upper
244 100
212 7.2 5.5 8.3
122 9.5 9.0 13.4

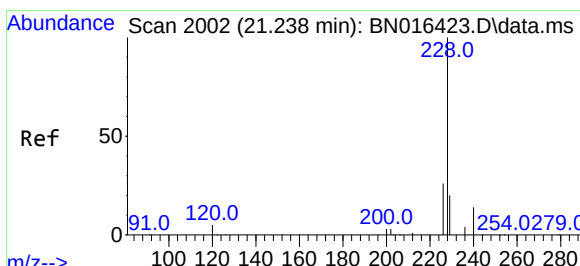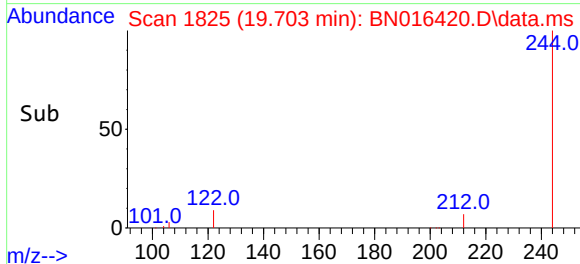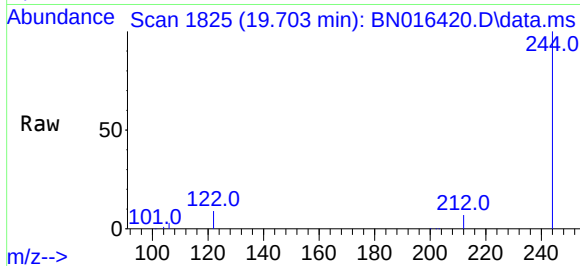

#32
Benzo(a)anthracene
Concen: 0.345 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:228 Resp: 96173
Ion Ratio Lower Upper
228 100
226 27.1 20.8 31.2
229 19.5 15.8 23.6

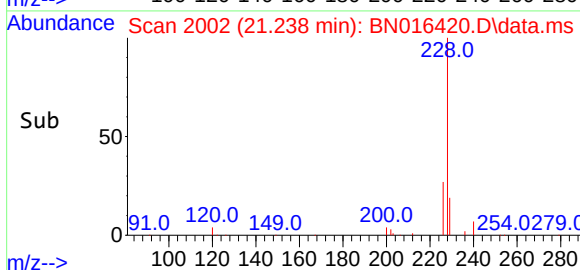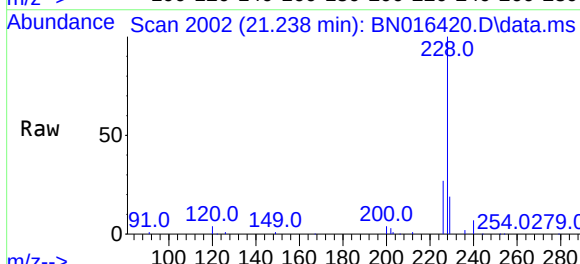




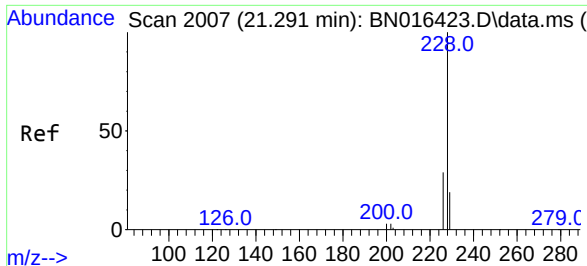


#33
Chrysene
Concen: 0.398 ng
RT: 21.291 min Scan# 2007
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:228 Resp: 107273




Ion	Ratio	Lower	Upper
228	100		
226	29.8	23.0	34.4
229	19.5	15.6	23.4

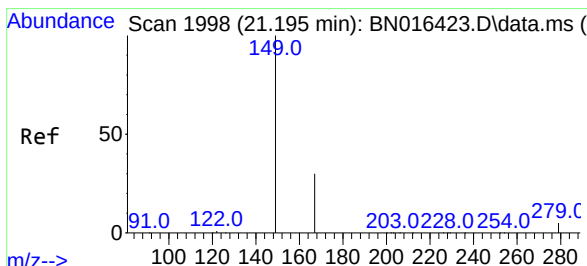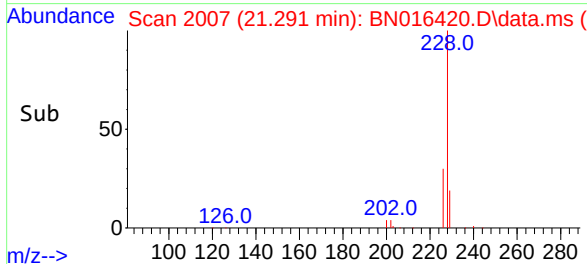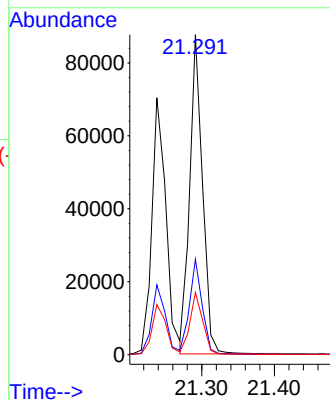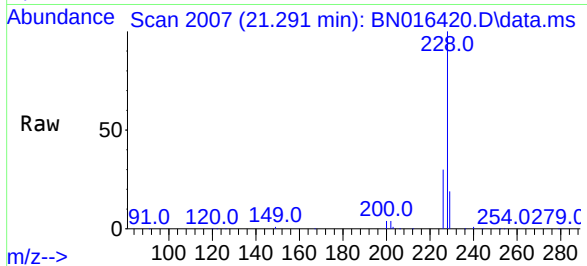


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.185 ng
RT: 21.196 min Scan# 1998
Delta R.T. 0.000 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Tgt Ion:149 Resp: 27850


Ion	Ratio	Lower	Upper
149	100		
167	27.9	23.4	35.0
279	4.3	3.9	5.9

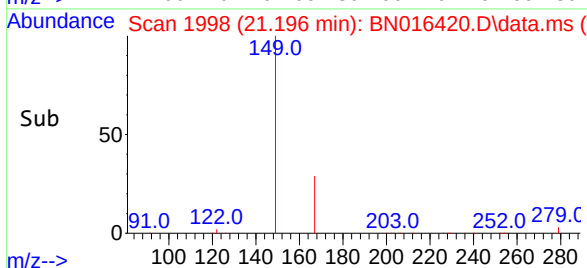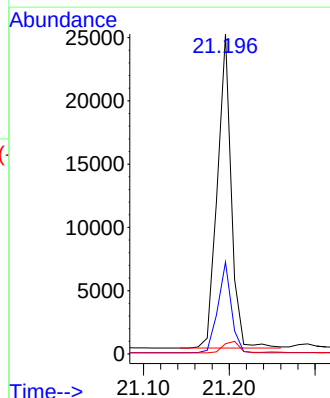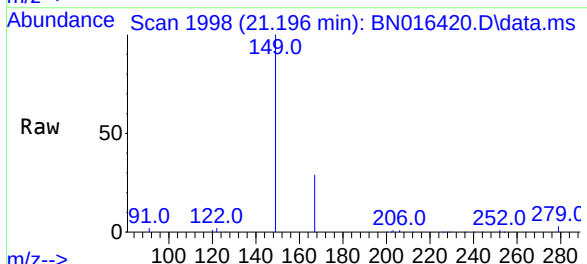






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.522 min Scan# 2438
Delta R.T. 0.004 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:264 Resp: 73299
Ion Ratio Lower Upper
264 100
260 24.8 18.9 28.3
265 25.4 23.7 35.5

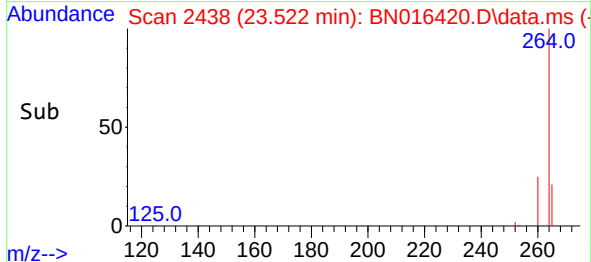

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.391 ng
RT: 25.819 min Scan# 3109
Delta R.T. 0.004 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31


Tgt Ion:276 Resp: 92472
Ion Ratio Lower Upper
276 100
138 22.8 19.3 28.9
277 25.1 20.2 30.2

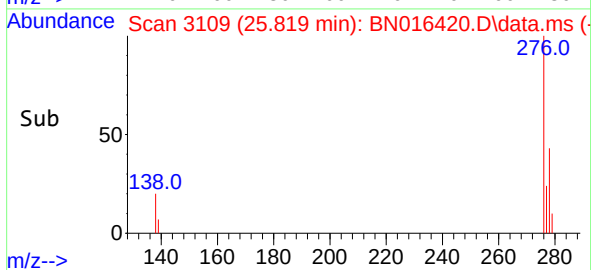





#37
Benzo(b)fluoranthene
Concen: 0.416 ng
RT: 22.841 min Scan# 2239
Delta R.T. 0.004 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4





Tgt Ion:252 Resp: 96803
Ion Ratio Lower Upper
252 100
253 22.2 18.2 27.2
125 9.1 8.4 12.6




#38
Benzo(k)fluoranthene
Concen: 0.420 ng
RT: 22.885 min Scan# 2252
Delta R.T. 0.004 min
Lab File: BN016420.D
Acq: 23 Sep 2021 13:31

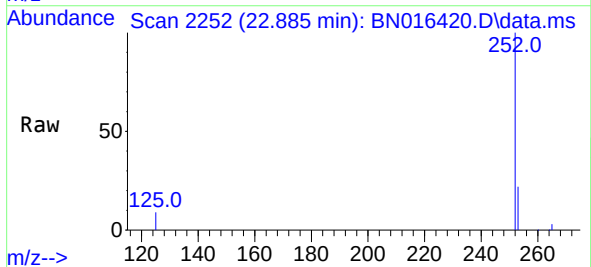

Tgt Ion:252 Resp: 94127
Ion Ratio Lower Upper
252 100
253 22.3 18.2 27.2
125 9.4 8.2 12.4

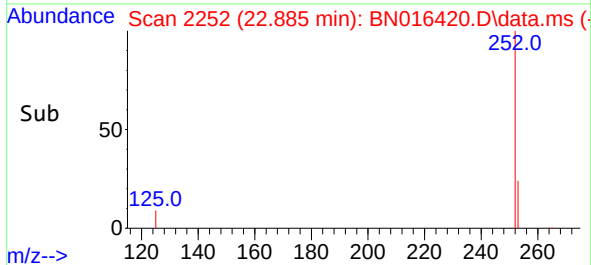



#39

Benzo(a)pyrene

Concen: 0.364 ng

RT: 23.423 min Scan# 2409

Delta R.T. 0.004 min

Lab File: BN016420.D

Acq: 23 Sep 2021 13:31





Tgt Ion:252	Resp:	76560
Ion Ratio	Lower	Upper
252	100	
253	22.5	18.7 28.1
125	10.3	9.9 14.9

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4

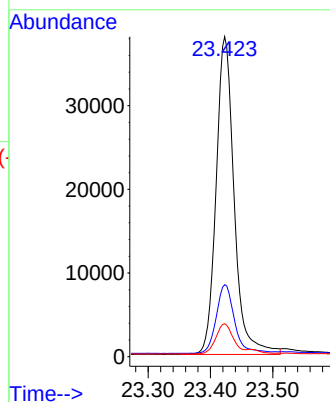

#40

Dibenzo(a,h)anthracene

Concen: 0.396 ng




RT: 25.843 min Scan# 3116


Delta R.T. 0.007 min

Lab File: BN016420.D

Acq: 23 Sep 2021 13:31

Tgt Ion:278	Resp:	79632
Ion Ratio	Lower	Upper
278	100	
139	14.7	14.2 21.2
279	23.7	21.3 31.9

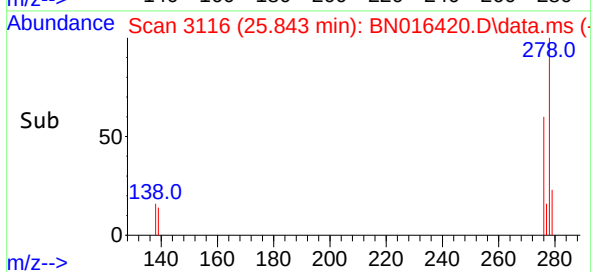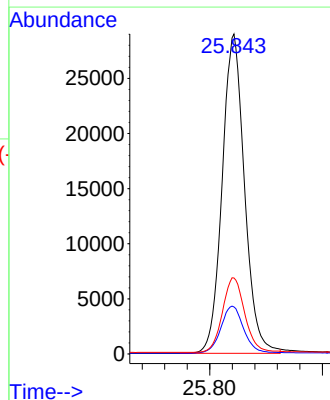

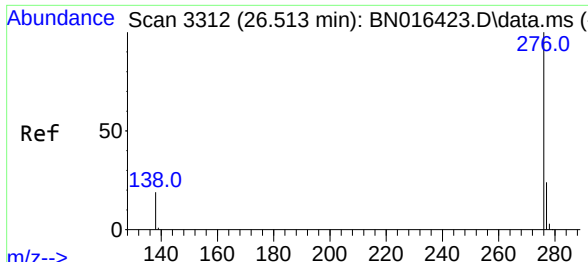

#41
 Benzo(g,h,i)perylene
 Concen: 0.408 ng
 RT: 26.521 min Scan# 3314
 Delta R.T. 0.007 min
 Lab File: BN016420.D
 Acq: 23 Sep 2021 13:31

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	276	Resp:	81674
Ion	Ratio	Lower	Upper
276	100		
277	24.1	20.5	30.7
138	19.4	18.2	27.4

