
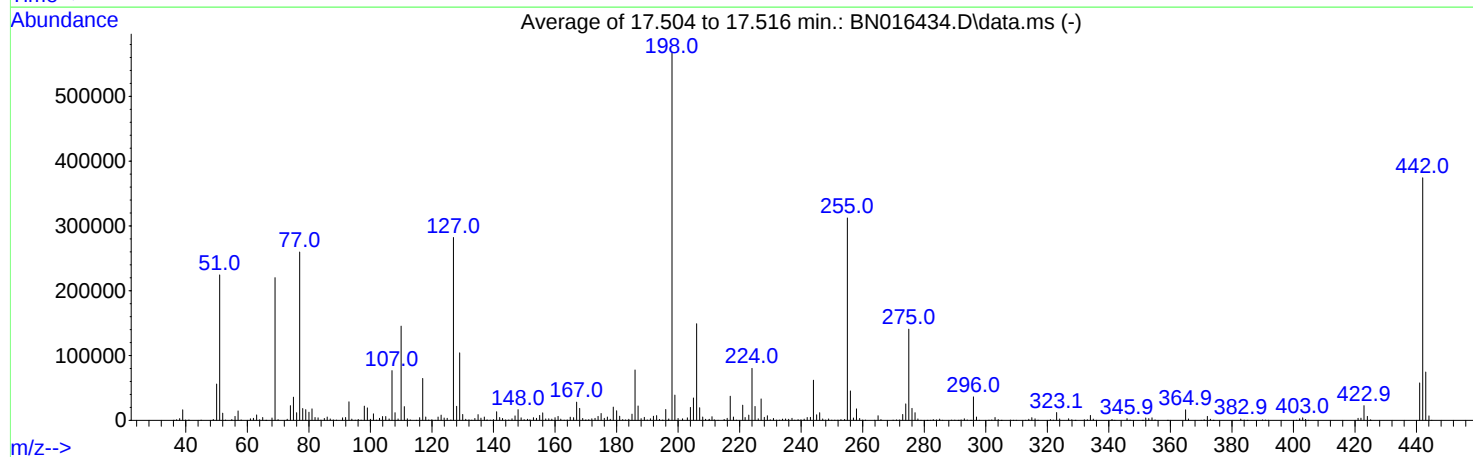


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
 Data File : BN016434.D
 Acq On : 24 Sep 2021 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 03:35:41 2021

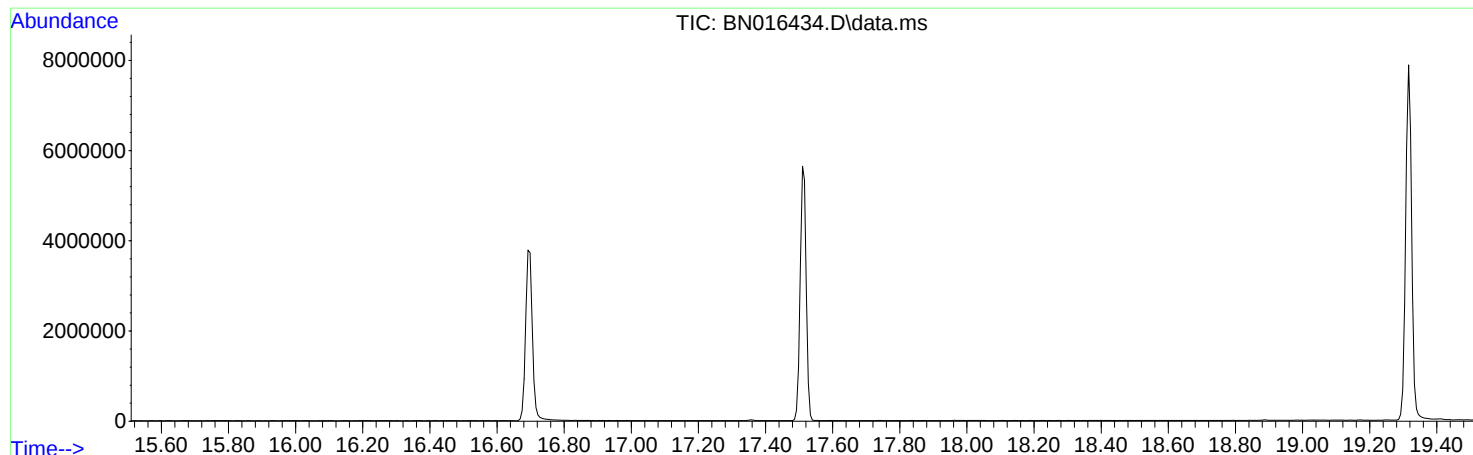




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	224555	PASS
68	69	0.00	2	1.7	3751	PASS
69	198	0.00	100	38.8	220203	PASS
70	69	0.00	2	0.5	1178	PASS
127	198	10	80	49.7	282155	PASS
197	198	0.00	2	0.4	2262	PASS
198	198	100	100	100.0	567659	PASS
199	198	5	9	6.9	39147	PASS
275	198	10	60	24.8	140725	PASS
365	198	1	100	2.9	16294	PASS
441	198	0.01	100	10.2	57829	PASS
442	442	50	100	100.0	374443	PASS
443	442	15	24	19.9	74675	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
 Data File : BN016434.D
 Acq On : 24 Sep 2021 10:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 11:28:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 13:04:53 2021
 Response via : Initial Calibration

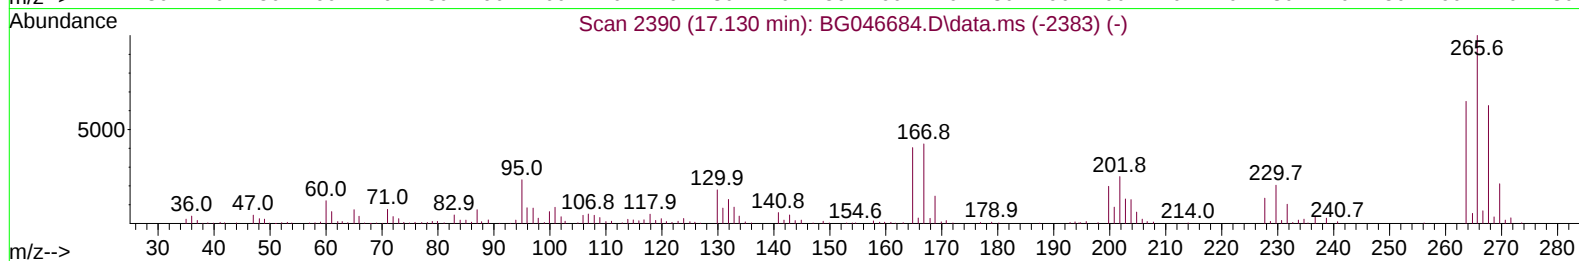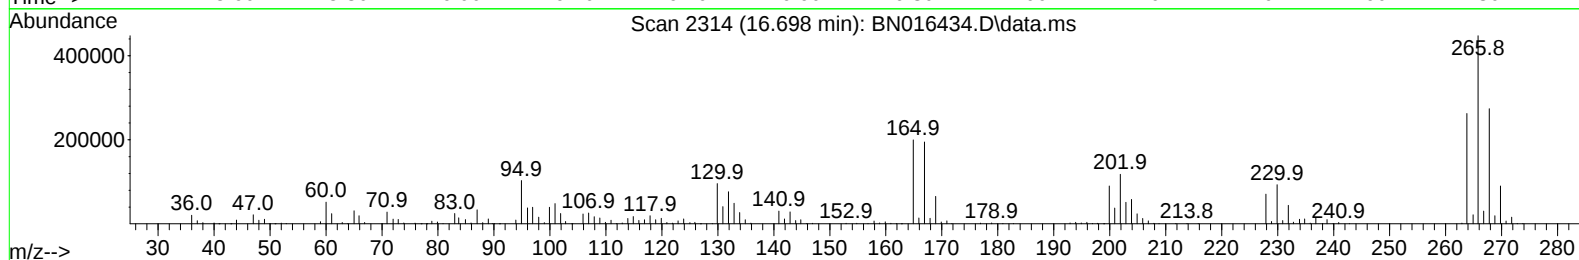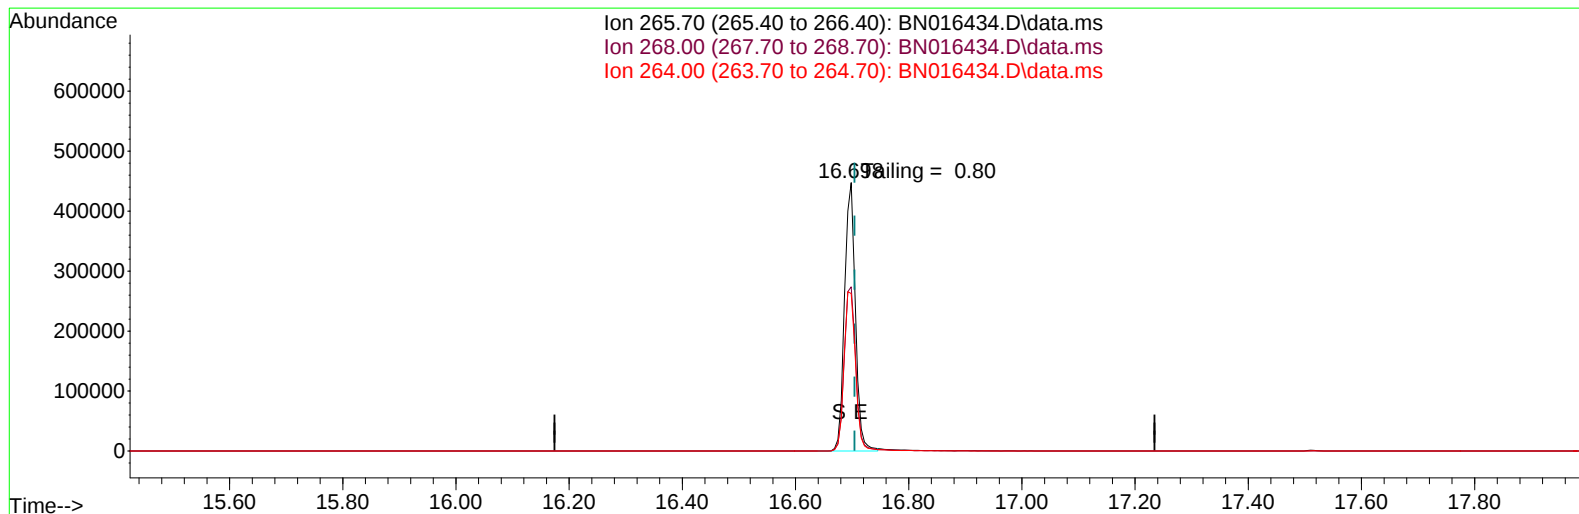

TIC: BN016434.D\data.ms

(70) Pentachlorophenol (C)

16.698min (-0.006) 21366.07 ng




response 607153

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.19
264.00	61.60	58.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
Data File : BN016434.D
Acq On : 24 Sep 2021 10:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 24 11:28:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 13:04:53 2021
Response via : Initial Calibration

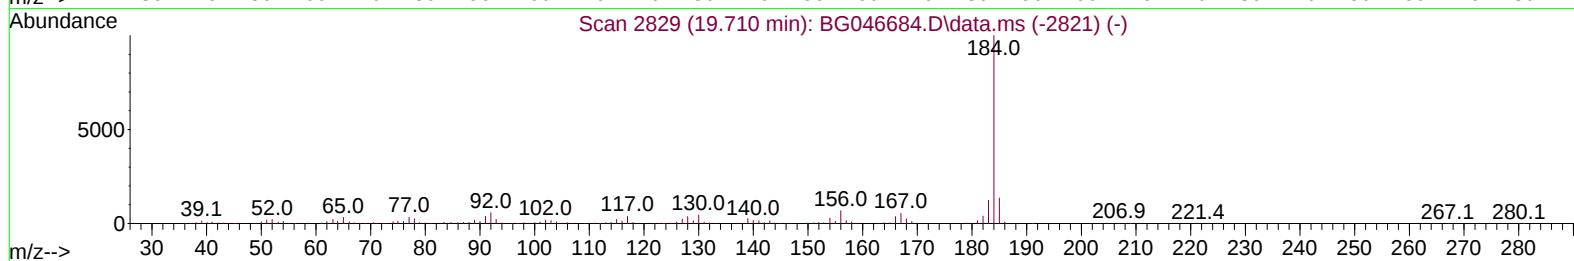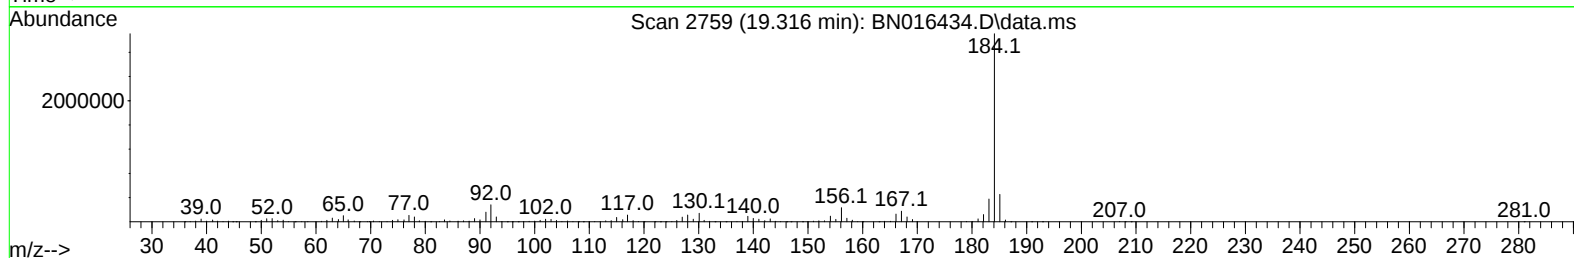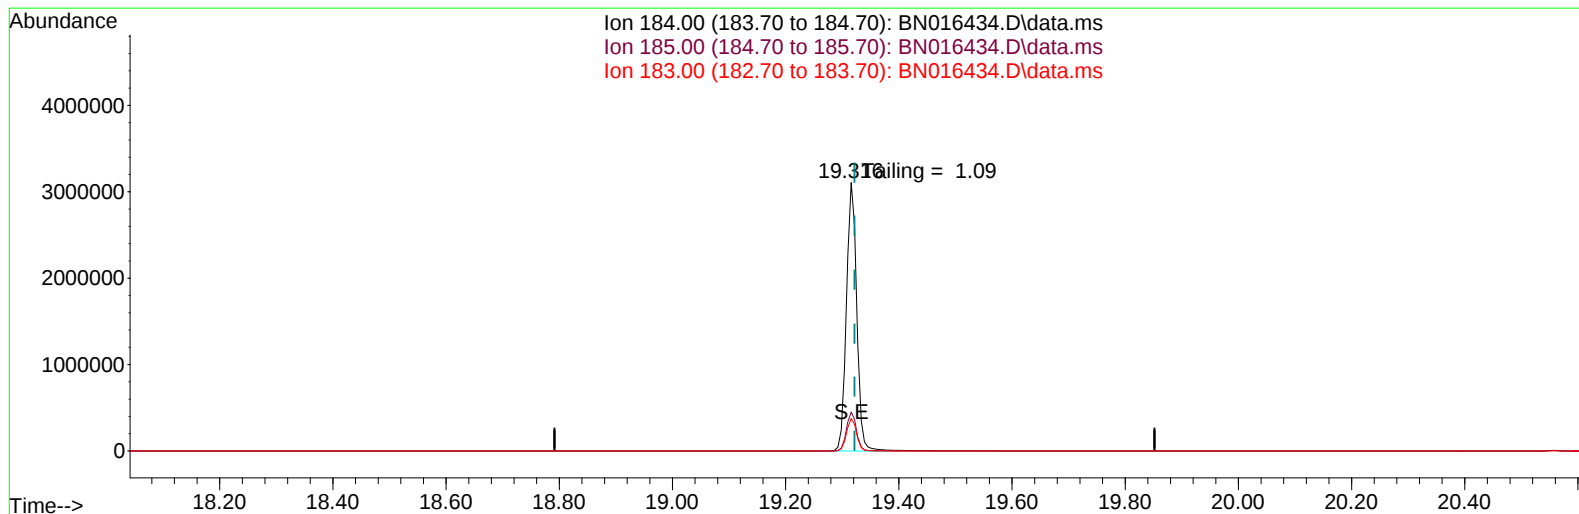

TIC: BN016434.D\data.ms

(77) Benzidine

19.316min (-0.006) 0.00 ng

response 3955260

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.53
183.00	13.20	12.13
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/24/2021	BNA_N	<u>BN016434.D</u>
Compound Name	Response	Retention Time
DDT	1842883	20.55
DDD	10430	20.11
DDE	2267	19.6
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12697	1855580	0.68

Instrument :
BNA_N
ClientSampleId :
DFTPP