
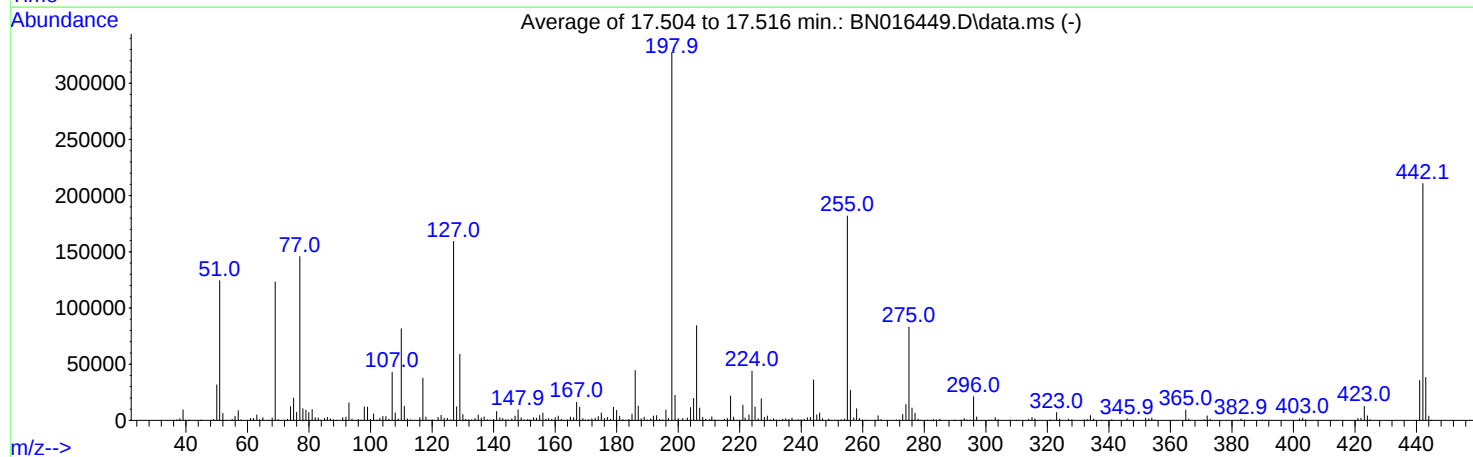


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
 Data File : BN016449.D
 Acq On : 24 Sep 2021 23:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 03:35:41 2021

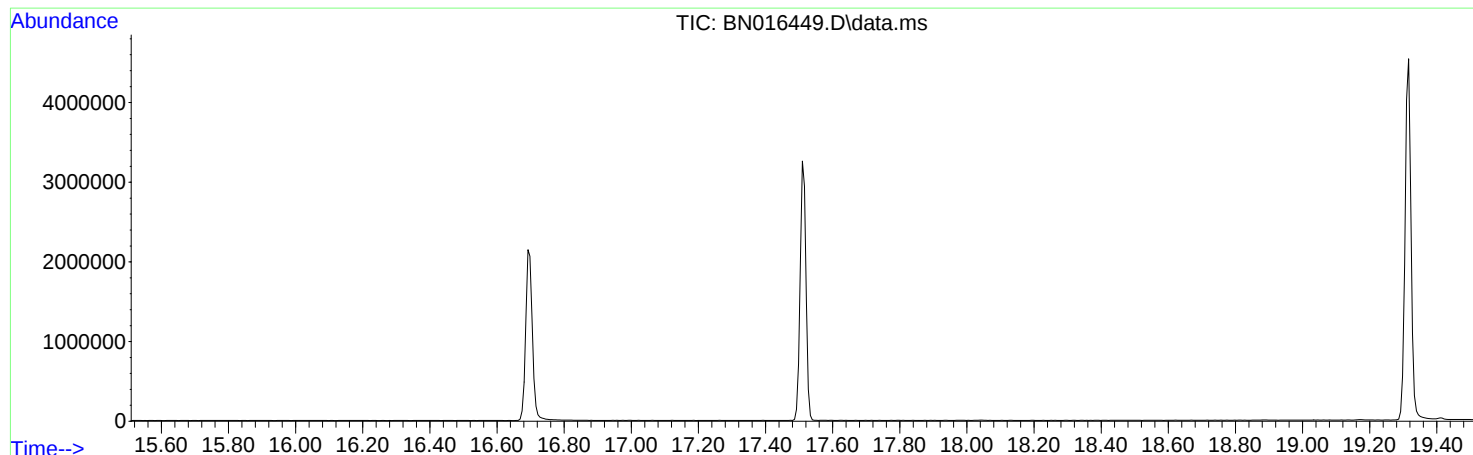




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	124375	PASS
68	69	0.00	2	1.7	2123	PASS
69	198	0.00	100	37.6	123125	PASS
70	69	0.00	2	0.6	727	PASS
127	198	10	80	48.6	159179	PASS
197	198	0.00	2	0.5	1665	PASS
198	198	100	100	100.0	327360	PASS
199	198	5	9	6.8	22419	PASS
275	198	10	60	25.4	83067	PASS
365	198	1	100	2.8	9170	PASS
441	198	0.01	100	10.8	35501	PASS
442	442	50	100	100.0	210717	PASS
443	442	15	24	18.1	38181	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
Data File : BN016449.D
Acq On : 24 Sep 2021 23:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 25 06:18:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 13:04:53 2021
Response via : Initial Calibration

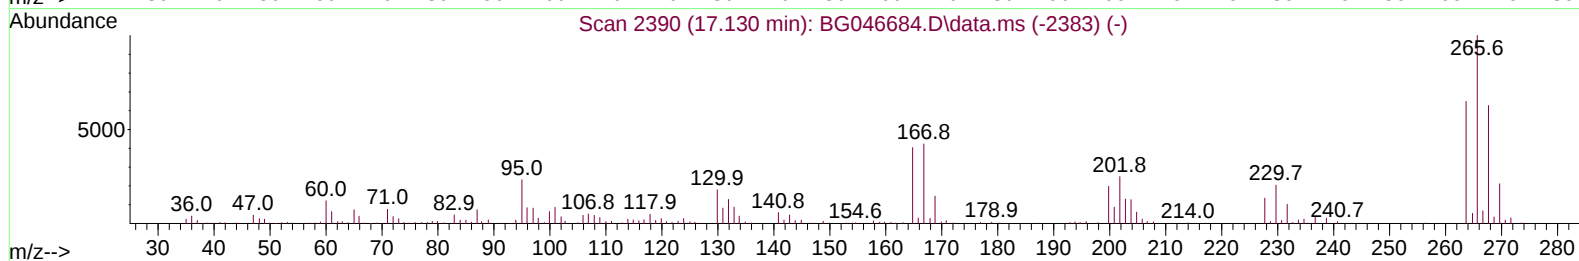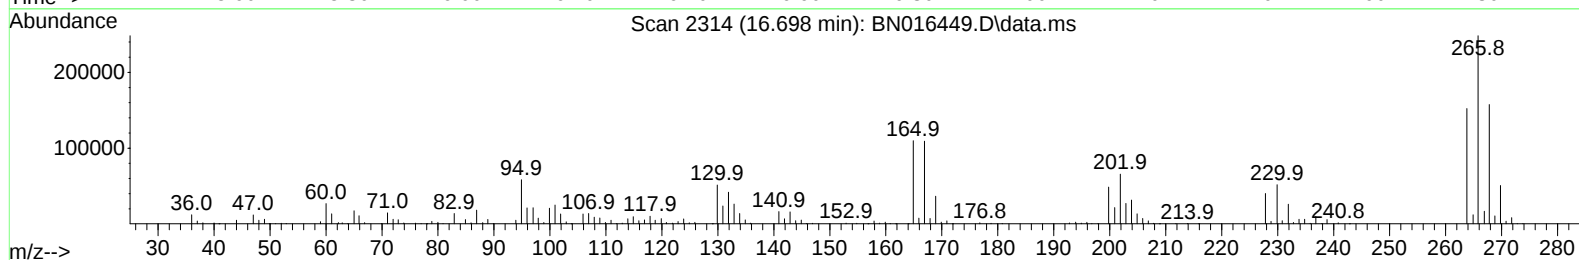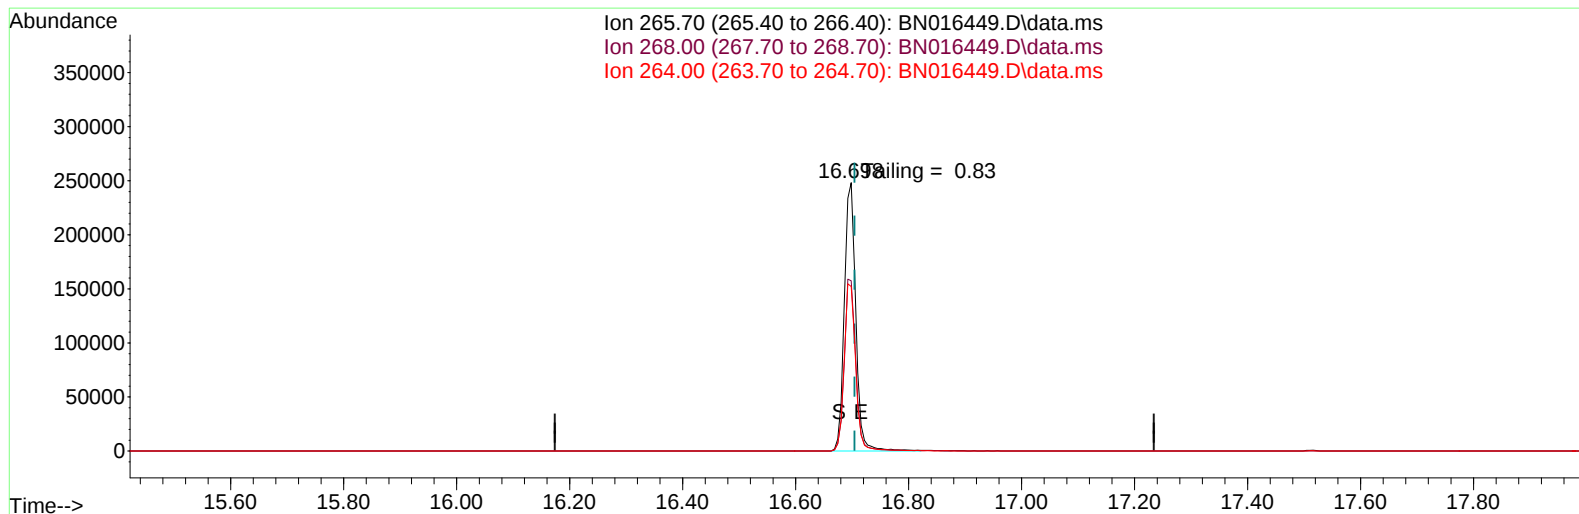

TIC: BN016449.D\data.ms

(70) Pentachlorophenol (C)

16.698min (-0.006) 22911.78 ng




response 350082

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.44
264.00	61.60	61.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092421\
Data File : BN016449.D
Acq On : 24 Sep 2021 23:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 25 06:18:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 13:04:53 2021
Response via : Initial Calibration

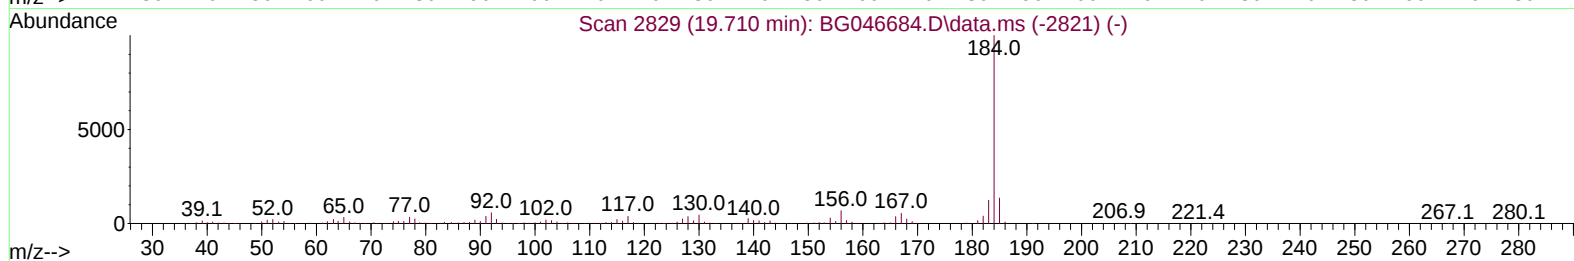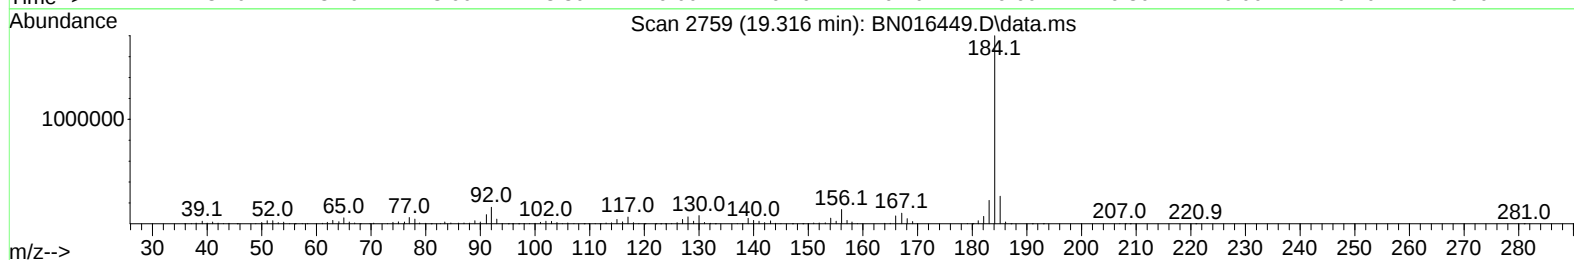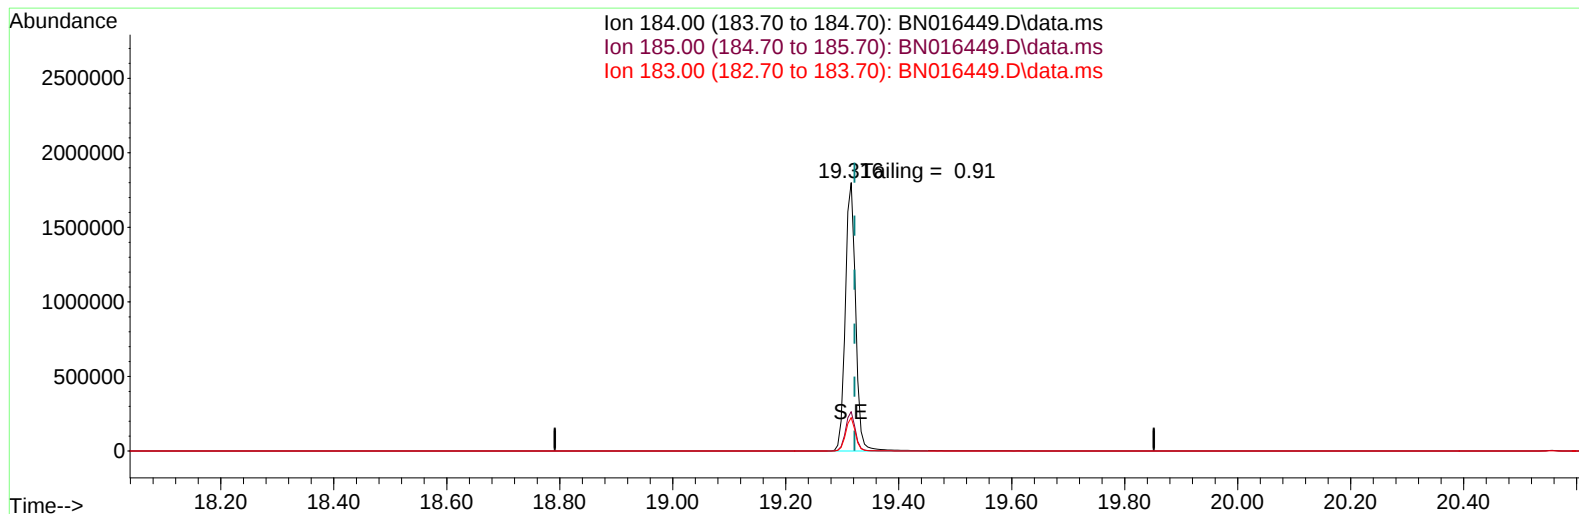

TIC: BN016449.D\data.ms

(77) Benzidine

19.316min (-0.006) 0.00 ng

response 2282766

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.67
183.00	13.20	12.46
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/24/2021	BNA_N	<u>BN016449.D</u>
Compound Name	Response	Retention Time
DDT	1043888	20.557
DDD	27023	20.116
DDE	763	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27786	1071674	2.59

Instrument :
BNA_N
ClientSampleId :
DFTPP