

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
 Data File : BN034173.D
 Acq On : 23 Sep 2024 20:27
 Operator : RC/JU
 Sample : PB163503BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK503

Quant Time: Sep 24 01:50:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 23 19:39:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.423	152	6805	0.400	ng/ul	0.00
4) Naphthalene-d8	10.179	136	20164	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.074	164	11873	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.928	188	1337932	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.05
23) Perylene-d12	23.165	264	14748	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.039	96	37464	5.355	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.785	152	7231	0.250	ng/ul	0.00
18) Fluoranthene-d10	18.870	212	13452	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.078	166	2636	0.061	ng/ul#	14
26) Benzo(a)pyrene	23.033	252	3461	0.075	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034173.D
Acq On : 23 Sep 2024 20:27
Operator : RC/JU
Sample : PB163503BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK503

Quant Time: Sep 24 01:50:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration




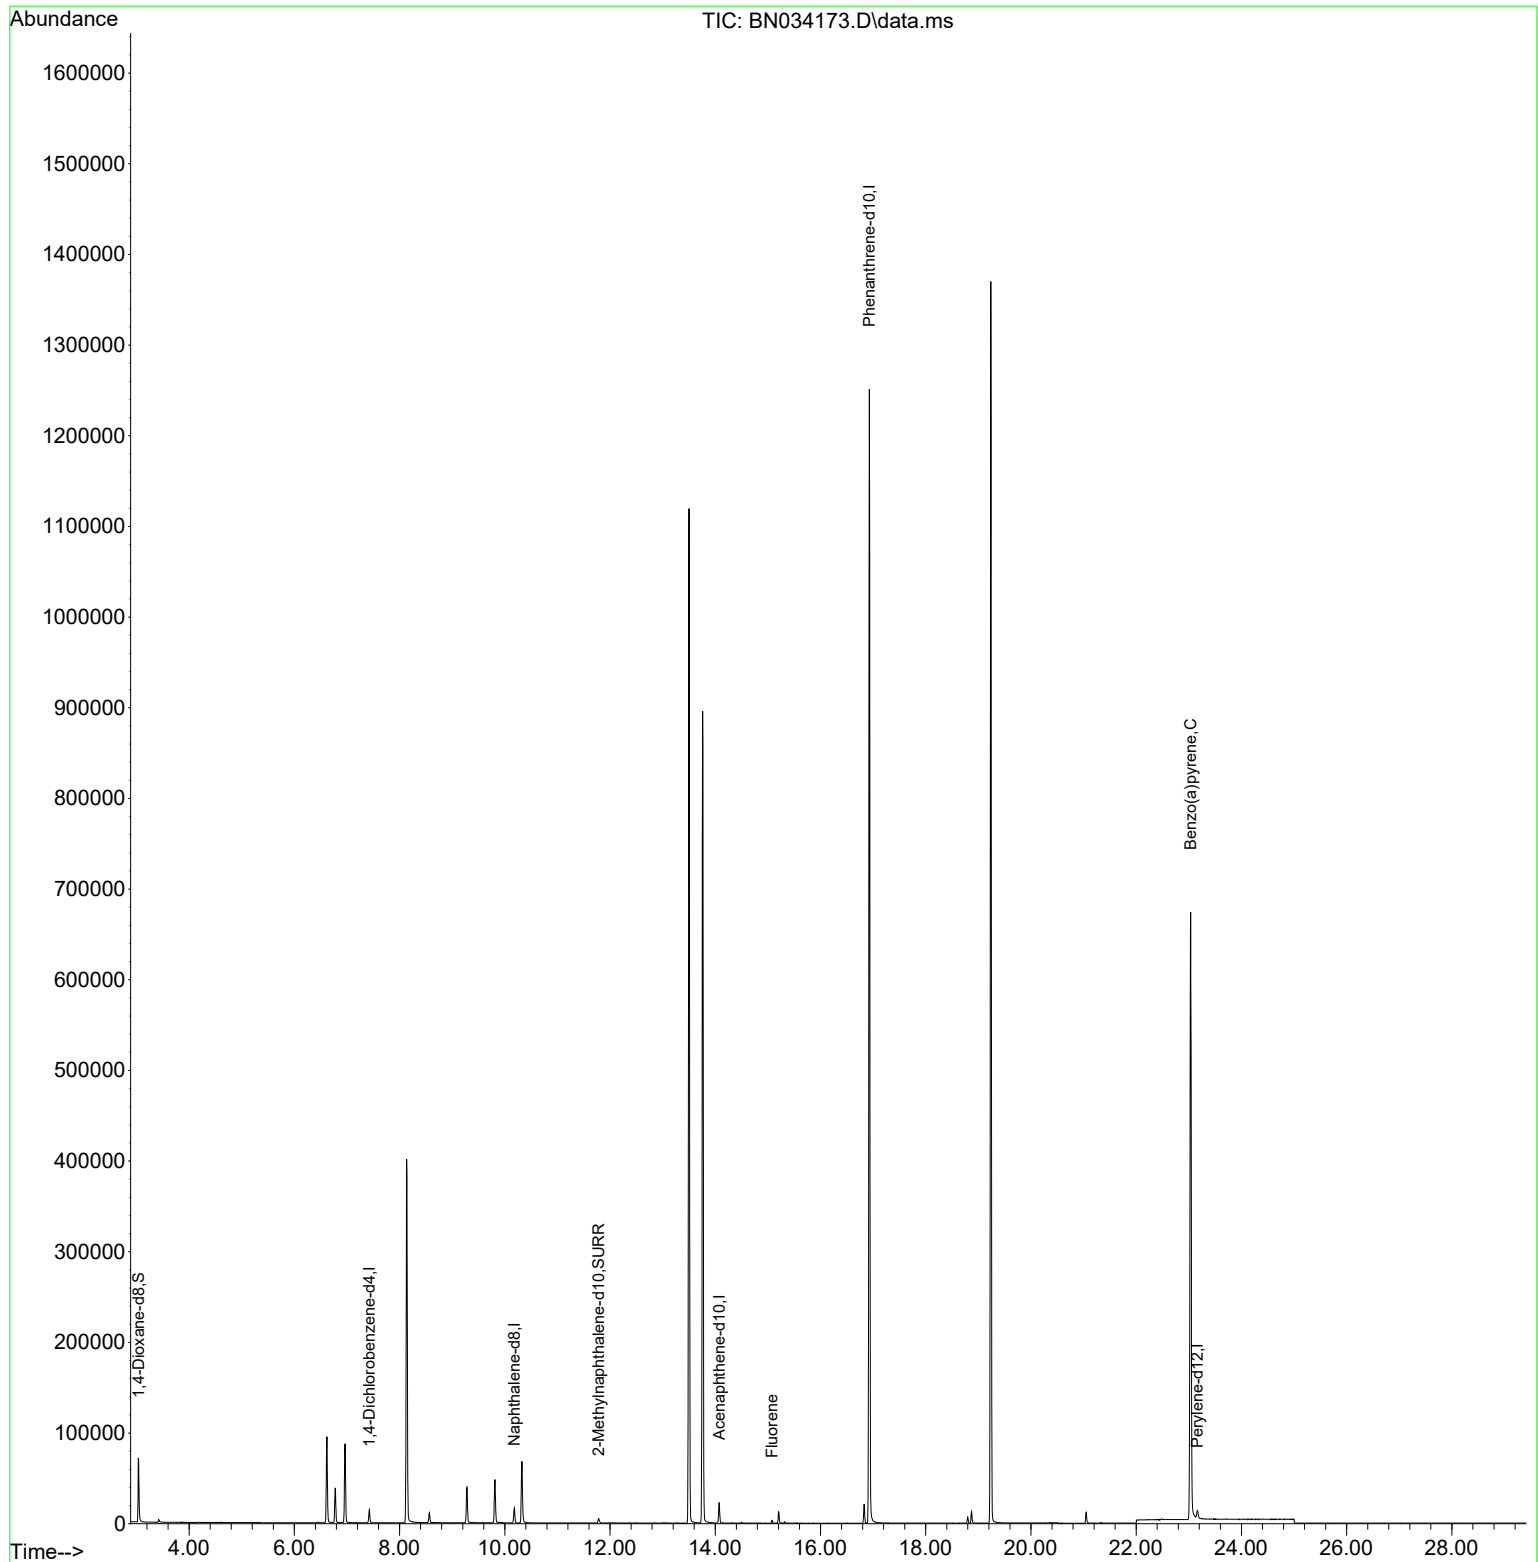


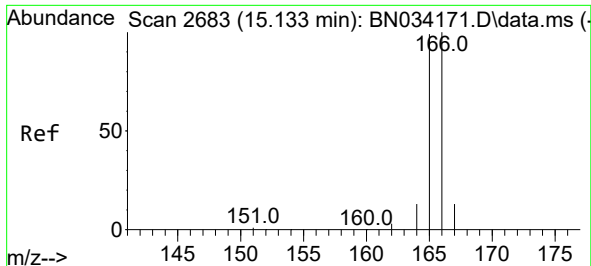

#12
Fluorene
Concen: 0.061 ng/ul
RT: 15.078 min Scan# 2683
Delta R.T. -0.056 min
Lab File: BN034173.D
Acq: 23 Sep 2024 20:27

Instrument :
BNA_N
ClientSampleId :
SBLK503

Tgt Ion:166 Resp: 2636
Ion Ratio Lower Upper
166 100
165 6.8 79.1 118.7#
167 31.8 11.4 17.0#

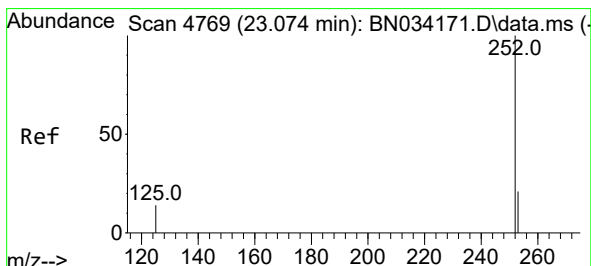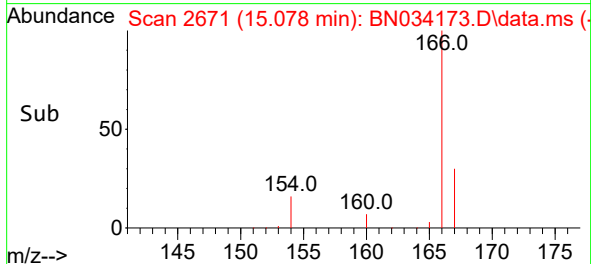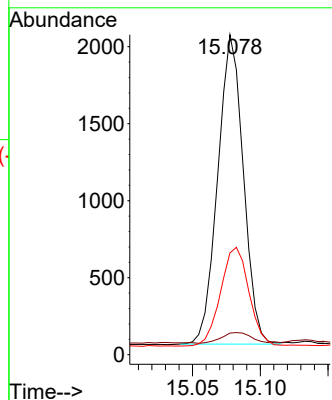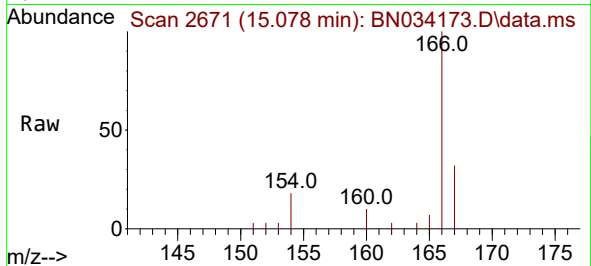

#26
Benzo(a)pyrene
Concen: 0.075 ng/ul
RT: 23.033 min Scan# 4755
Delta R.T. -0.041 min
Lab File: BN034173.D
Acq: 23 Sep 2024 20:27

Tgt Ion:252 Resp: 3461
Ion Ratio Lower Upper
252 100
253 49.5 22.8 34.2#
125 51.5 18.0 27.0#

