




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

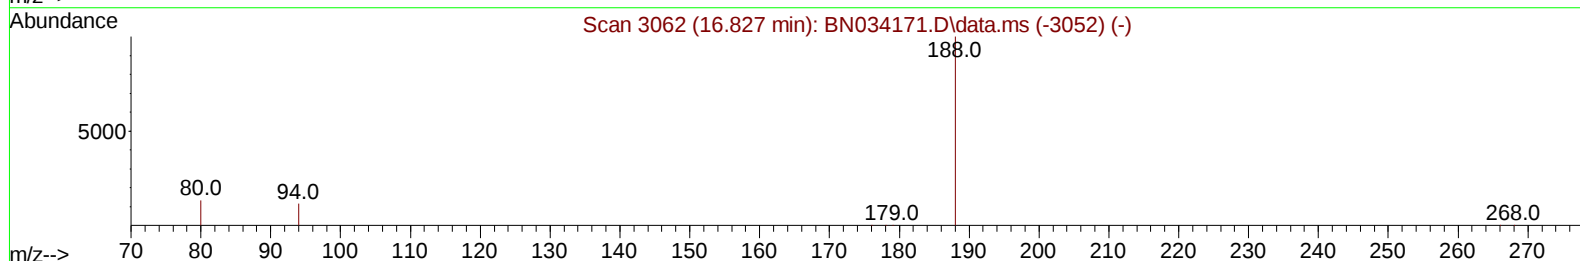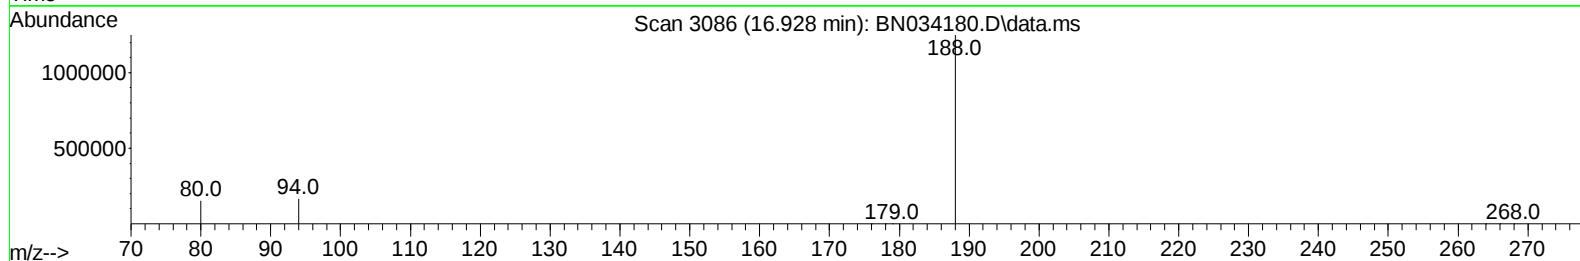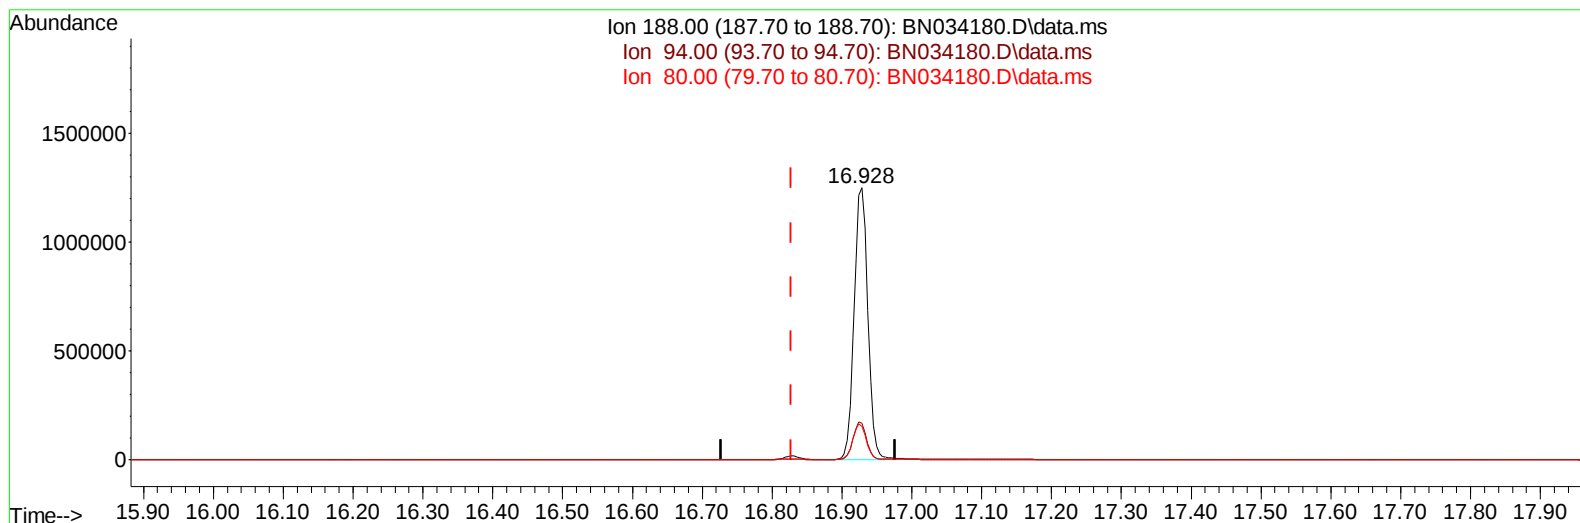

TIC: BN034180.D\data.ms

(13) Phenanthrene-d10 (I)

16.928min (+ 0.101) 0.40 ng/u1

response 1695984

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	13.24#
80.00	11.50	12.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

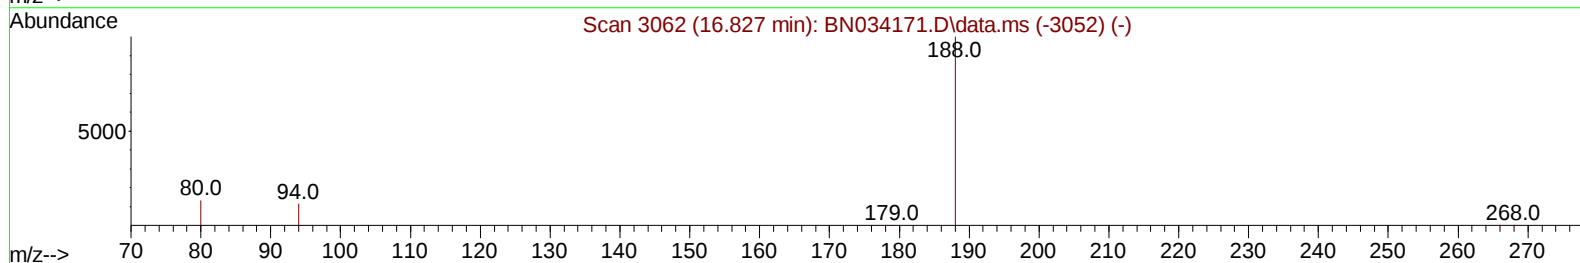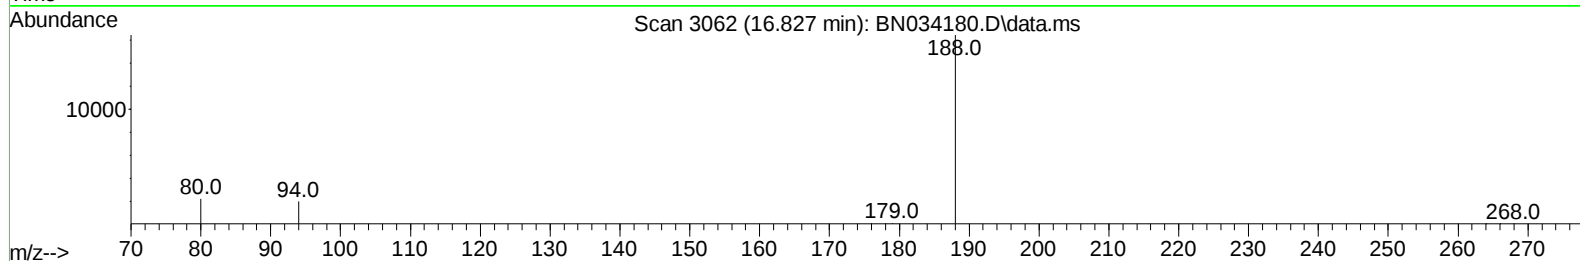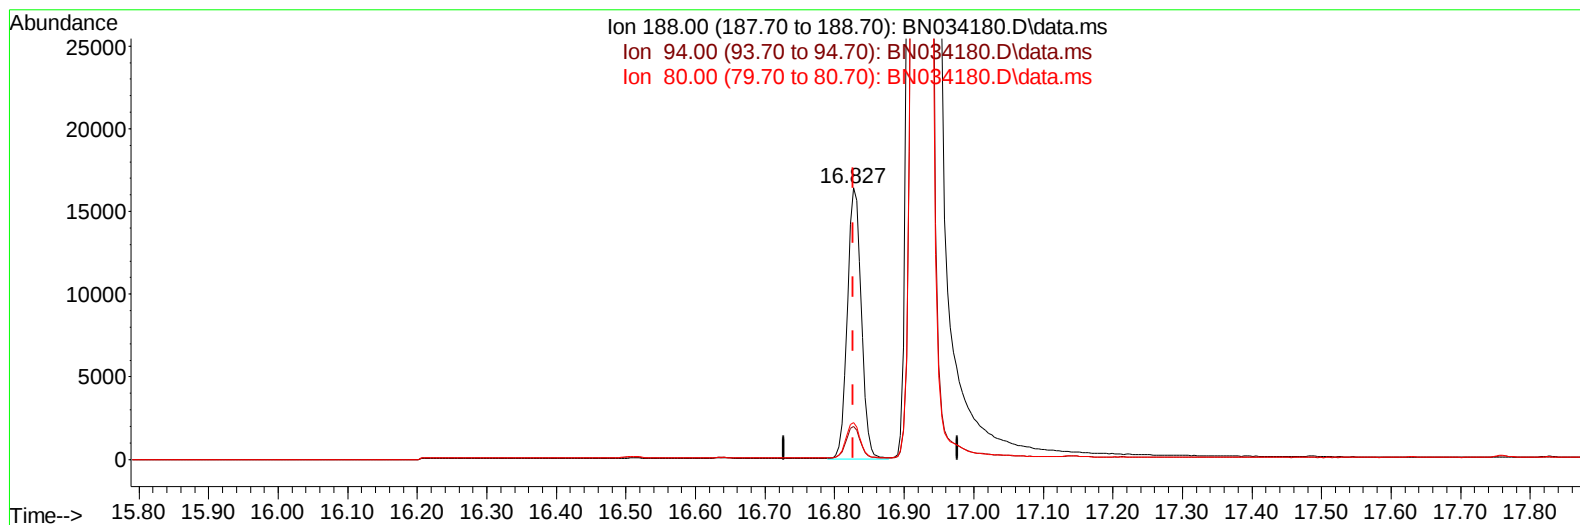

TIC: BN034180.D\data.ms

(13) Phenanthrene-d10 (I)

16.827min (+ 0.000) 0.40 ng/u1 m

response 22756

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	12.12
80.00	11.50	13.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

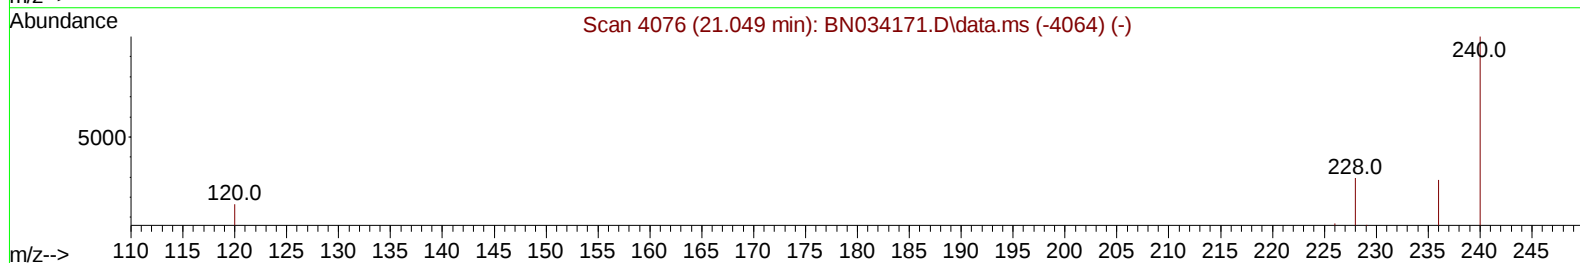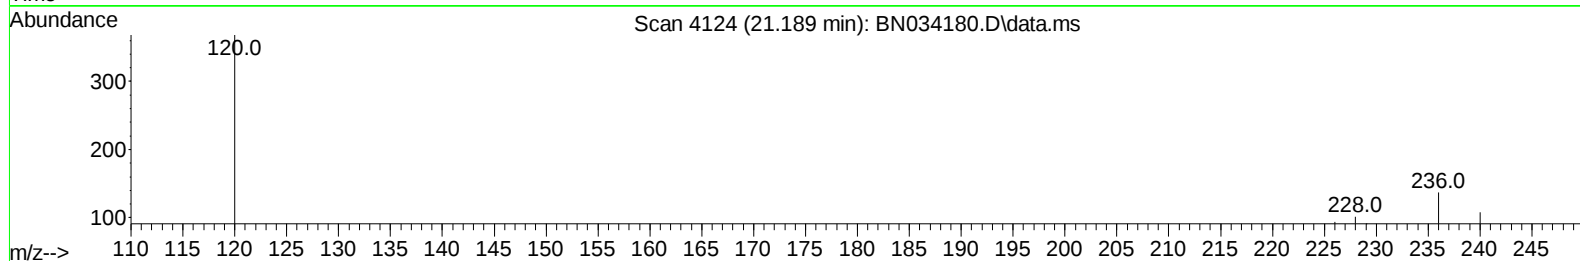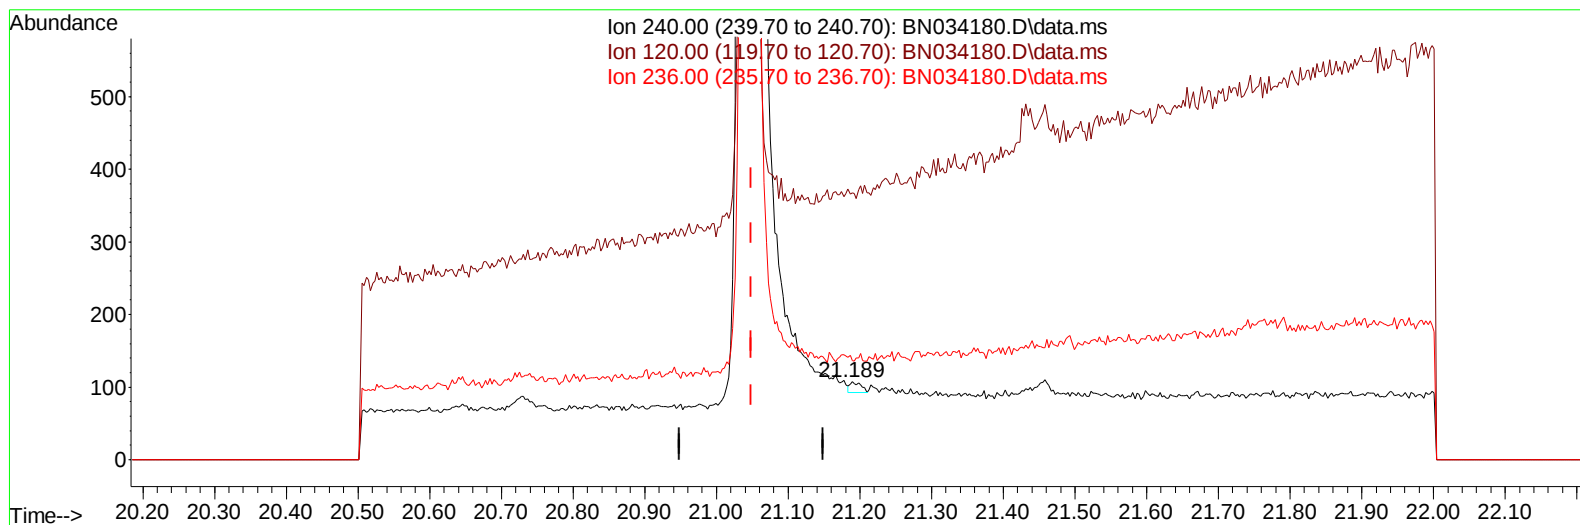

TIC: BN034180.D\data.ms

(17) Chrysene-d12

21.189min (+ 0.140) 0.40 ng/u1

response 15

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	340.74#
236.00	28.30	126.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

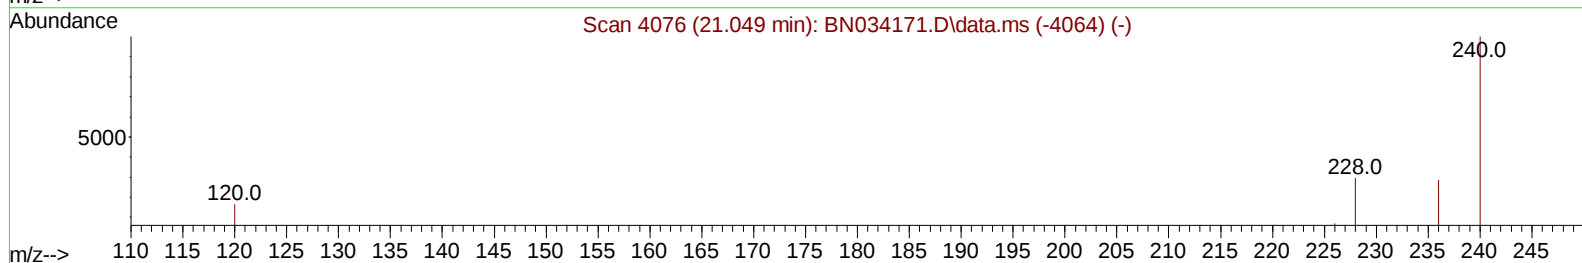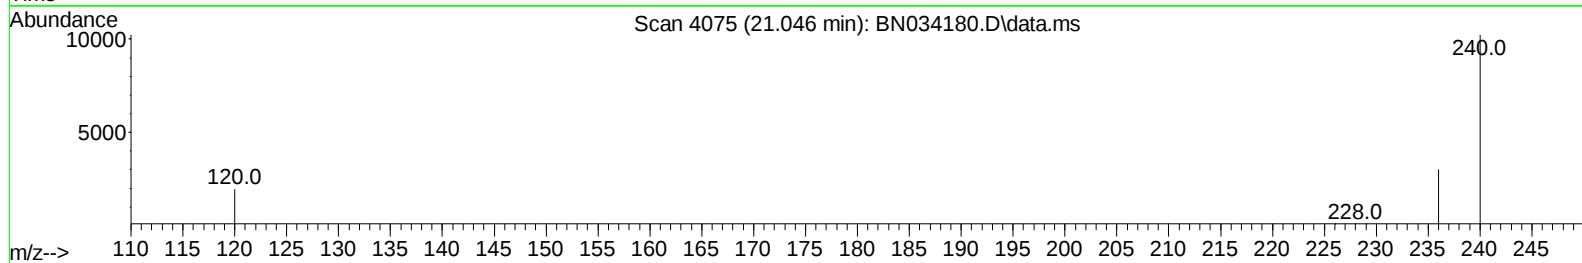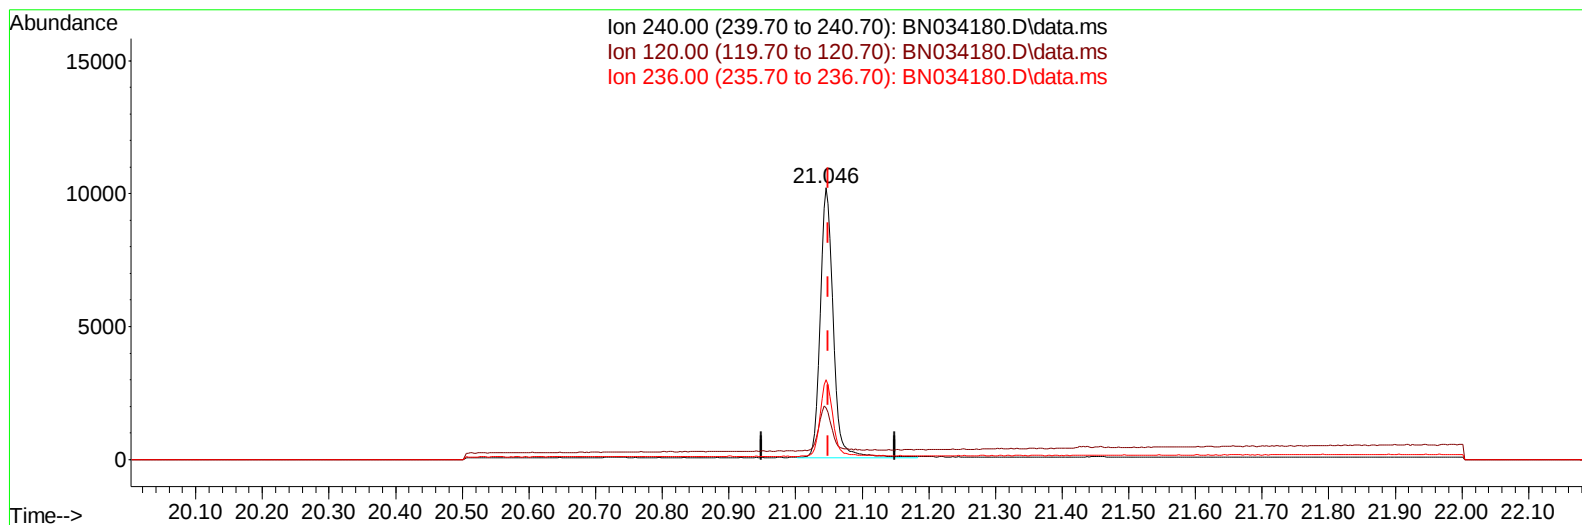

TIC: BN034180.D\data.ms

(17) Chrysene-d12

21.046min (-0.003) 0.40 ng/u1 m

response 13482

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	19.09
236.00	28.30	29.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

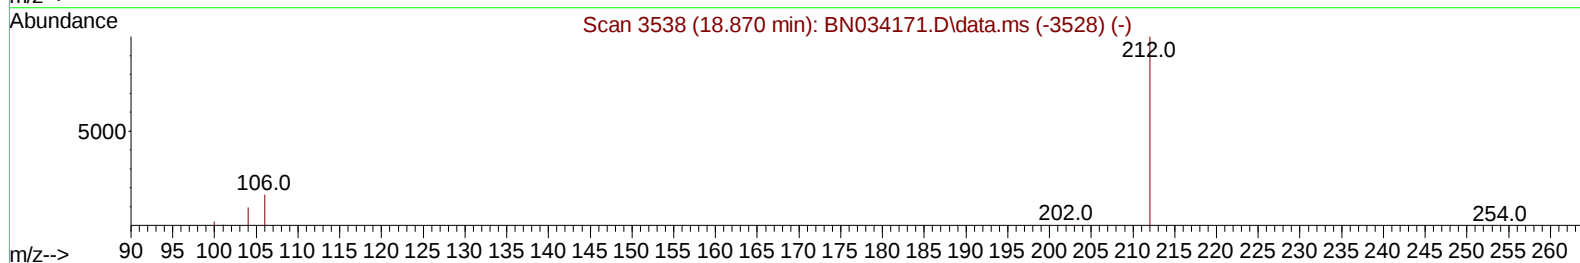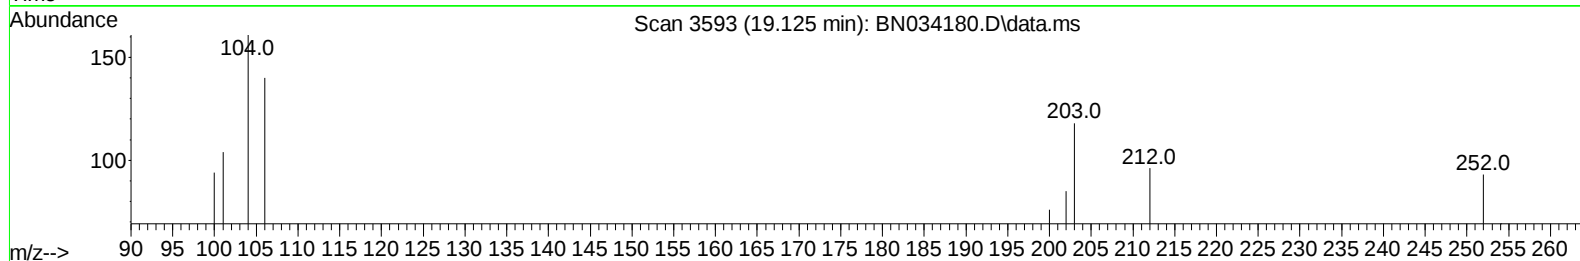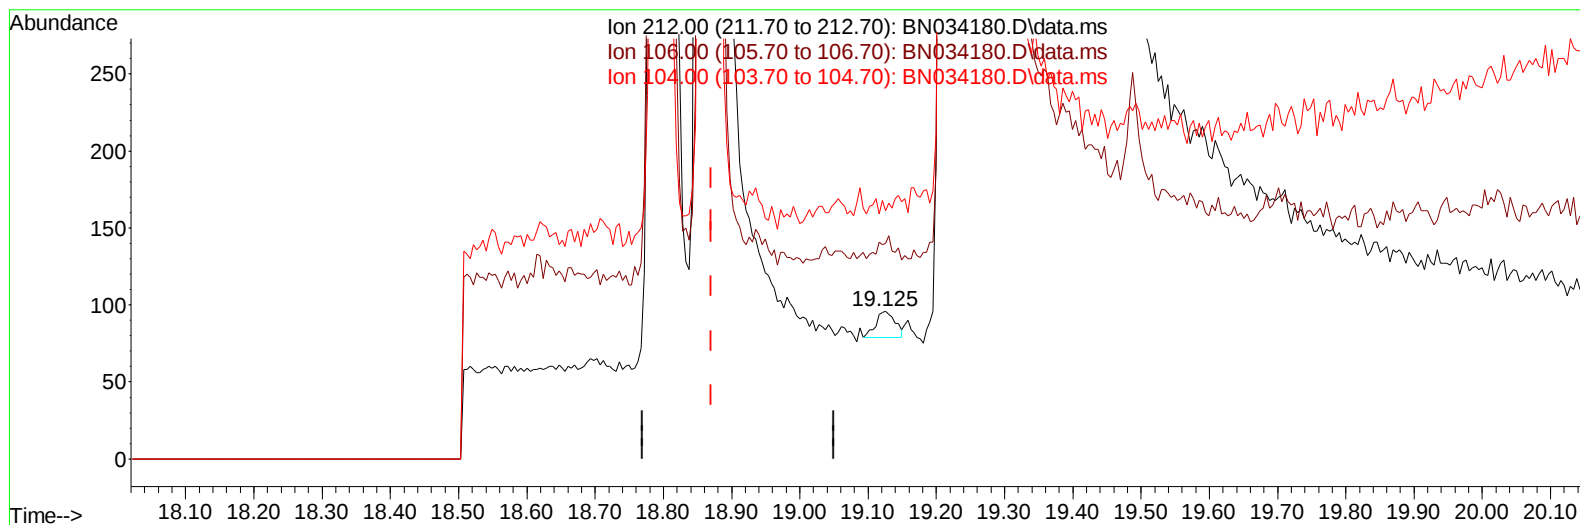

TIC: BN034180.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.125min (+ 0.256) 0.00 ng/u1

response 33

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	14.40	66.67#
104.00	8.30	30.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

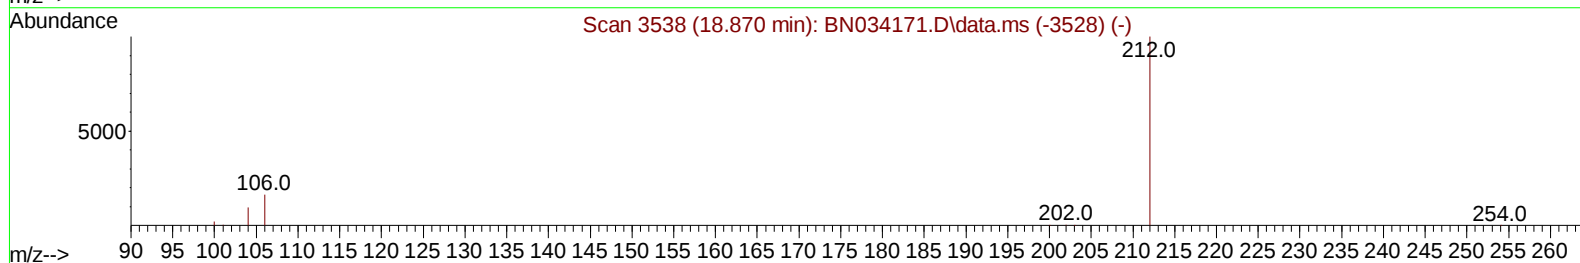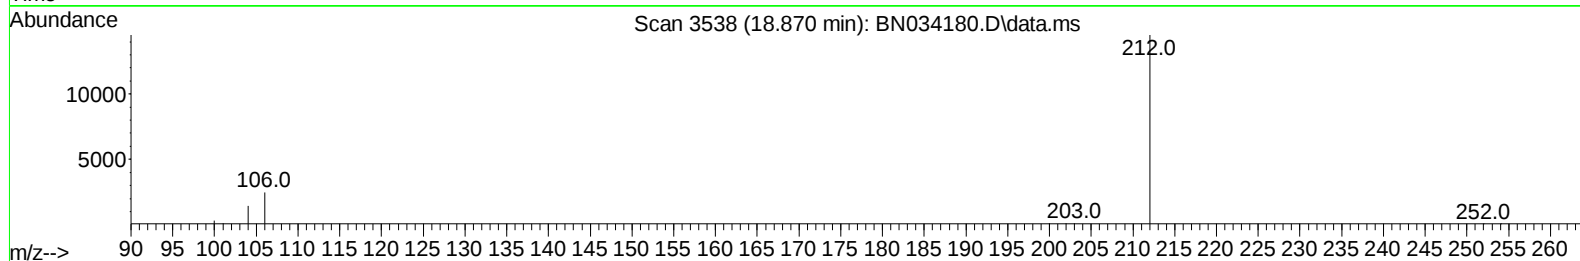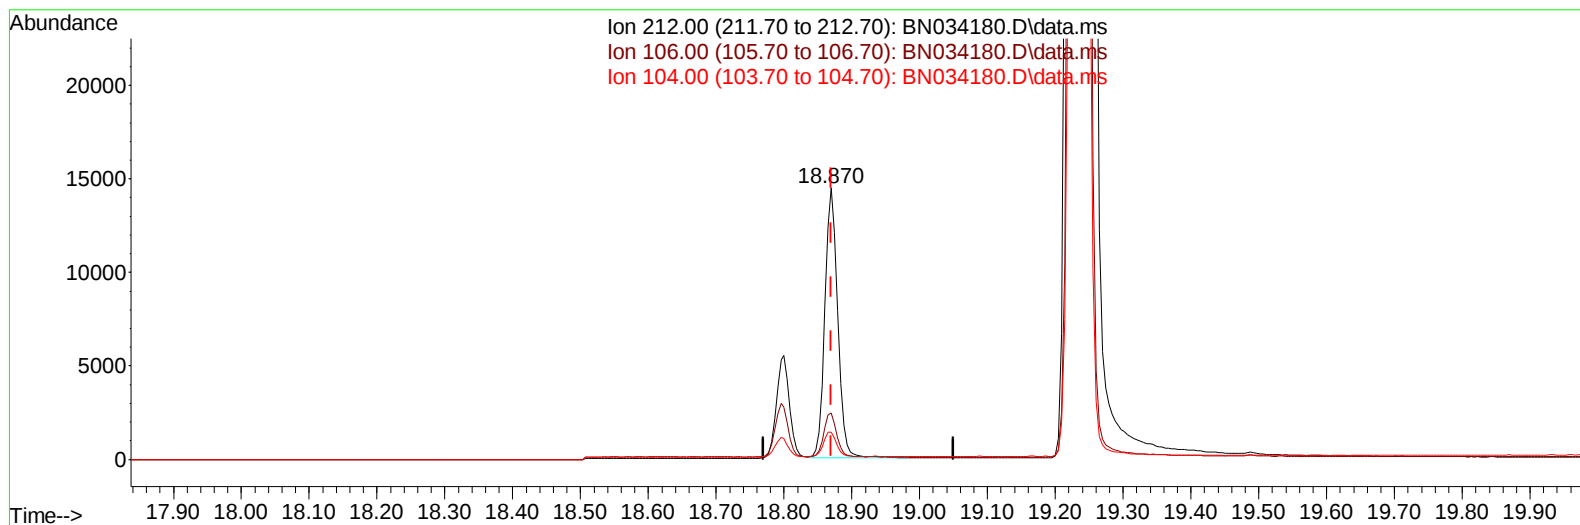

TIC: BN034180.D\data.ms

(18) Fluoranthene-d10 (SURR)

18.870min (+ 0.000) 0.47 ng/ul m

response 18988

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	14.40	0.12#
104.00	8.30	0.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

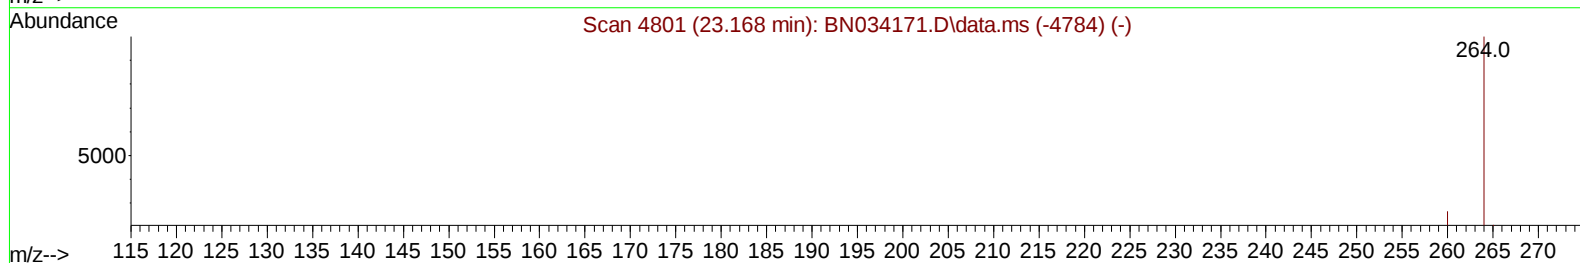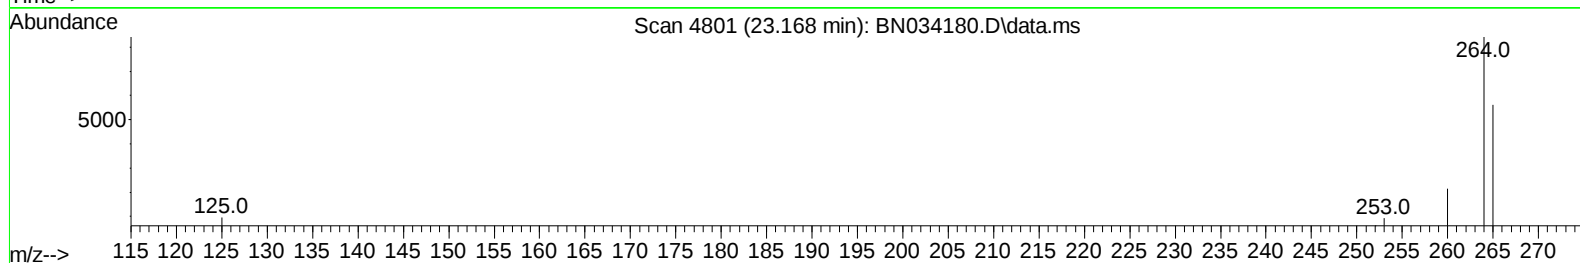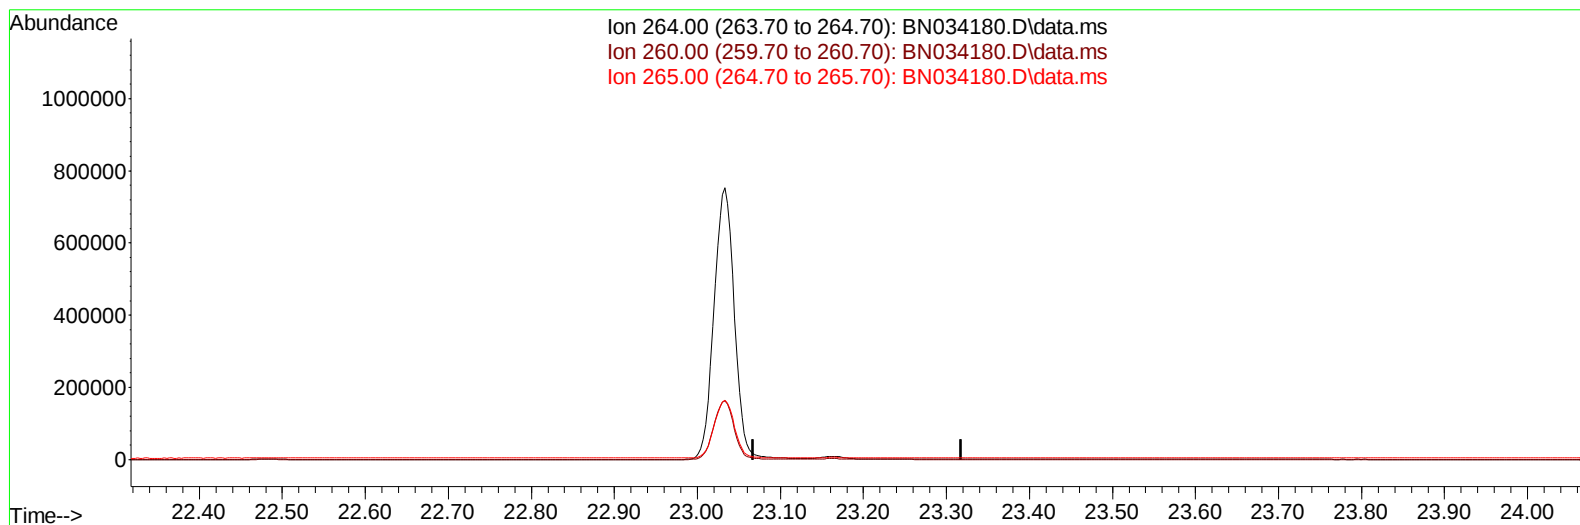

TIC: BN034180.D\data.ms

(23) Perylene-d12 (I)

23.168min (-23.168) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.60	0.00#
265.00	73.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034180.D
Acq On : 24 Sep 2024 00:40
Operator : RC/JU
Sample : P4092-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

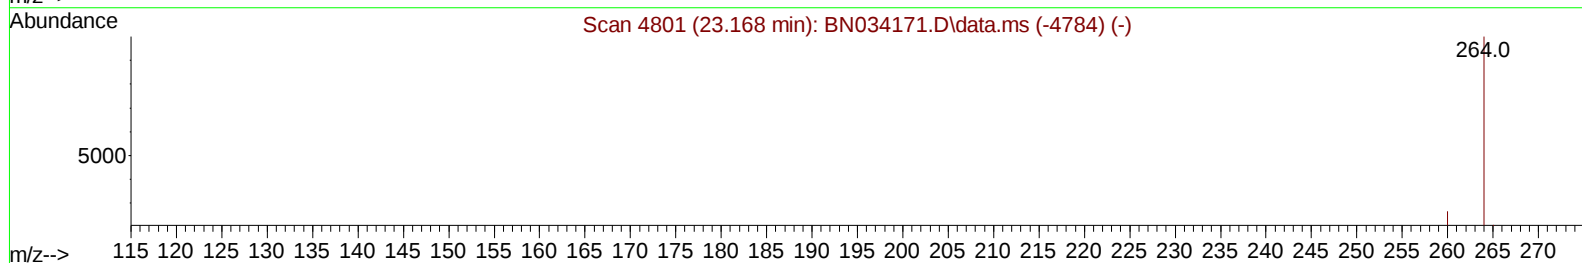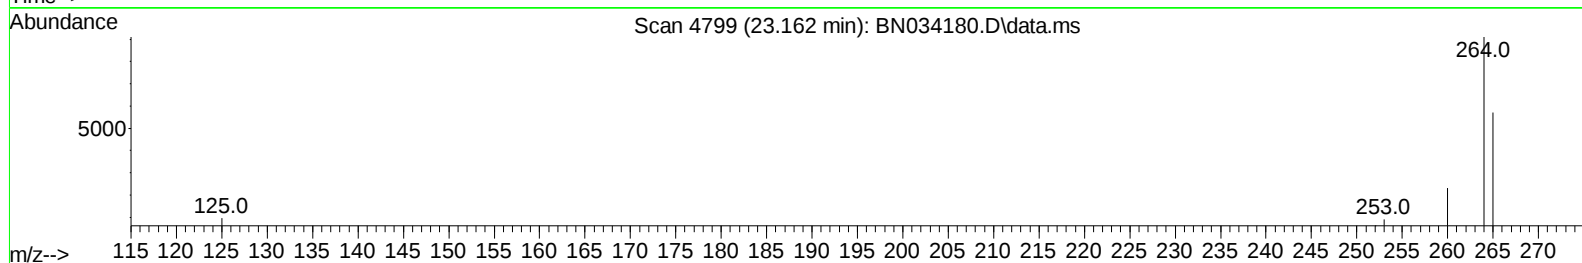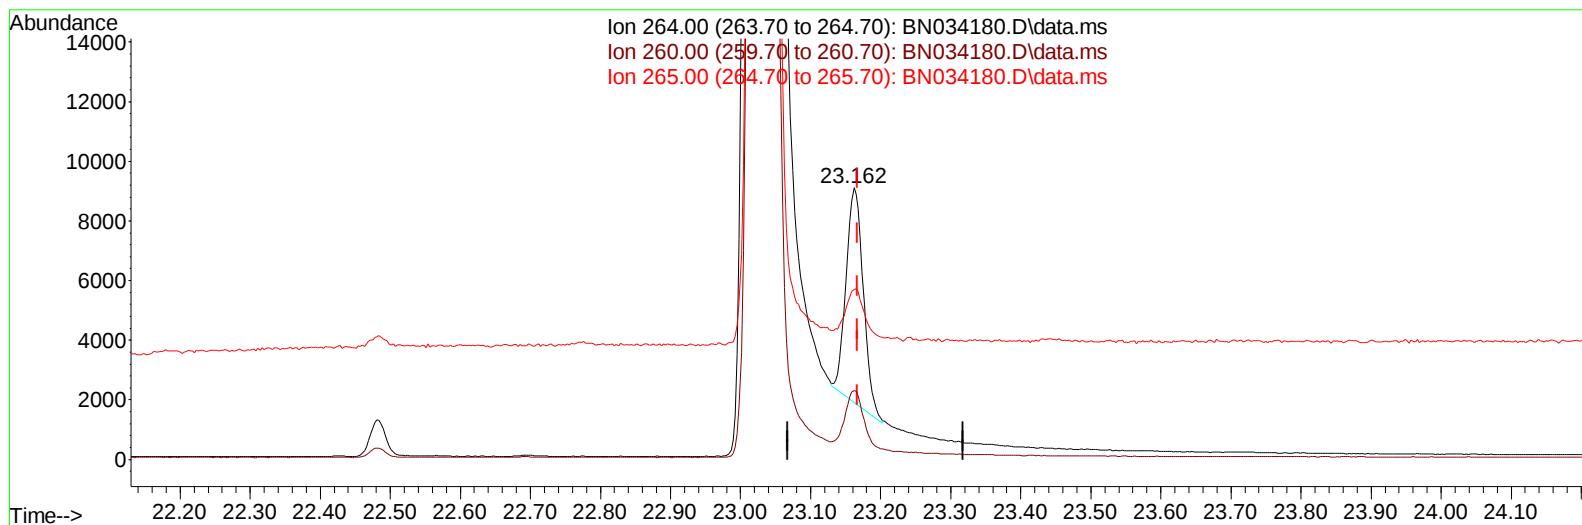

TIC: BN034180.D\data.ms

(23) Perylene-d12 (I)

23.162min (-0.006) 0.40 ng/ul m

response 12182

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.40
265.00	73.30	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
 Data File : BN034180.D
 Acq On : 24 Sep 2024 00:40
 Operator : RC/JU
 Sample : P4092-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B47

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 24 01:51:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 23 19:39:10 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.423	152		6851	0.400	ng/ul	0.00
4) Naphthalene-d8	10.180	136		21529	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.074	164		12462	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.827	188		22756m	0.400	ng/ul	0.00
17) Chrysene-d12	21.046	240		13482m	0.400	ng/ul	0.00
23) Perylene-d12	23.162	264		12182m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.039	96		34286	4.868	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.780	152		10303	0.334	ng/ul	0.00
18) Fluoranthene-d10	18.870	212		18988m	0.472	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.073	88		2038	0.261	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\  
Data File : BN034180.D  
Acq On    : 24 Sep 2024  00:40  
Operator  : RC/JU  
Sample    : P4092-11  
Misc      :  
ALS Vial  : 11    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
C0B47

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 24 01:51:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

