

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
 Data File : BN034182.D
 Acq On : 24 Sep 2024 01:53
 Operator : RC/JU
 Sample : P4092-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B15

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 24 03:12:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 23 19:39:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.423	152	6750	0.400	ng/ul	0.00
4) Naphthalene-d8	10.179	136	20885	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.074	164	12398	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.827	188	22599m	0.400	ng/ul	0.00
17) Chrysene-d12	21.046	240	13551m	0.400	ng/ul	0.00
23) Perylene-d12	23.165	264	12149m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.039	96	37438	5.395	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.780	152	10217	0.341	ng/ul	0.00
18) Fluoranthene-d10	18.870	212	18314m	0.453	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.073	88	5831	0.757	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034182.D
Acq On : 24 Sep 2024 01:53
Operator : RC/JU
Sample : P4092-01
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B15

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024


Quant Time: Sep 24 03:12:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

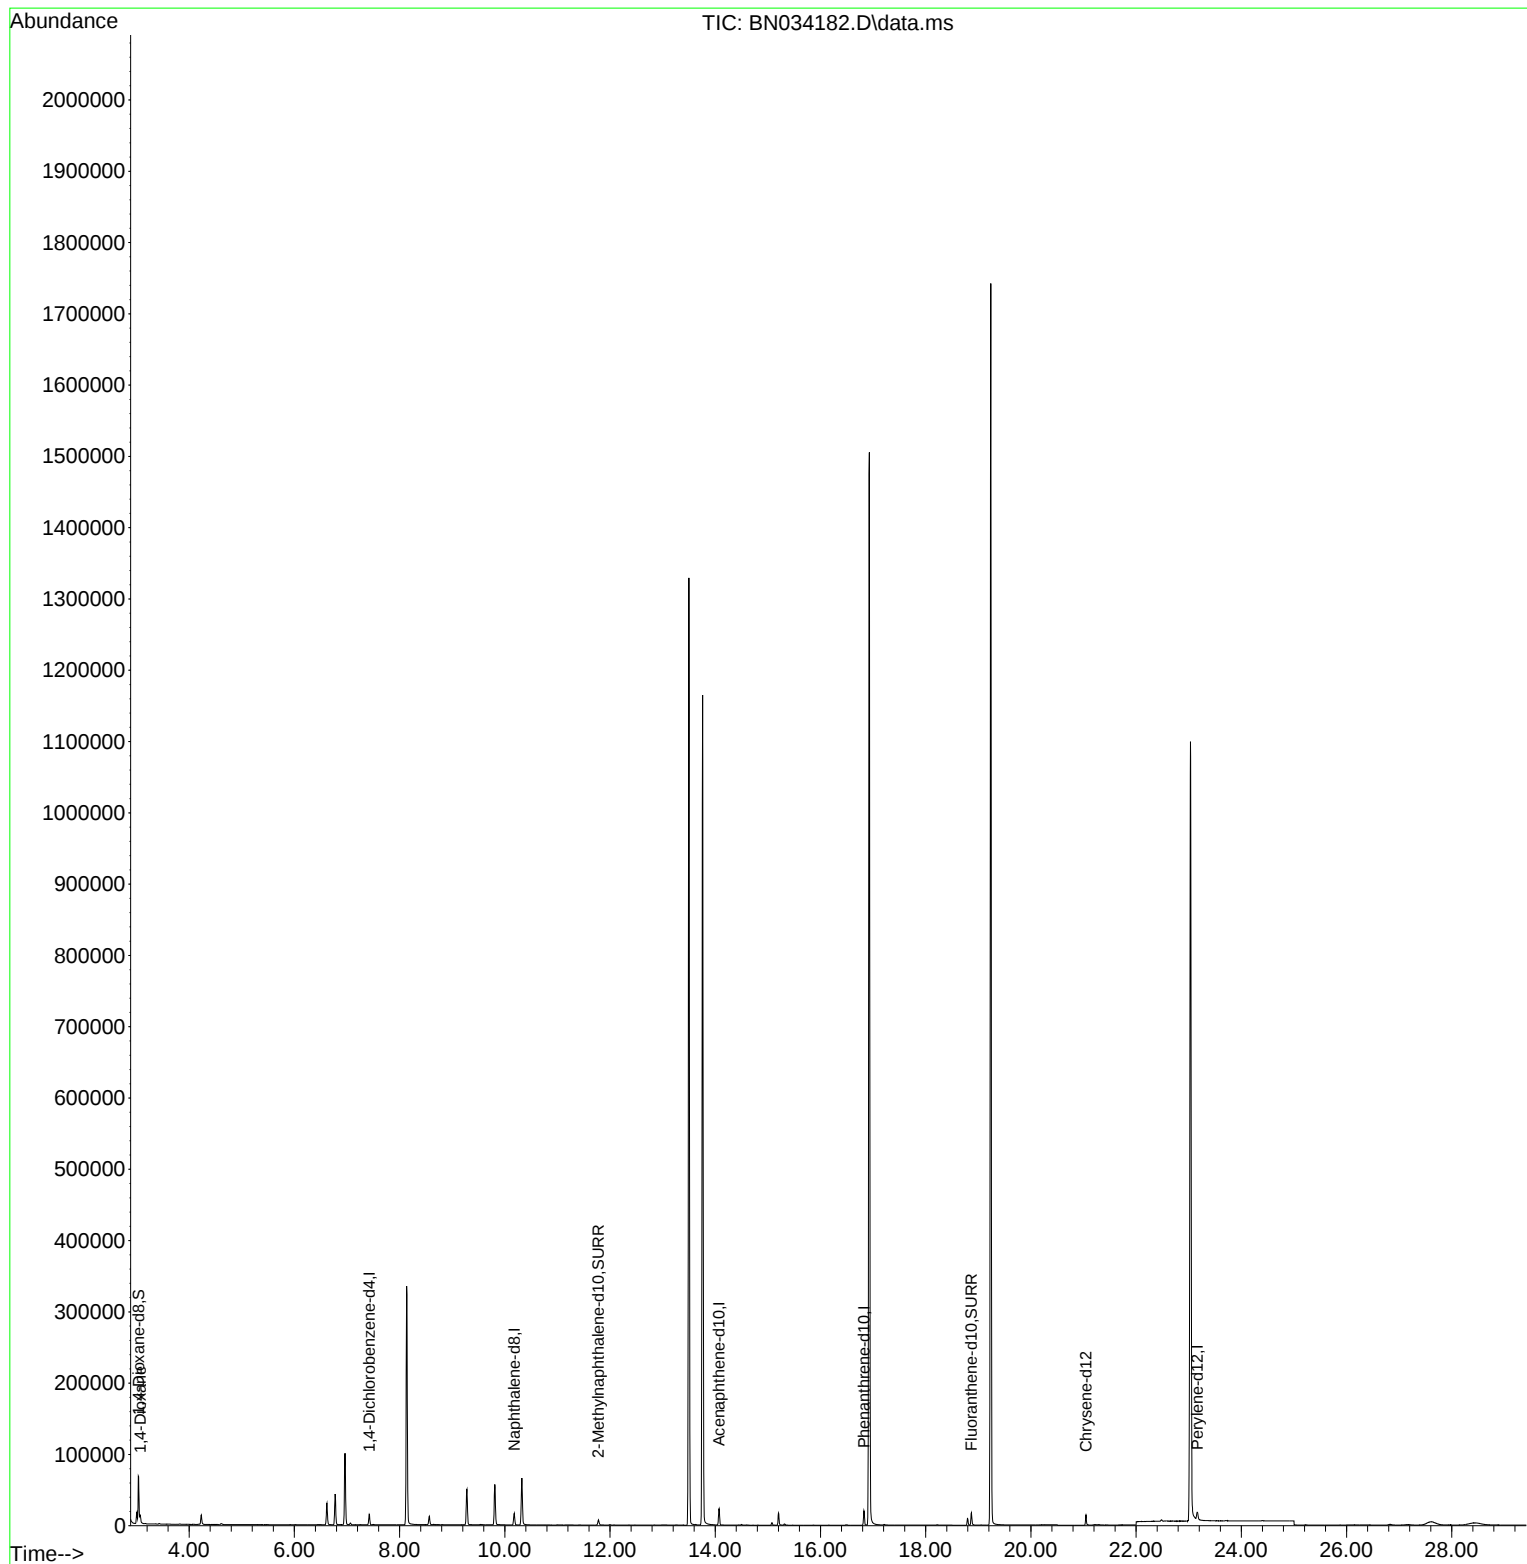

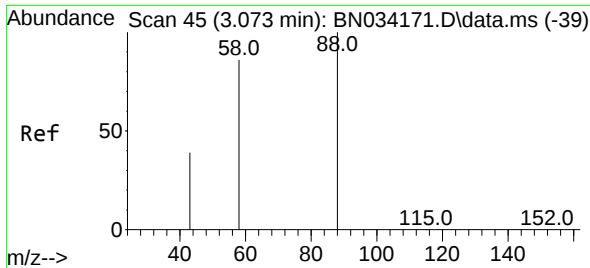

#2
 1,4-Dioxane
 Concen: 0.757 ng/ul
 RT: 3.073 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BN034182.D
 Acq: 24 Sep 2024 01:53

Instrument :
 BNA_N
 ClientSampleId :
 C0B15

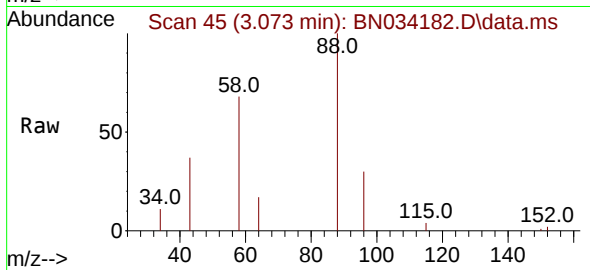

Tgt Ion: 88 Resp: 583

Ion	Ratio	Lower	Upper
88	100		
43	37.2	47.0	70.4
58	67.8	53.0	79.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/25/2024

