

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
 Data File : BN034204.D
 Acq On : 24 Sep 2024 16:20
 Operator : RC/JU
 Sample : P4107-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B23

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 24 16:57:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 23 19:39:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.423	152	6035	0.400	ng/ul	0.00
4) Naphthalene-d8	10.174	136	17211	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.069	164	9865	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.827	188	18939m	0.400	ng/ul	0.00
17) Chrysene-d12	21.046	240	13603m	0.400	ng/ul	0.00
23) Perylene-d12	23.162	264	13484m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.039	96	32639	5.261	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.780	152	6165	0.250	ng/ul	0.00
18) Fluoranthene-d10	18.870	212	14942	0.368	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.073	88	4232	0.615	ng/ul#	Qvalue 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034204.D
Acq On : 24 Sep 2024 16:20
Operator : RC/JU
Sample : P4107-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 24 16:57:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

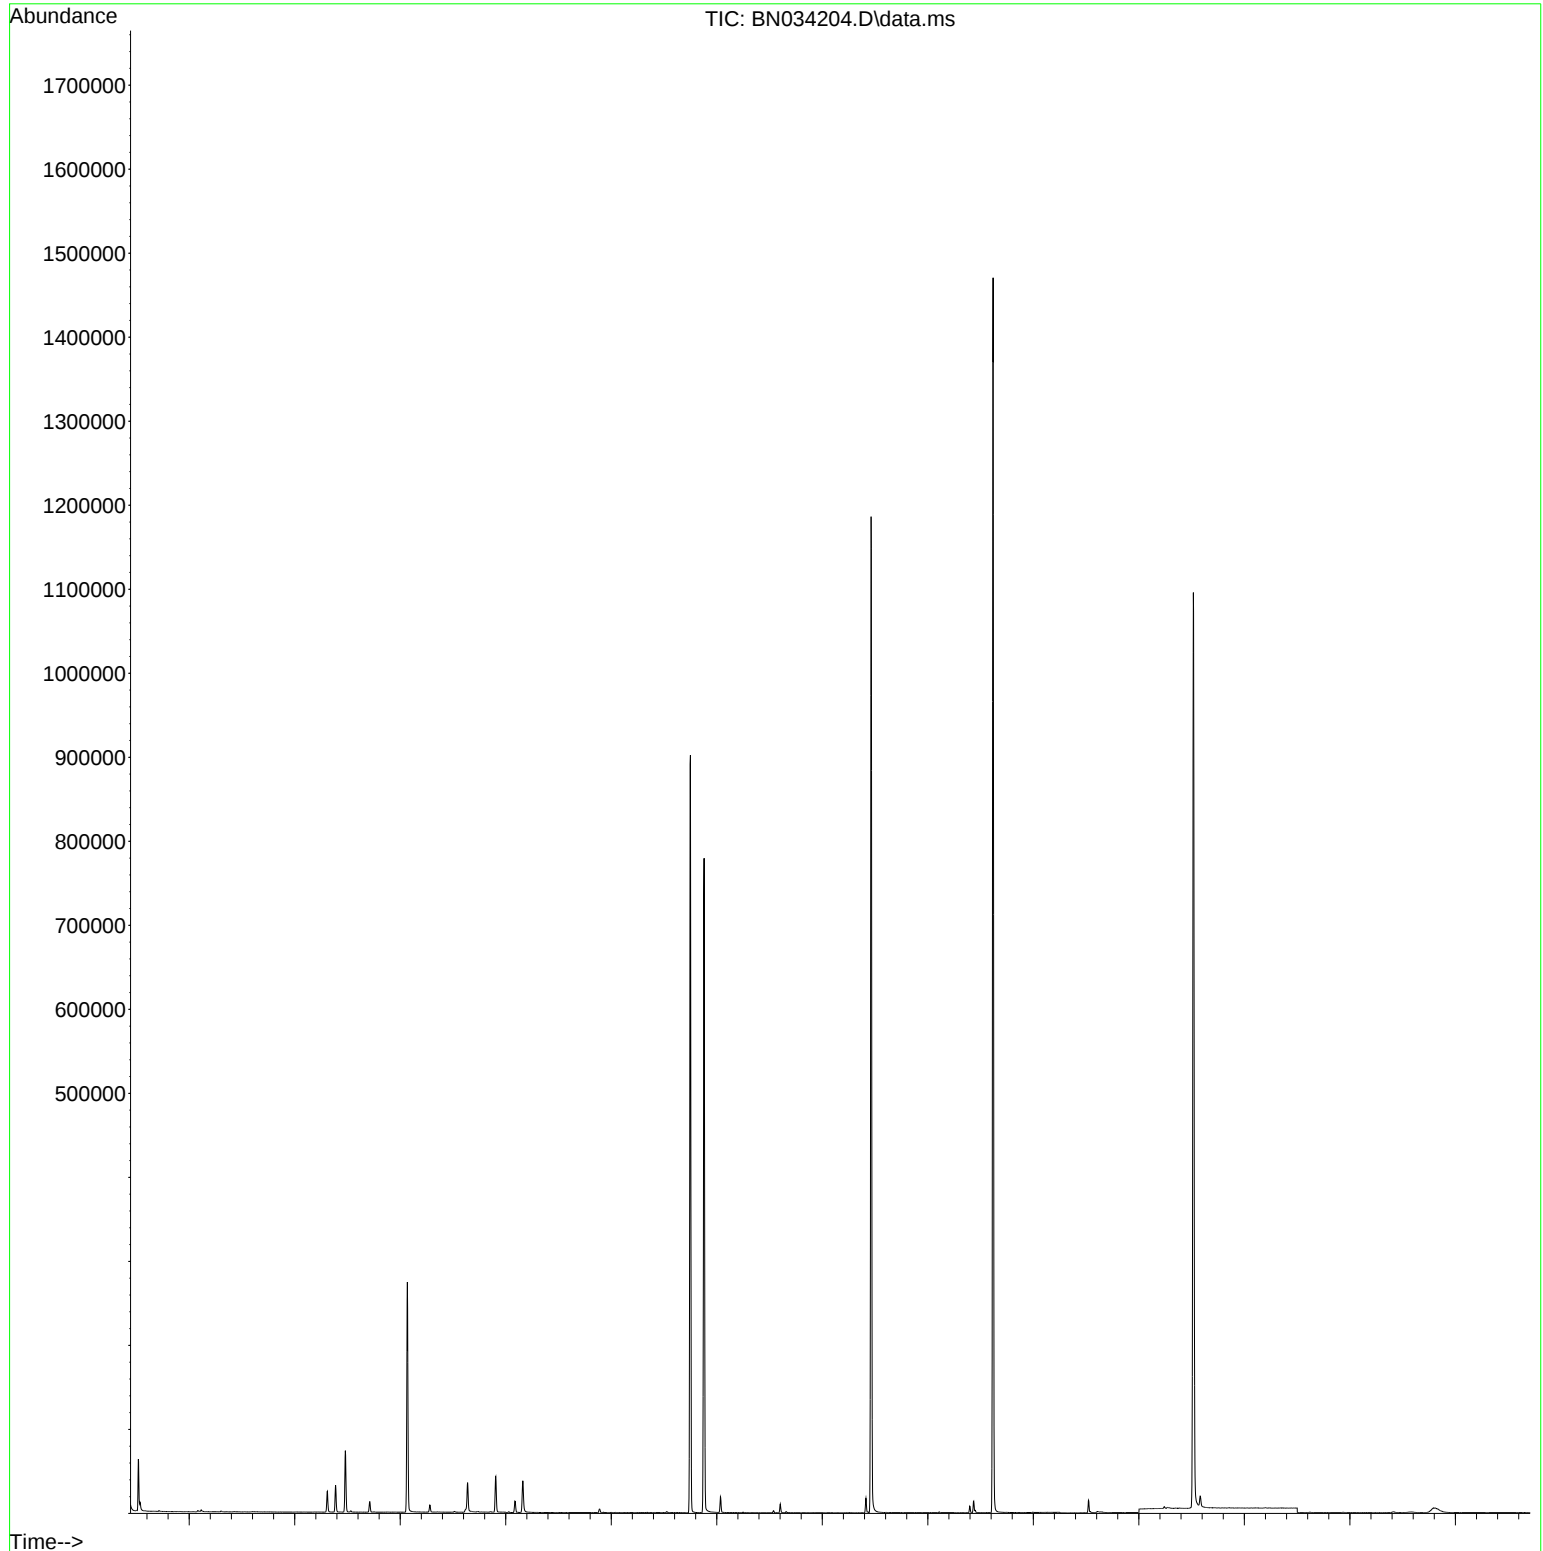


Abundance Scan 45 (3.073 min): BN034193.D\data.ms (-39)

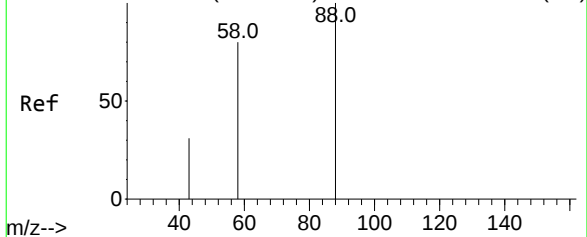

#2
1,4-Dioxane
Concen: 0.615 ng/ul
RT: 3.073 min Scan# 45
Delta R.T. -0.000 min
Lab File: BN034204.D
Acq: 24 Sep 2024 16:20

Instrument :
BNA_N
ClientSampleId :
C0B23

Abundance Scan 45 (3.073 min): BN034204.D\data.ms

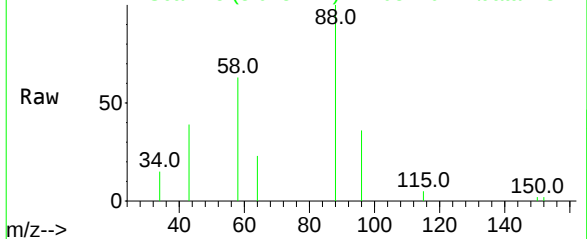

Tgt Ion: 88 Resp: 4232
Ion Ratio Lower Upper
88 100
43 38.7 47.0 70.4#
58 62.8 53.0 79.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

Abundance Scan 45 (3.073 min): BN034204.D\data.ms (-21)

