

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
 Data File : BN034216.D
 Acq On : 25 Sep 2024 00:10
 Operator : RC/JU
 Sample : P4107-06
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B43

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/25/2024

Quant Time: Sep 25 01:06:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 23 19:39:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.419	152	6875	0.400	ng/u1	0.00
4) Naphthalene-d8	10.174	136	21186	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.069	164	12723	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.827	188	25540m	0.400	ng/u1	0.00
17) Chrysene-d12	21.046	240	14937m	0.400	ng/u1	0.00
23) Perylene-d12	23.162	264	11579m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.035	96	38716	5.478	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.774	152	9075	0.299	ng/u1	0.00
18) Fluoranthene-d10	18.870	212	21958m	0.493	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.069	88	1609	0.205	ng/u1	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092424\
Data File : BN034216.D
Acq On : 25 Sep 2024 00:10
Operator : RC/JU
Sample : P4107-06
Misc :
ALS Vial : 50 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B43

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024


Quant Time: Sep 25 01:06:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 19:39:10 2024
Response via : Initial Calibration

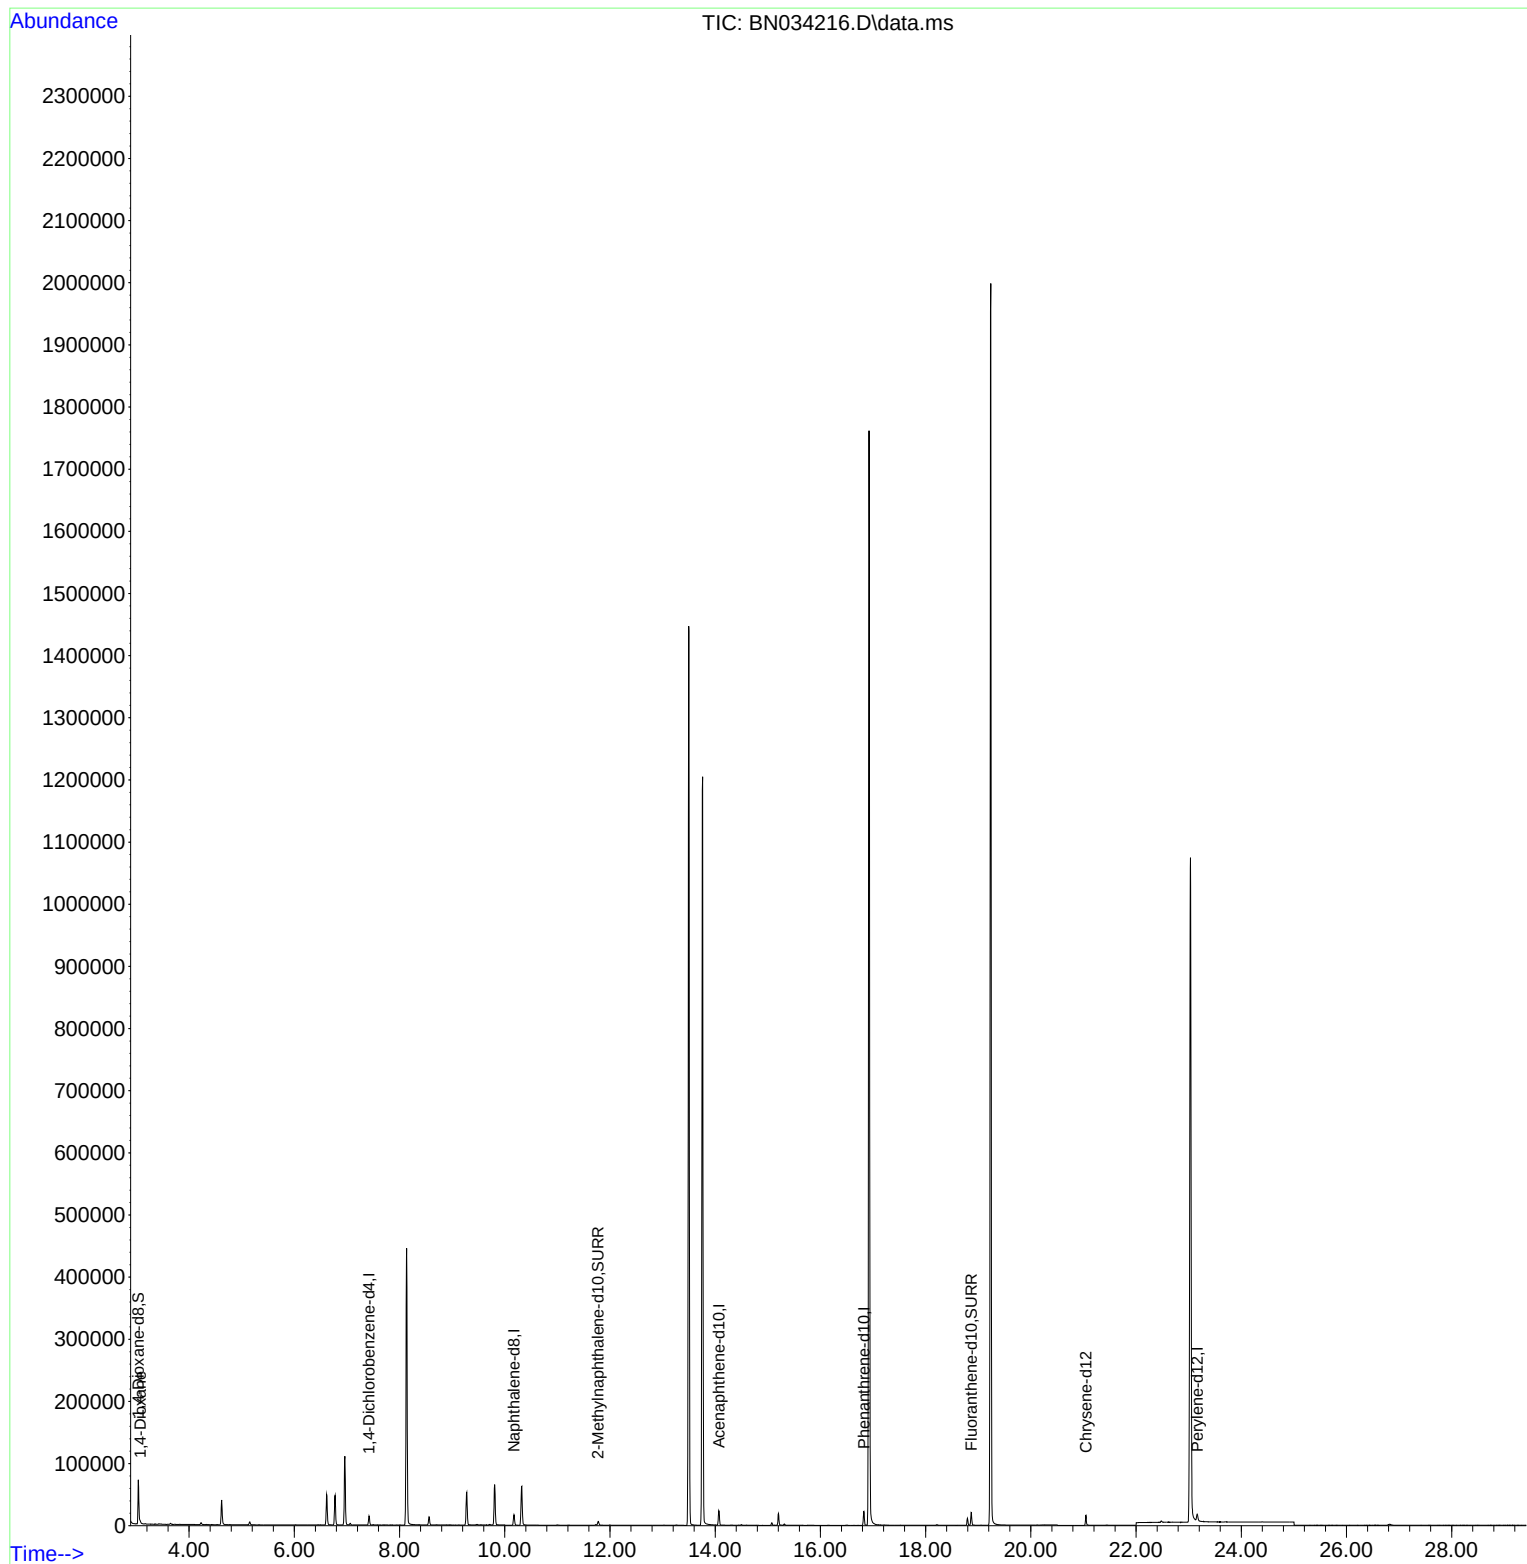

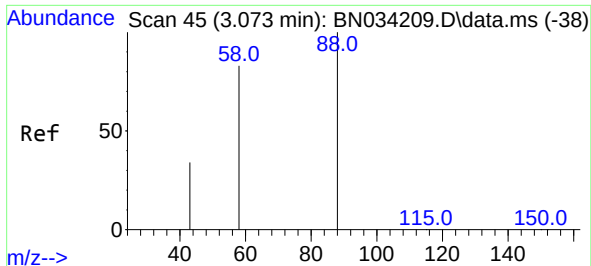

#2
1,4-Dioxane
Concen: 0.205 ng/ul
RT: 3.069 min Scan# 44
Delta R.T. -0.004 min
Lab File: BN034216.D
Acq: 25 Sep 2024 00:10

Instrument :
BNA_N
ClientSampleId :
C0B43

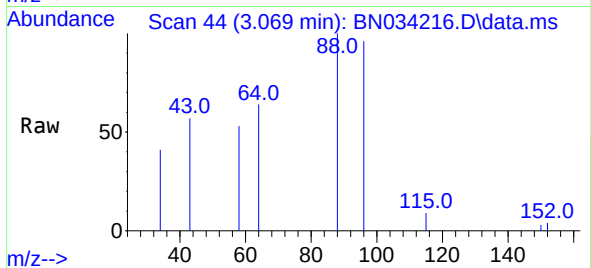

Tgt Ion: 88 Resp: 1609
Ion Ratio Lower Upper
88 100
43 57.1 47.0 70.4
58 53.1 53.0 79.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/25/2024

