


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092519\
 Data File : BN007850.D
 Acq On : 25 Sep 2019 12:48
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

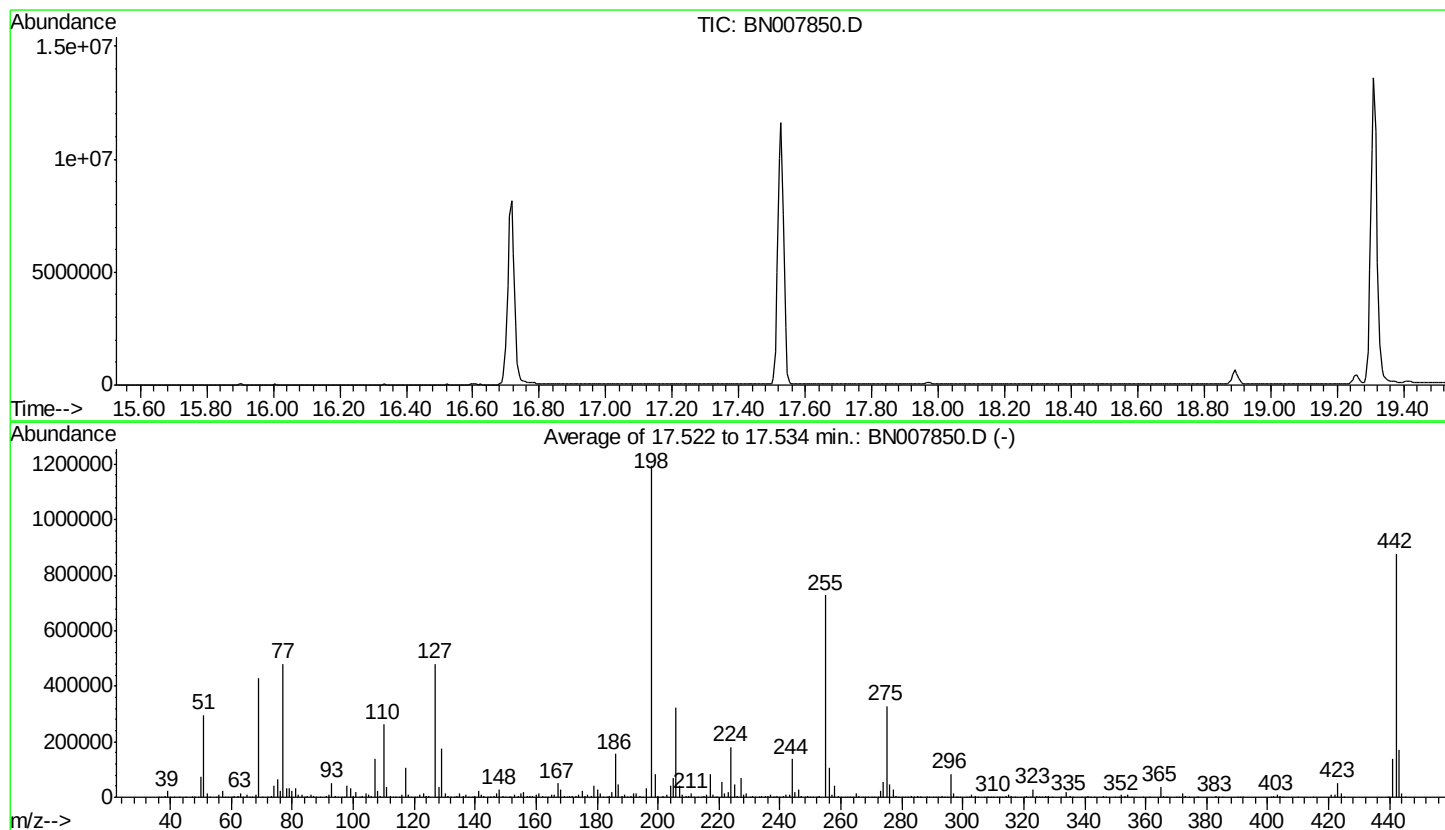

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	295534	PASS
68	69	0.00	2	1.7	7166	PASS
69	198	0.00	100	35.9	428217	PASS
70	69	0.00	2	0.5	2123	PASS
127	198	10	80	40.3	480874	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1194368	PASS
199	198	5	9	6.8	81520	PASS
275	198	10	60	27.6	329813	PASS
365	198	1	100	3.2	38186	PASS
441	198	0.01	100	11.4	136424	PASS
442	198	50	100	73.4	876906	PASS
443	442	15	24	19.4	170474	PASS