

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092524\
 Data File : BN034229.D
 Acq On : 25 Sep 2024 17:45
 Operator : RC/JU
 Sample : P3970-03RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BPOW6-8-HYD-20240910RE

Quant Time: Sep 25 18:11:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 16:09:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	5981	0.400	ng	0.02
7) Naphthalene-d8	10.212	136	16458	0.400	ng	# 0.02
13) Acenaphthene-d10	14.094	164	8439	0.400	ng	0.01
19) Phenanthrene-d10	16.846	188	17941	0.400	ng	# 0.00
29) Chrysene-d12	21.062	240	13121	0.400	ng	# 0.00
35) Perylene-d12	23.198	264	10591	0.400	ng	# 0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.098	112	812	0.048	ng	0.02
5) Phenol-d6	6.650	99	7	0.000	ng	0.02
8) Nitrobenzene-d5	8.600	82	3541	0.281	ng	0.03
11) 2-Methylnaphthalene-d10	11.814	152	897	0.037	ng	0.02
14) 2,4,6-Tribromophenol	15.604	330	357	0.093	ng	0.02
15) 2-Fluorobiphenyl	12.715	172	10049	0.293	ng	0.01
27) Fluoranthene-d10	18.890	212	15116	0.334	ng	0.00
31) Terphenyl-d14	19.508	244	12510	0.477	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.008	149	5036	0.291	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092524\
Data File : BN034229.D
Acq On : 25 Sep 2024 17:45
Operator : RC/JU
Sample : P3970-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BPOW6-8-HYD-20240910RE


Quant Time: Sep 25 18:11:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 16:09:28 2024
Response via : Initial Calibration

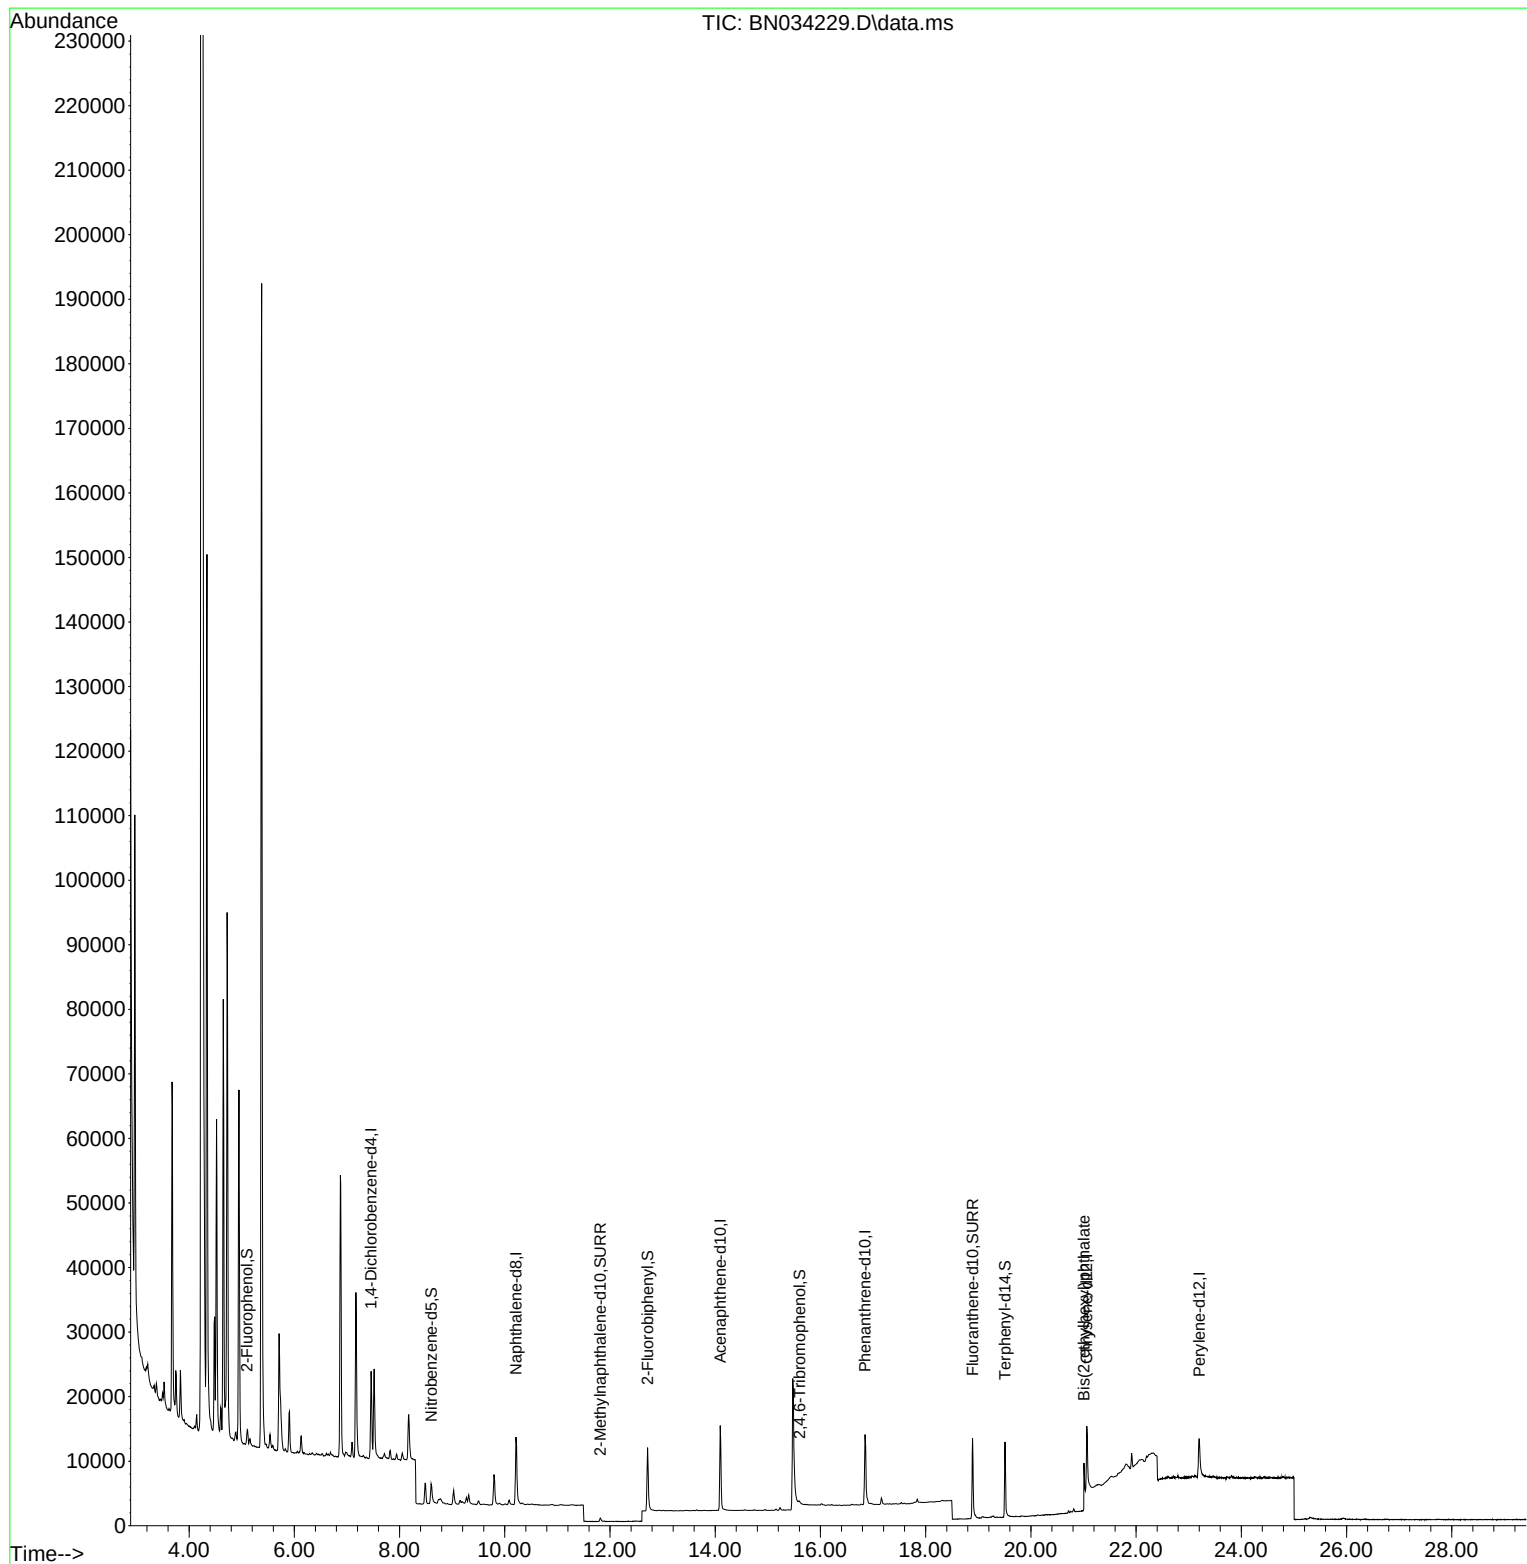



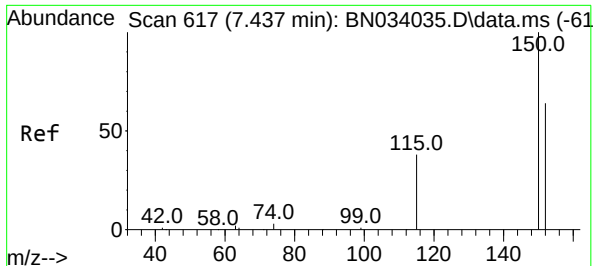


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.459 min Scan# 61
Delta R.T. 0.022 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45

Instrument :
BNA_N
ClientSampleId :
BPOW6-8-HYD-20240910RE



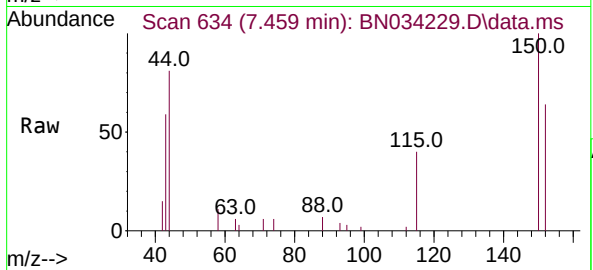



Tgt Ion:152 Resp: 5981
Ion Ratio Lower Upper
152 100
150 156.4 124.6 187.0
115 63.3 50.0 75.0

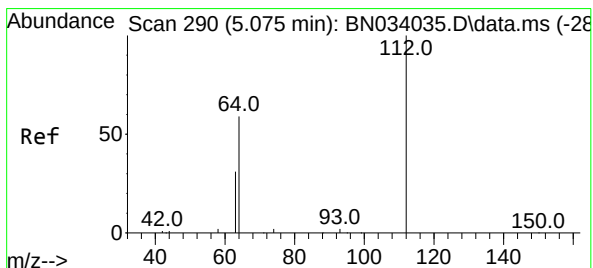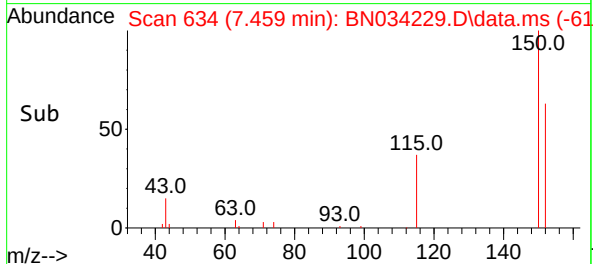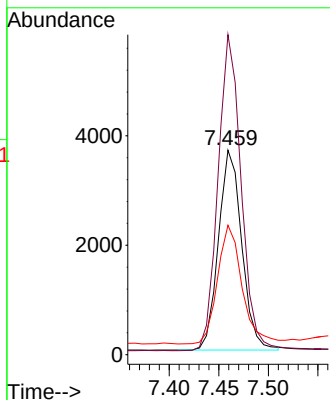

#4
2-Fluorophenol
Concen: 0.048 ng
RT: 5.098 min Scan# 307
Delta R.T. 0.023 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45

Tgt Ion:112 Resp: 812
Ion Ratio Lower Upper
112 100
64 63.7 48.6 72.8
63 30.4 25.6 38.4


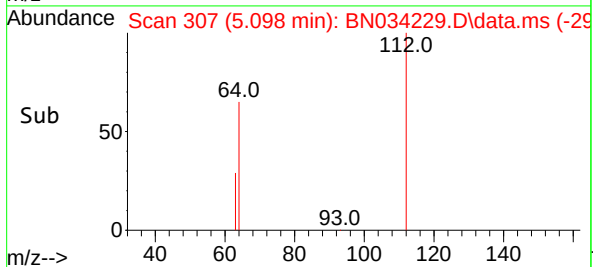
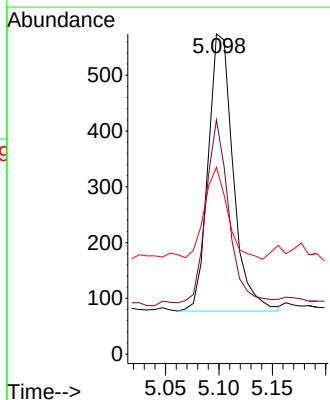
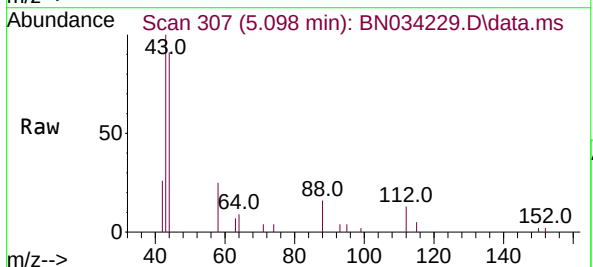


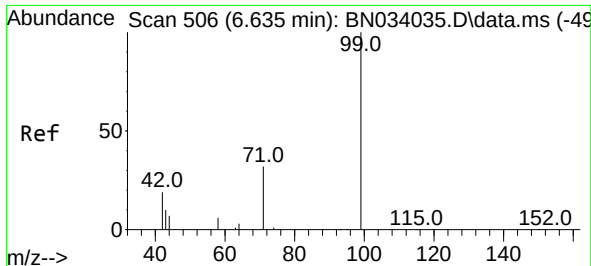

#5
Phenol-d6
Concen: 0.000 ng
RT: 6.650 min Scan# 51
Delta R.T. 0.015 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45




Instrument :
BNA_N
ClientSampleId :
BPOW6-8-HYD-20240910RE


Tgt Ion: 99 Resp: 7
Ion Ratio Lower Upper
99 100
42 0.0 17.8 26.8#
71 1685.7 26.2 39.2#

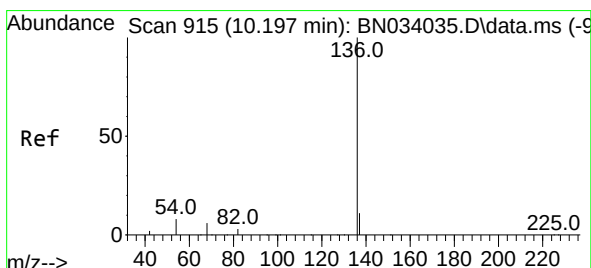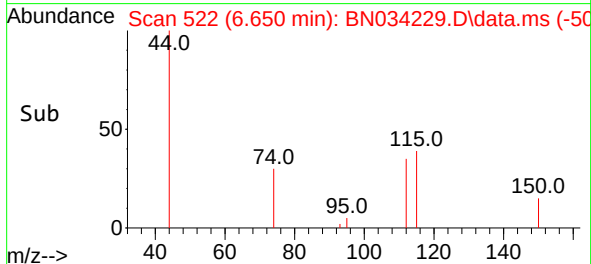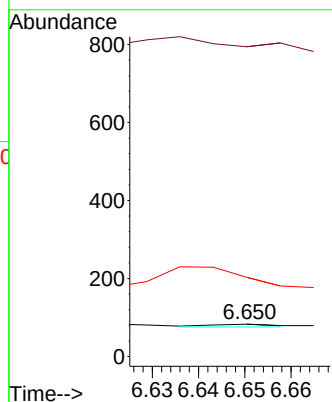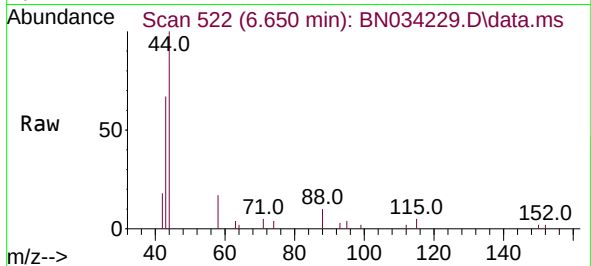

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.212 min Scan# 930
Delta R.T. 0.015 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45

Tgt Ion:136 Resp: 16458
Ion Ratio Lower Upper
136 100
137 11.5 9.0 13.6
54 12.8 6.8 10.2#
68 9.5 5.0 7.6#


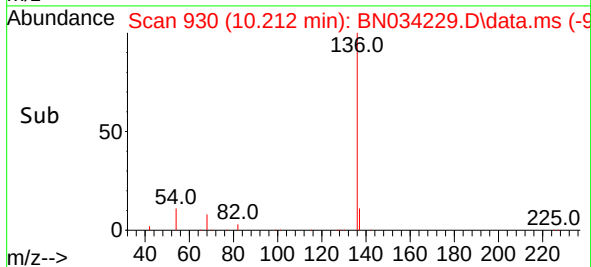
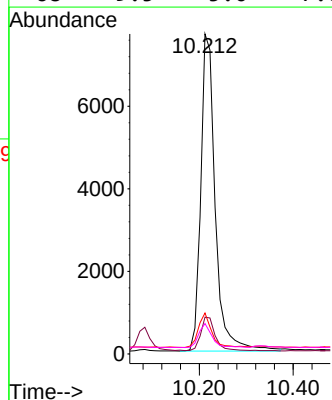
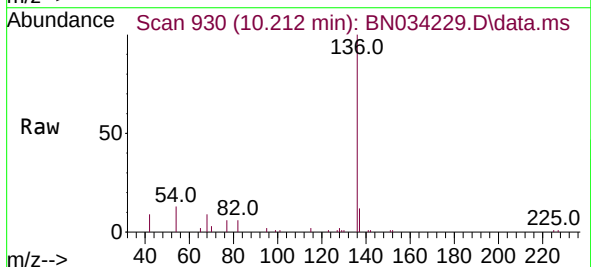


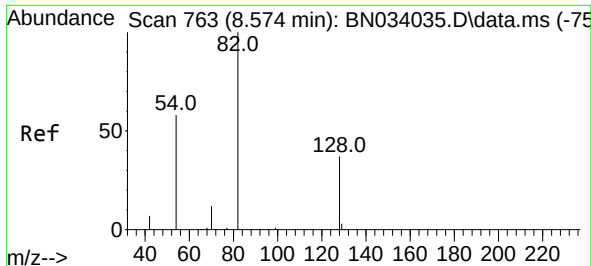

#8
Nitrobenzene-d5
Concen: 0.281 ng
RT: 8.600 min Scan# 71
Delta R.T. 0.026 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45




Instrument :
BNA_N
ClientSampleId :
BPOW6-8-HYD-20240910RE


Tgt Ion: 82 Resp: 3541
Ion Ratio Lower Upper
82 100
128 42.2 31.4 47.2
54 60.1 47.4 71.0

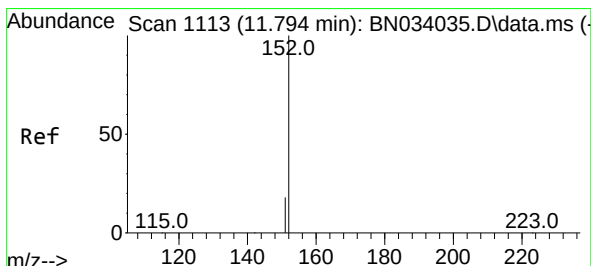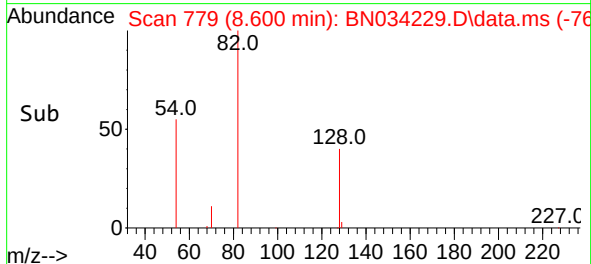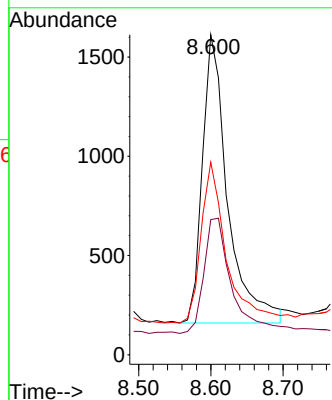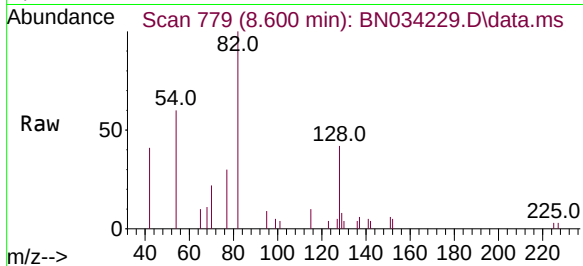

#11
2-Methylnaphthalene-d10
Concen: 0.037 ng
RT: 11.814 min Scan# 1133
Delta R.T. 0.020 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45

Tgt Ion:152 Resp: 897
Ion Ratio Lower Upper
152 100
151 21.6 16.8 25.2


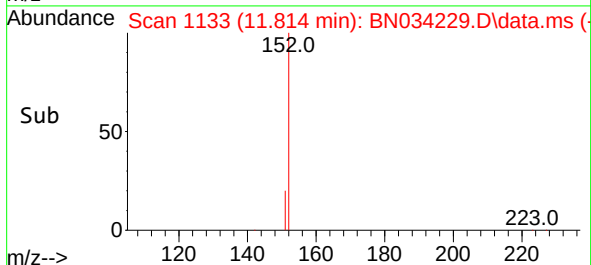
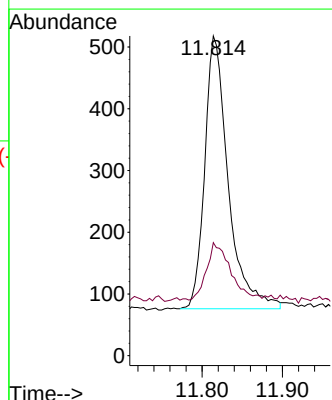
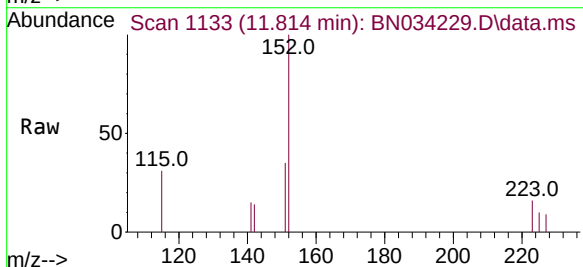


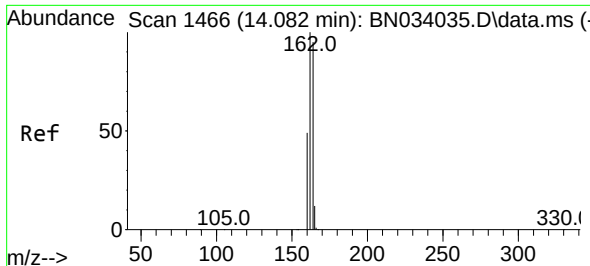

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.094 min Scan# 1466
Delta R.T. 0.012 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45




Instrument :
BNA_N
ClientSampleId :
BPOW6-8-HYD-20240910RE


Tgt Ion:164 Resp: 8439
Ion Ratio Lower Upper
164 100
162 105.7 84.2 126.2
160 51.1 41.7 62.5

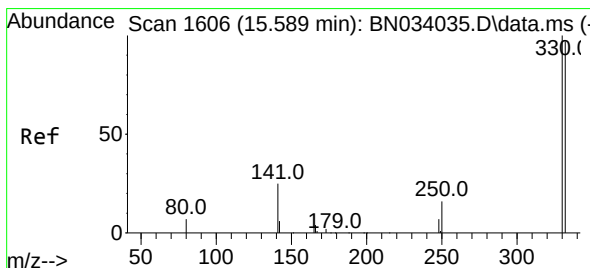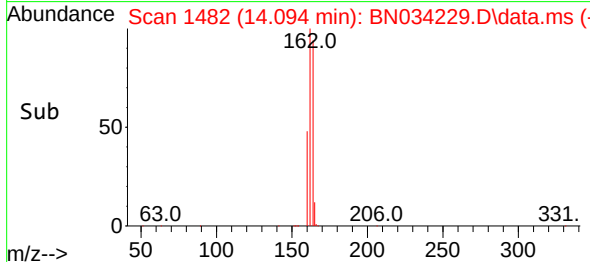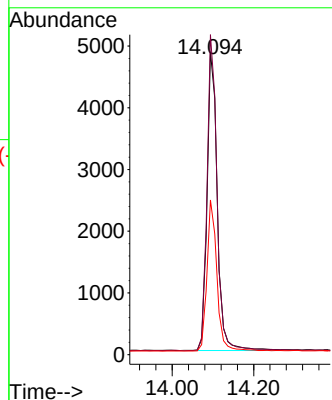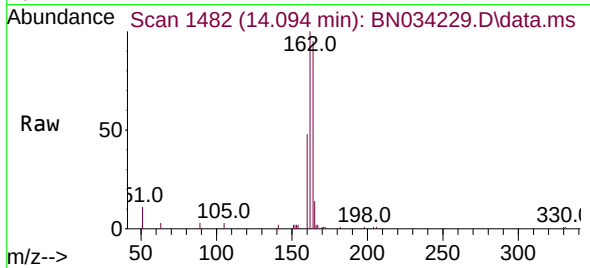

#14
2,4,6-Tribromophenol
Concen: 0.093 ng
RT: 15.604 min Scan# 1622
Delta R.T. 0.016 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45

Tgt Ion:330 Resp: 357
Ion Ratio Lower Upper
330 100
332 94.4 77.4 116.0
141 34.2 35.9 53.9#


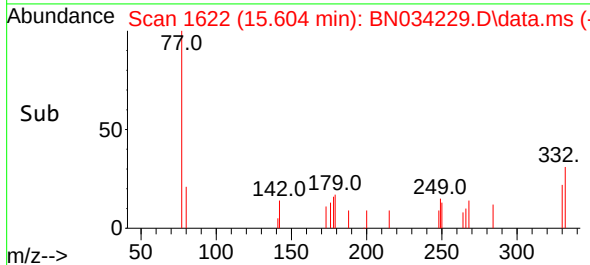
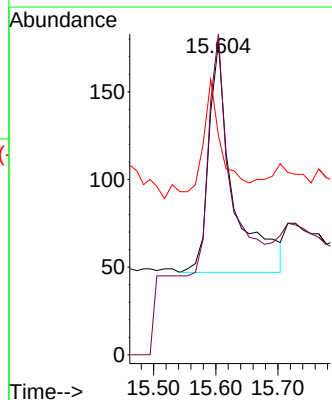
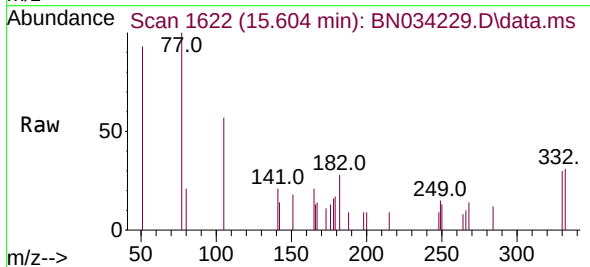


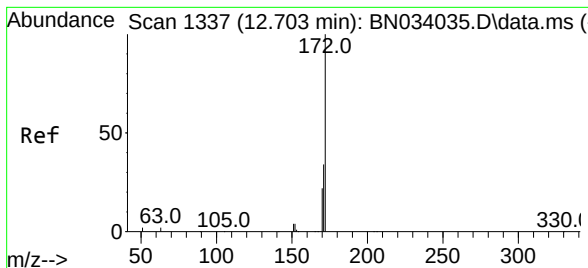

#15
2-Fluorobiphenyl
Concen: 0.293 ng
RT: 12.715 min Scan# 11
Delta R.T. 0.012 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45




Instrument :
BNA_N
ClientSampleId :
BPOW6-8-HYD-20240910RE


Tgt Ion:172 Resp: 10049
Ion Ratio Lower Upper
172 100
171 35.0 27.3 40.9
170 24.0 18.1 27.1

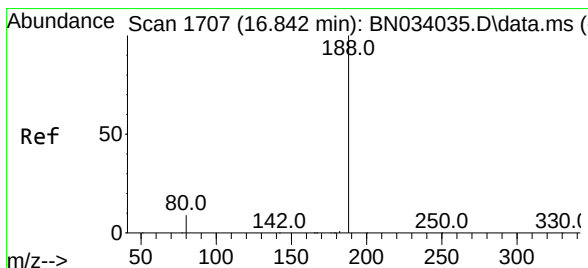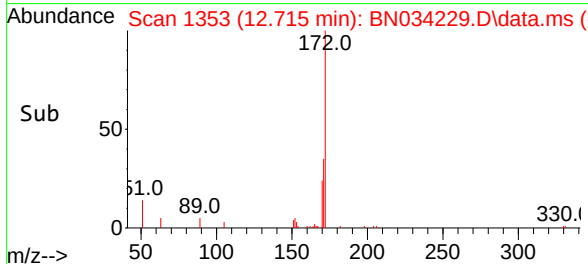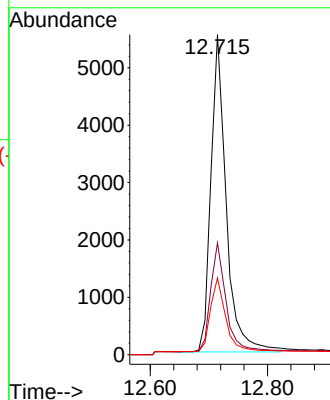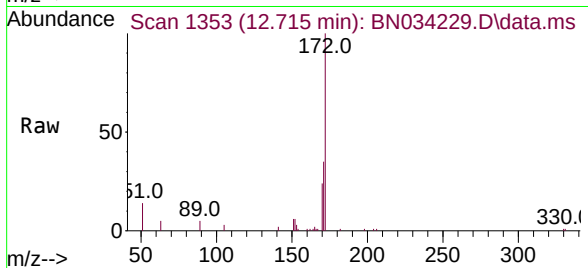

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.846 min Scan# 1722
Delta R.T. 0.003 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45

Tgt Ion:188 Resp: 17941
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 16.5 7.4 11.0#


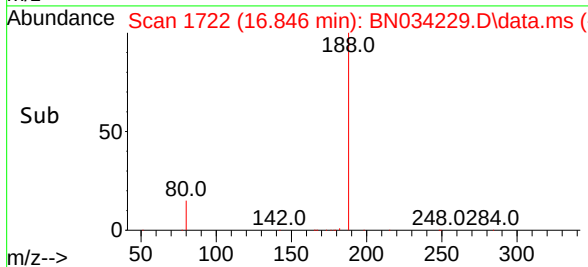
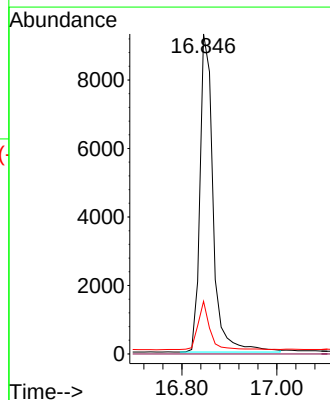
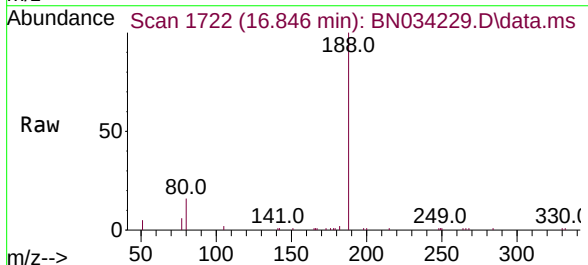


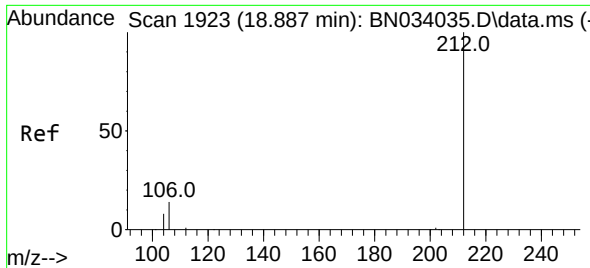

#27
Fluoranthene-d10
Concen: 0.334 ng
RT: 18.890 min Scan# 1923
Delta R.T. 0.003 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45




Instrument :
BNA_N
ClientSampleId :
BPOW6-8-HYD-20240910RE


Tgt Ion	Ratio	Lower	Upper
212	100		
106	16.6	13.4	20.2
104	9.3	7.8	11.6

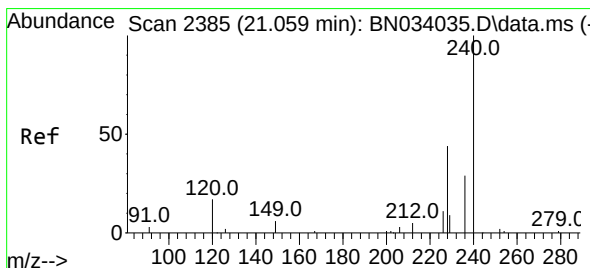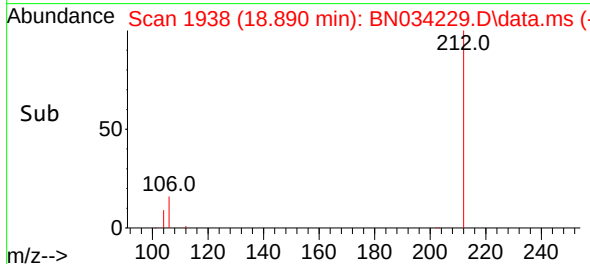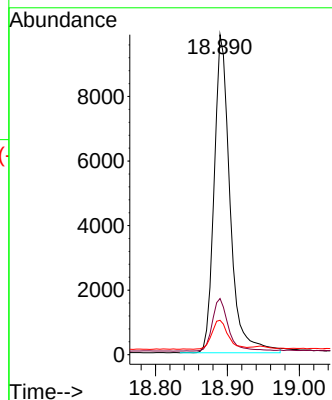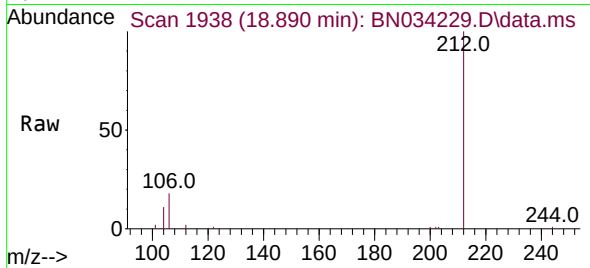

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.062 min Scan# 2400
Delta R.T. 0.003 min
Lab File: BN034229.D
Acq: 25 Sep 2024 17:45

Tgt Ion	Ratio	Lower	Upper
240	100		
120	22.5	13.5	20.3
236	30.1	23.4	35.0


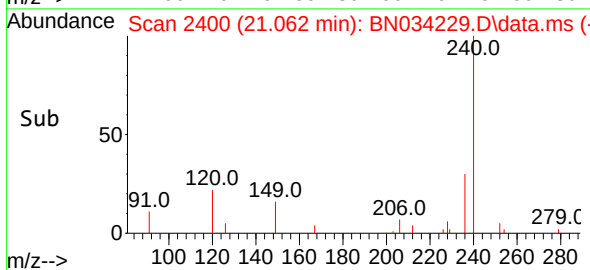
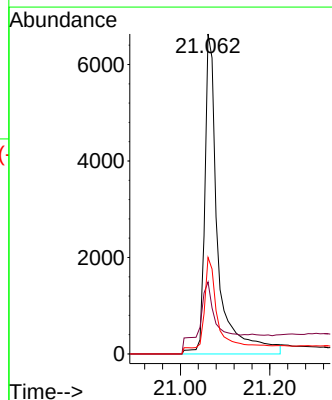
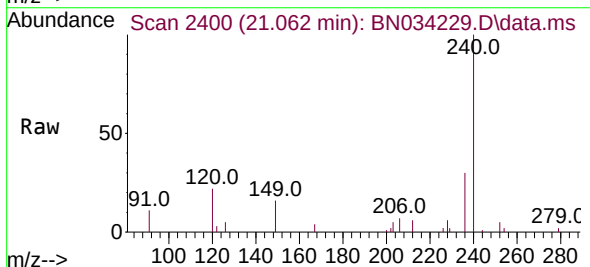


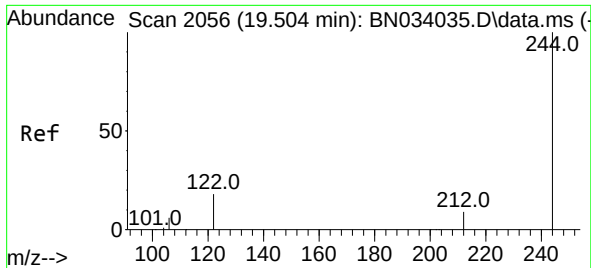

#31
 Terphenyl-d14
 Concen: 0.477 ng
 RT: 19.508 min Scan# 2056
 Delta R.T. 0.003 min
 Lab File: BN034229.D
 Acq: 25 Sep 2024 17:45




Instrument :
 BNA_N
 ClientSampleId :
 BPOW6-8-HYD-20240910RE


Tgt Ion:244 Resp: 12510
 Ion Ratio Lower Upper
 244 100
 212 9.6 7.8 11.6
 122 18.9 14.8 22.2

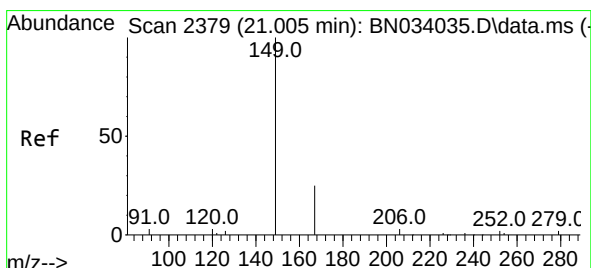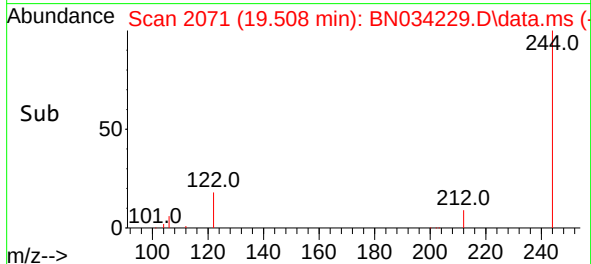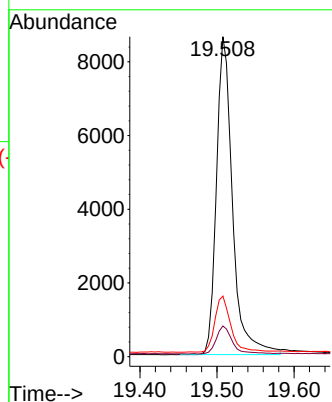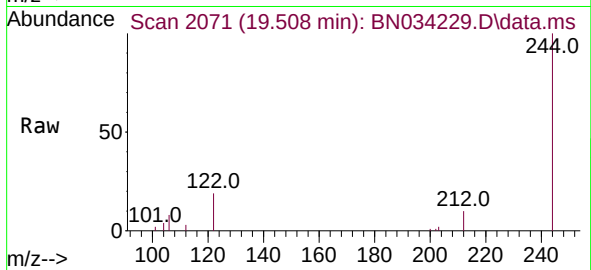

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.291 ng
 RT: 21.008 min Scan# 2394
 Delta R.T. 0.003 min
 Lab File: BN034229.D
 Acq: 25 Sep 2024 17:45

Tgt Ion:149 Resp: 5036
 Ion Ratio Lower Upper
 149 100
 167 24.3 19.9 29.9
 279 8.6 4.6 6.8#

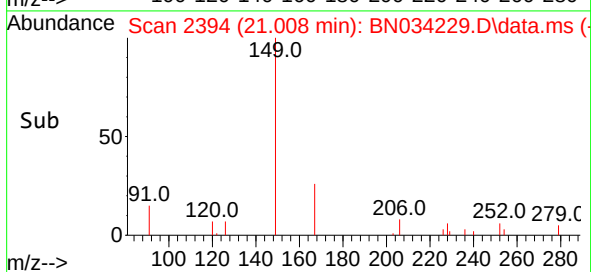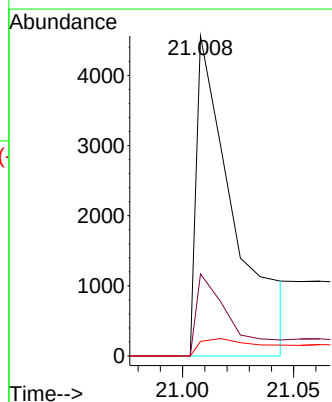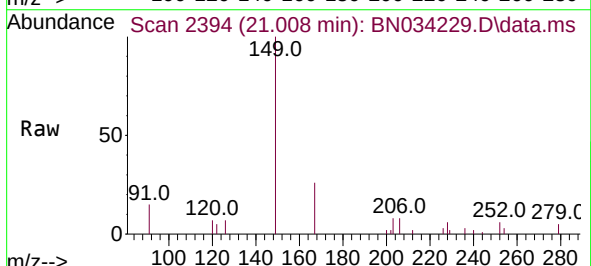

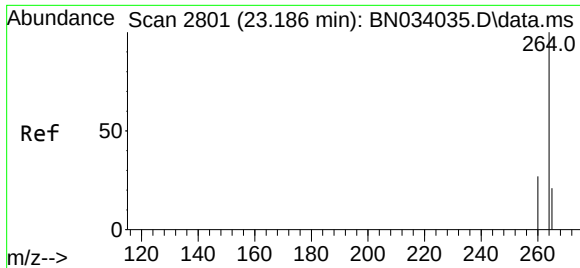

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.198 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: BN034229.D
 Acq: 25 Sep 2024 17:45

Instrument :
 BNA_N
 ClientSampleId :
 BPOW6-8-HYD-20240910RE

Tgt Ion:	264	Resp:	10591
Ion Ratio	Lower	Upper	
264	100		
260	26.6	21.7	32.5
265	123.7	52.1	78.1#

