
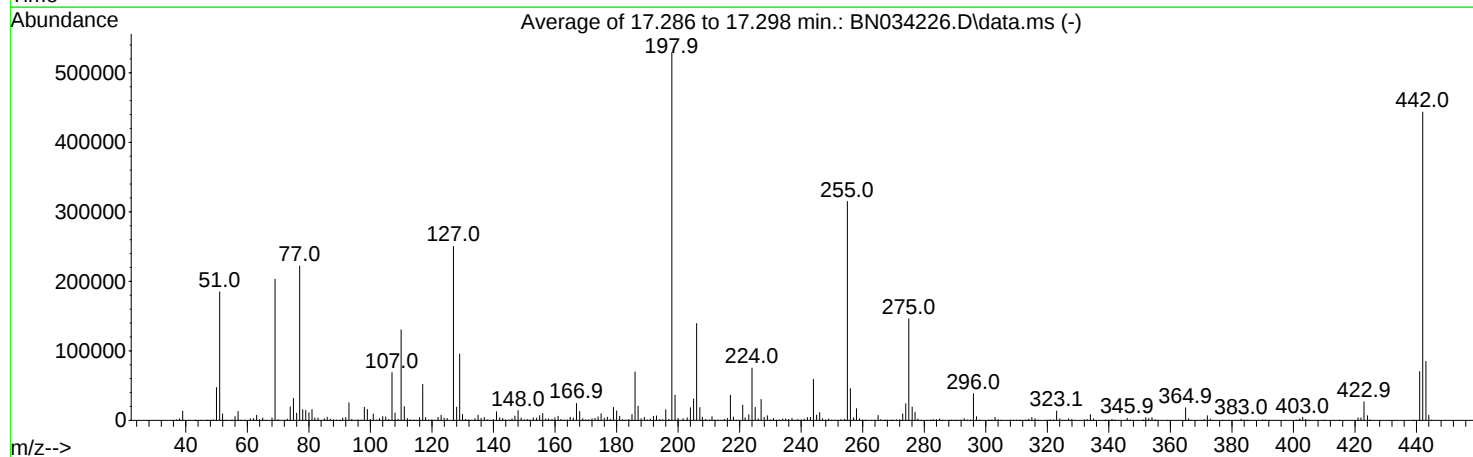


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092524\
Data File : BN034226.D
Acq On : 25 Sep 2024 15:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 26 03:57:12 2024

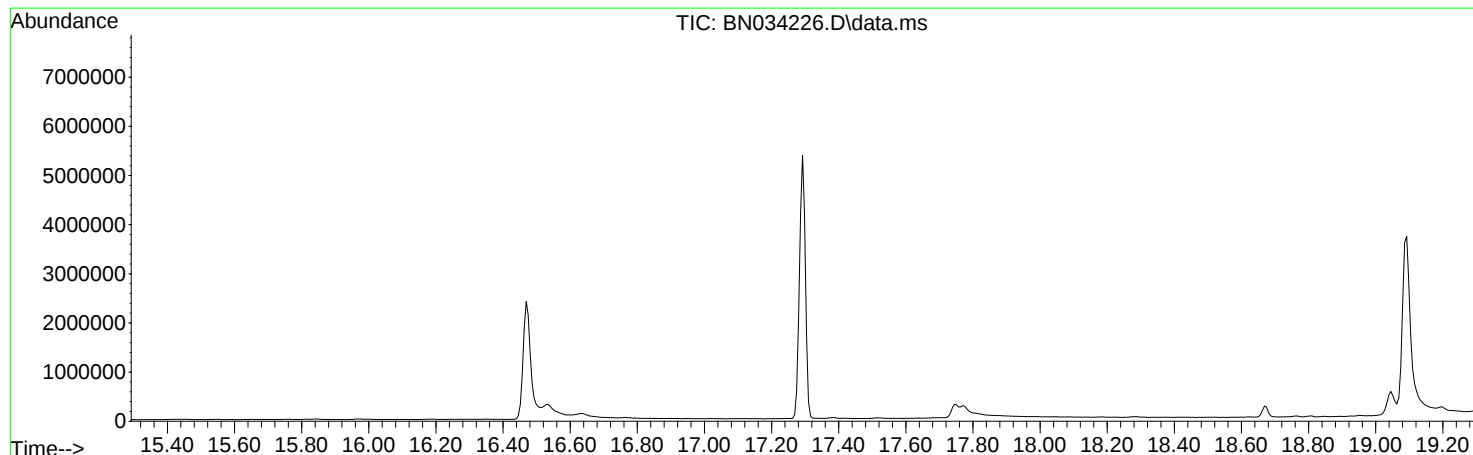

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	184848	PASS
68	69	0.00	2	1.7	3401	PASS
69	198	0.00	100	38.4	203003	PASS
70	69	0.00	2	0.5	1045	PASS
127	198	10	80	47.3	250347	PASS
197	198	0.00	2	0.2	1007	PASS
198	198	100	100	100.0	529301	PASS
199	198	5	9	6.9	36424	PASS
275	198	10	60	27.6	146235	PASS
365	198	1	100	3.4	18230	PASS
441	198	0.01	100	13.3	70152	PASS
442	442	50	100	100.0	443691	PASS
443	442	15	24	19.1	84928	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/25/2024	BNA_N	<u>BN034226.D</u>
Compound Name	Response	Retention Time
DDT	1815985	20.339
DDD	80989	19.892
DDE	2553	19.38
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
83542	1899527	4.40

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092524\
Data File : BN034226.D
Acq On : 25 Sep 2024 15:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 05:44:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 26 05:44:15 2024
Response via : Initial Calibration

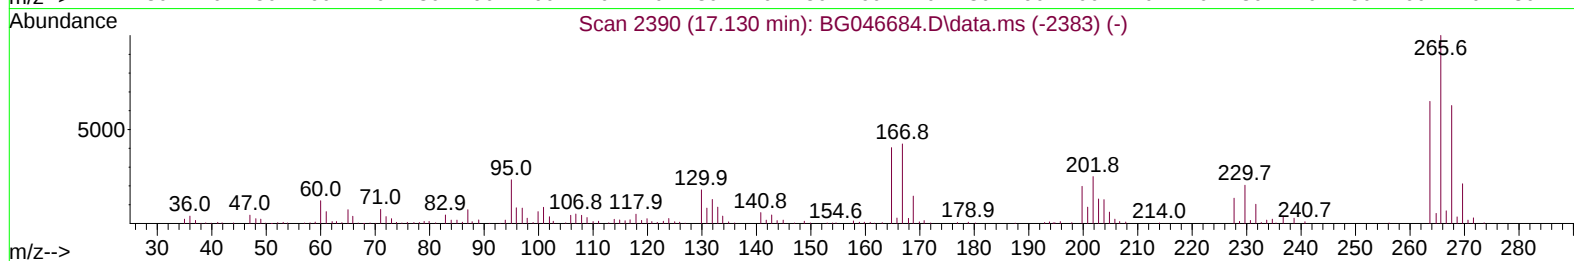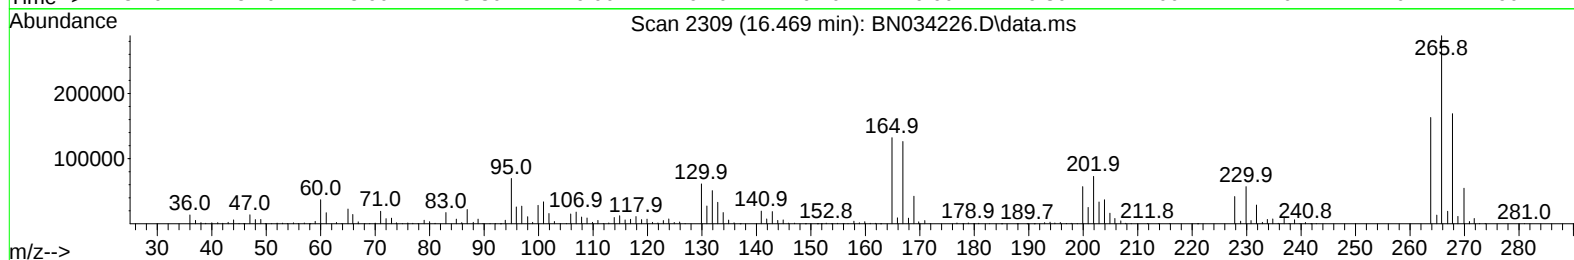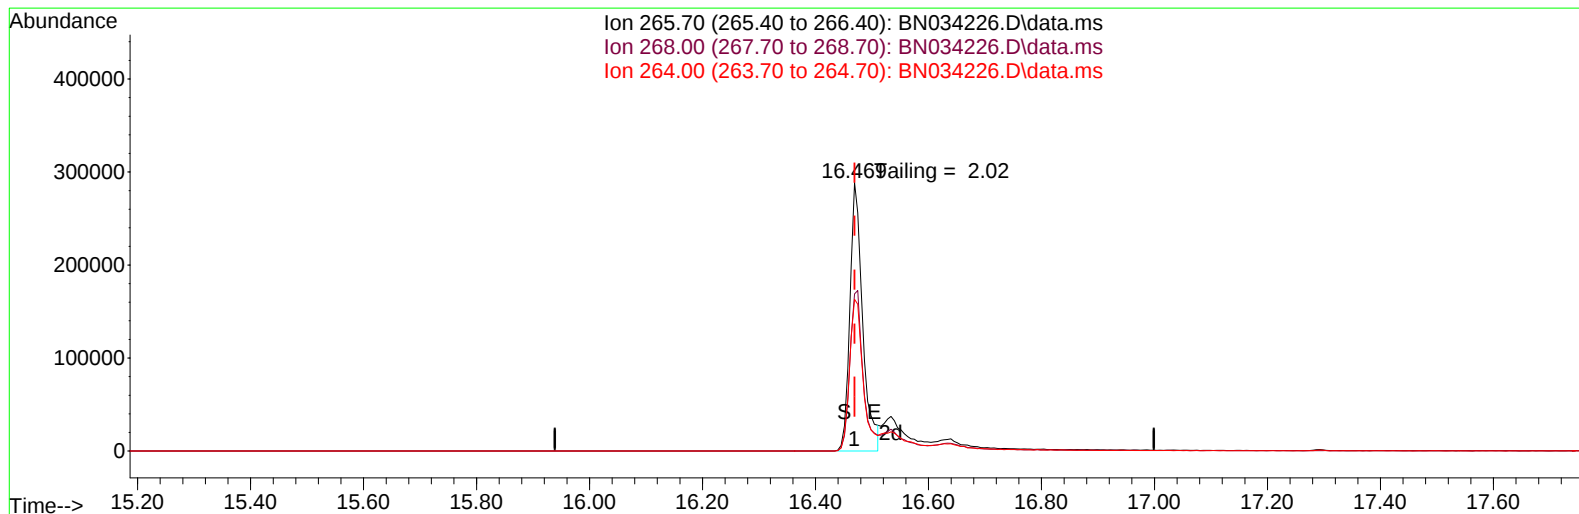

TIC: BN034226.D\data.ms

(70) Pentachlorophenol (C)

16.469min (0.000) 17410.53 ng




response 463324

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.57
264.00	61.60	56.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092524\
Data File : BN034226.D
Acq On : 25 Sep 2024 15:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 05:44:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 26 05:44:15 2024
Response via : Initial Calibration

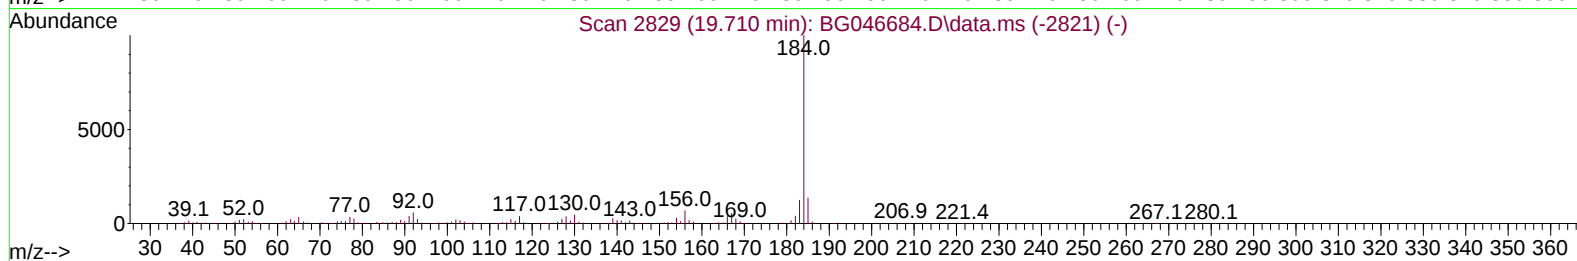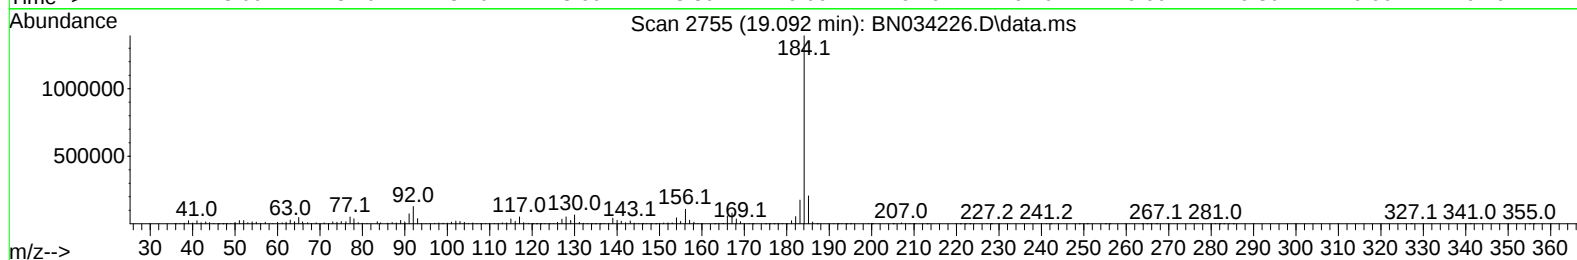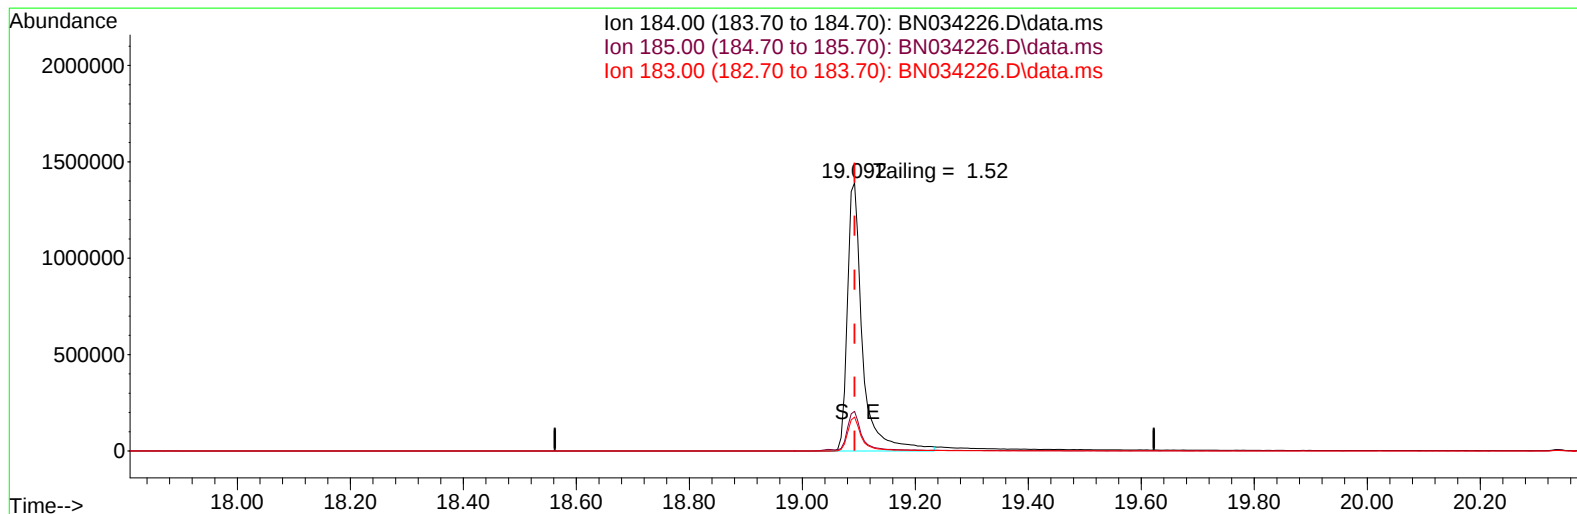

TIC: BN034226.D\data.ms

(77) Benzidine

19.092min (0.000) 0.00 ng

response 2707602

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.81
183.00	13.20	12.63
0.00	0.00	0.00