
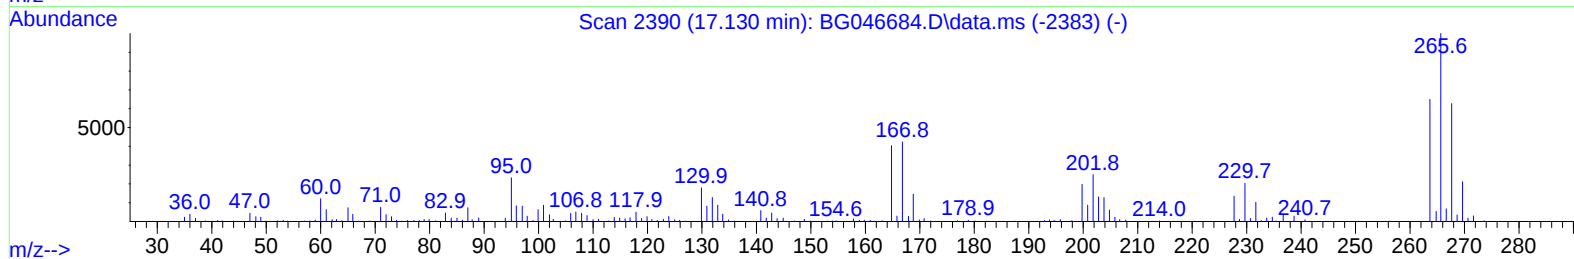
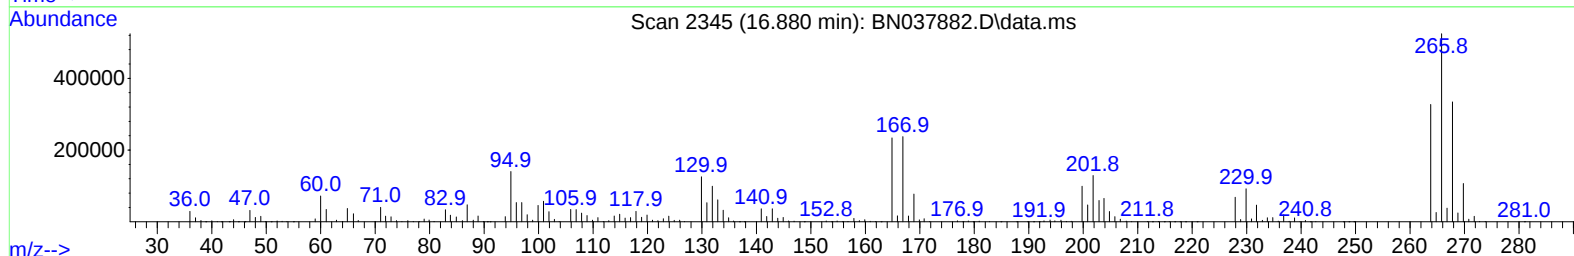


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037882.D
Acq On : 25 Sep 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 13:12:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

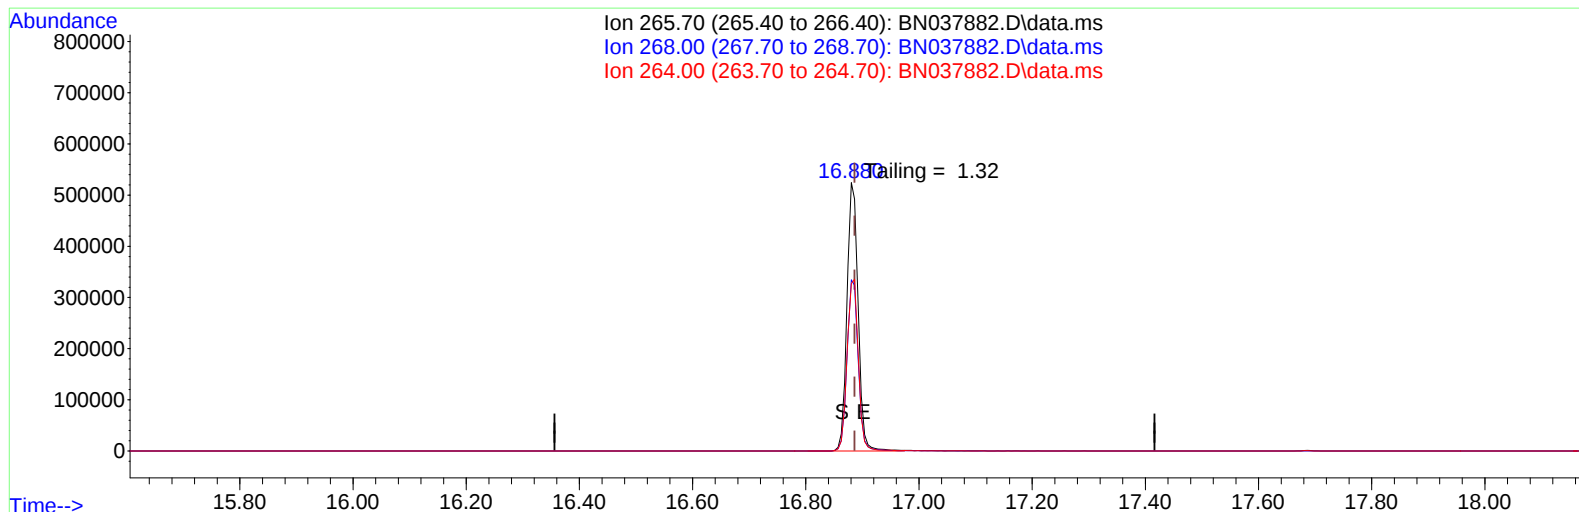

TIC: BN037882.D\data.ms

(70) Pentachlorophenol (C)




16.880min (-0.006) 31548.12 ng

response 718482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.80
264.00	61.60	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037882.D
Acq On : 25 Sep 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 13:12:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

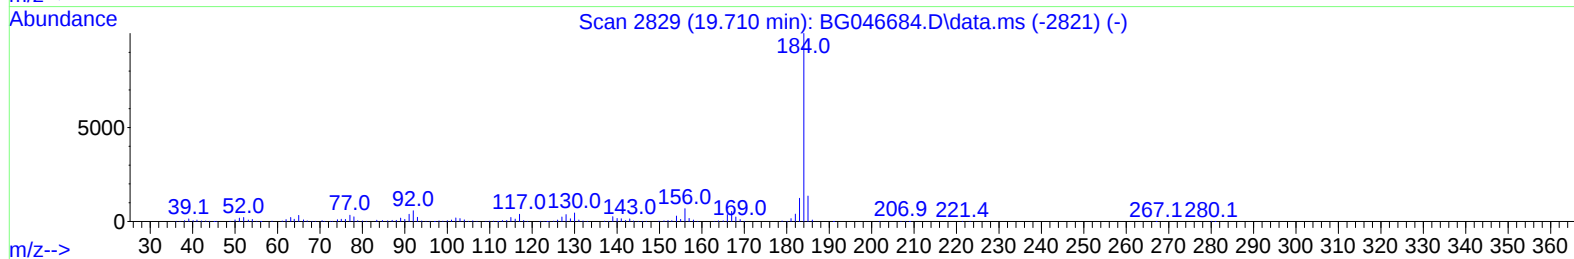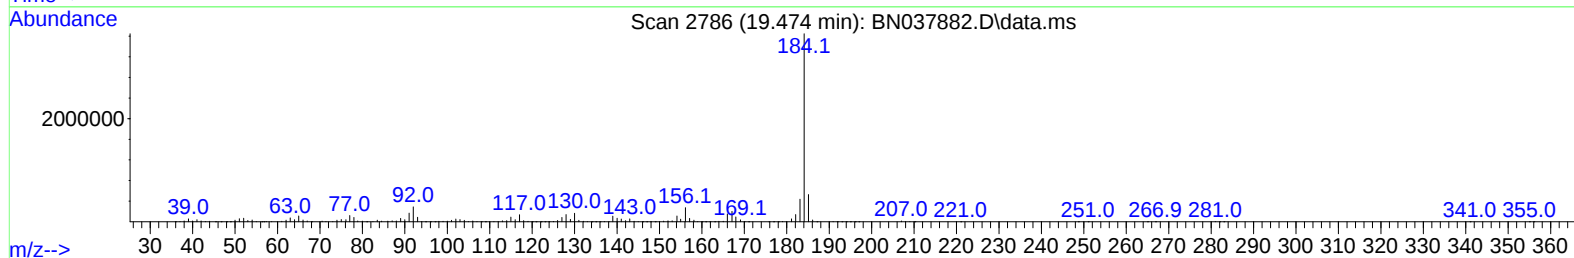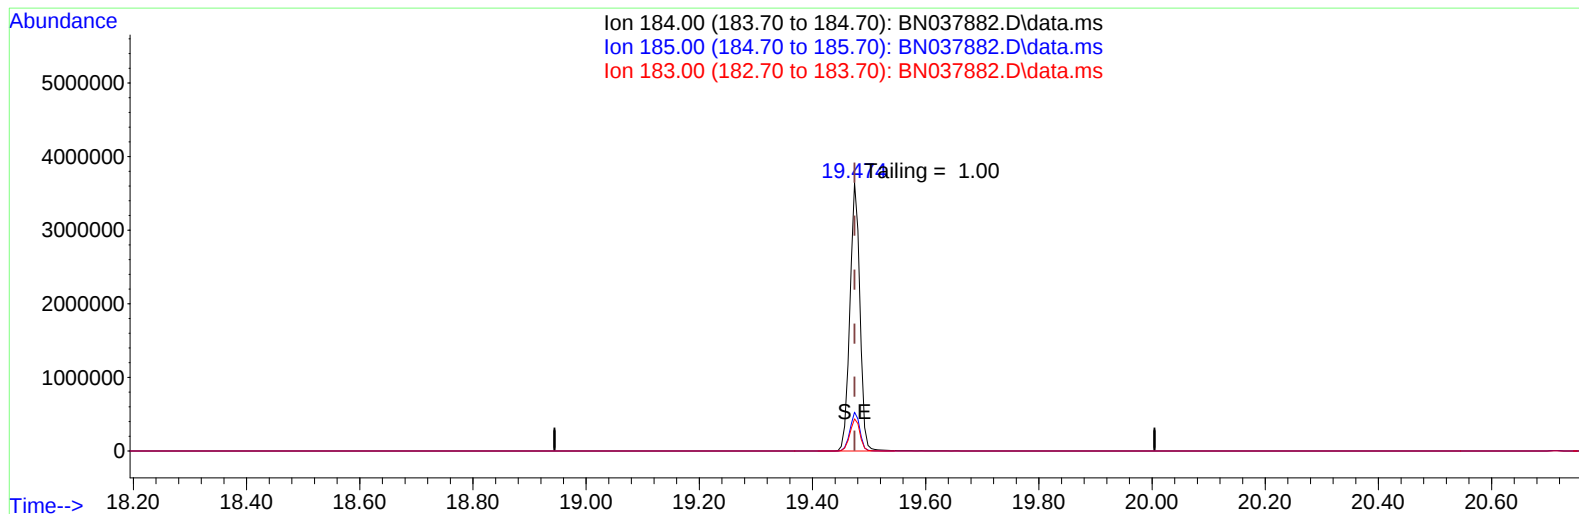

TIC: BN037882.D\data.ms

(77) Benzidine

19.474min (+ 0.000) 0.00 ng

response 4502688

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	12.03
0.00	0.00	0.00