
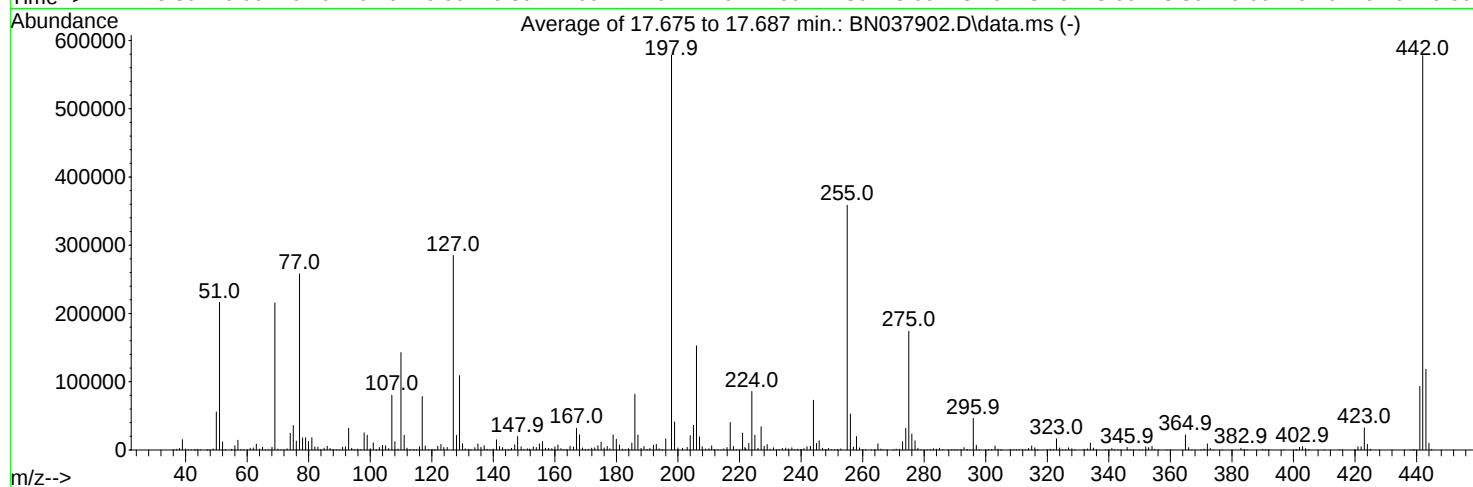


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037902.D
Acq On : 25 Sep 2025 23:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

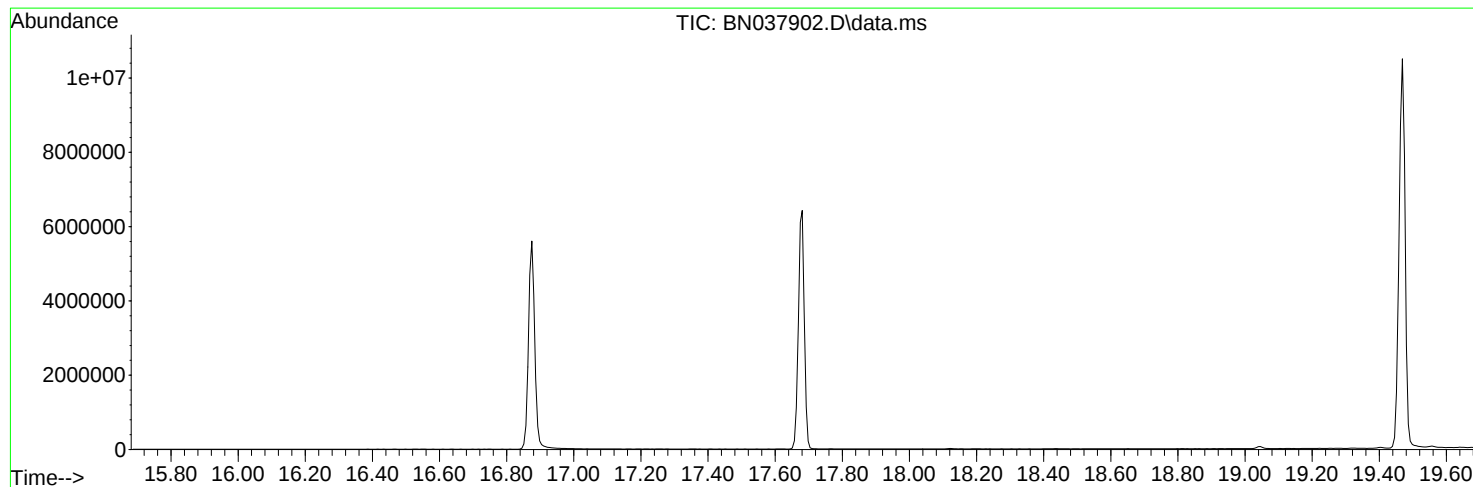




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	4059	PASS
69	69	100	100	100.0	215531	PASS
70	69	0.00	2	0.6	1236	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	578603	PASS
199	198	5	9	7.1	40861	PASS
365	198	1	100	3.8	22109	PASS
441	443	0.01	150	78.7	92987	PASS
442	442	100	100	100.0	577899	PASS
443	442	15	24	20.5	118221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037902.D
Acq On : 25 Sep 2025 23:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 00:18:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

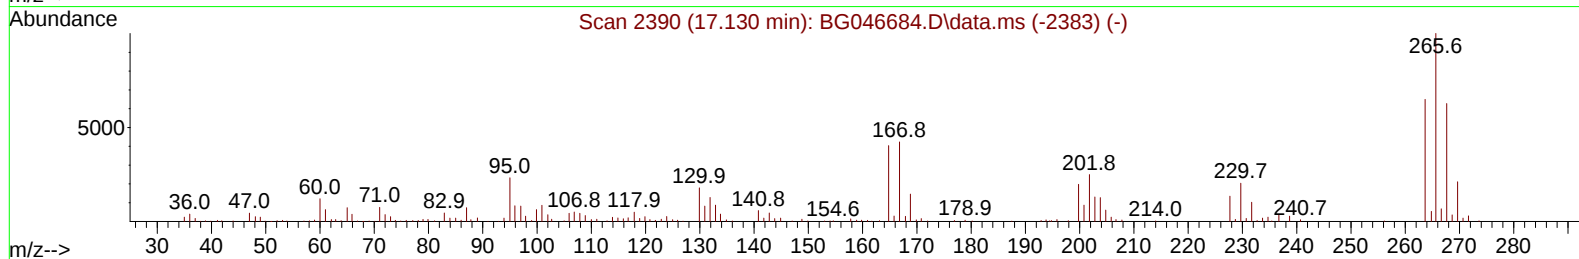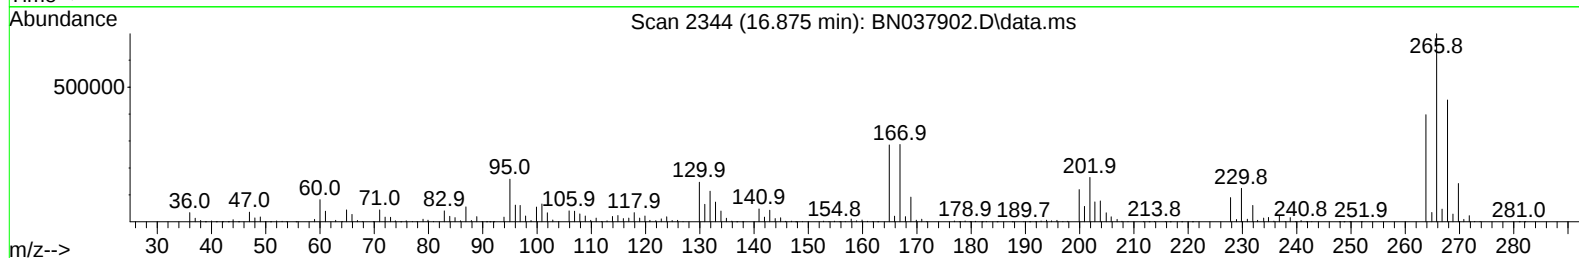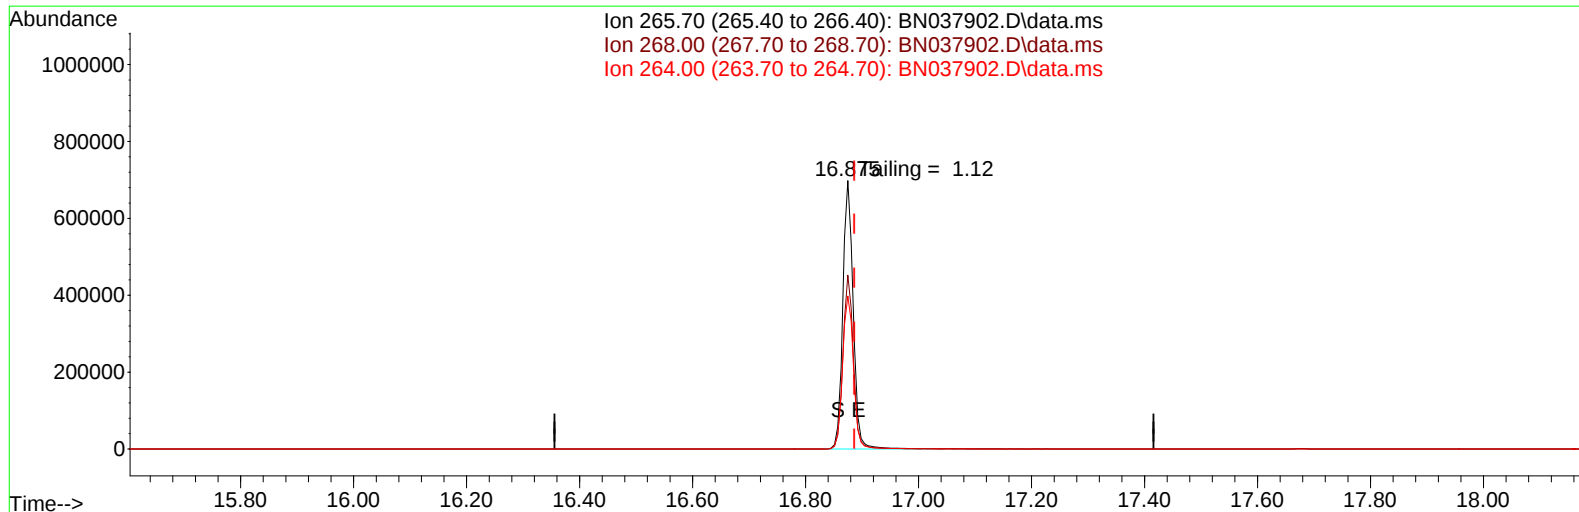

TIC: BN037902.D\data.ms

(70) Pentachlorophenol (C)

16.875min (-0.011) 30660.06 ng




response 887138

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.77
264.00	61.60	56.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092525\
Data File : BN037902.D
Acq On : 25 Sep 2025 23:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 00:18:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

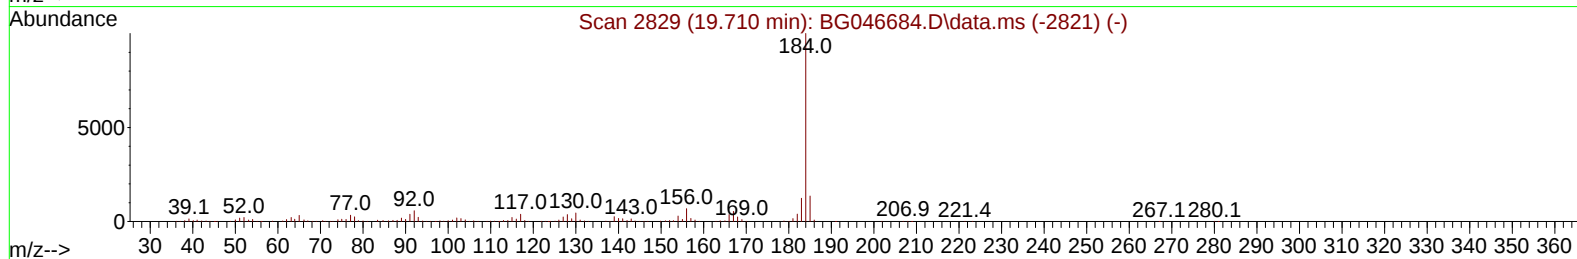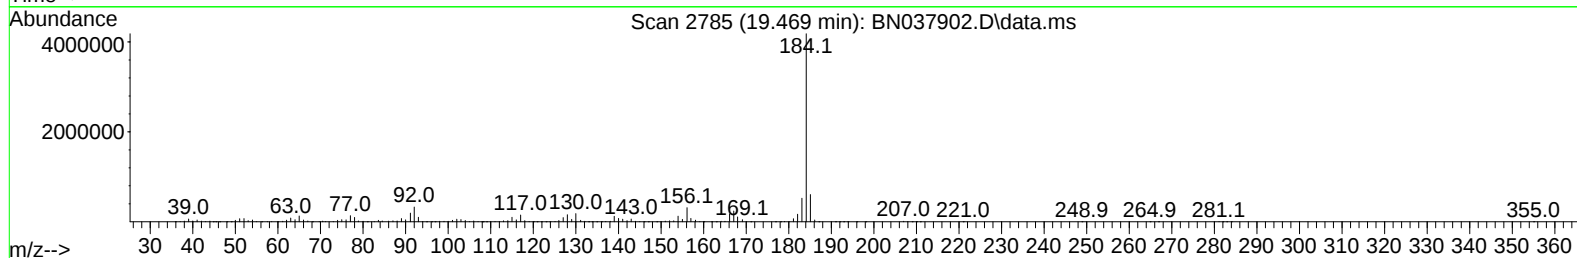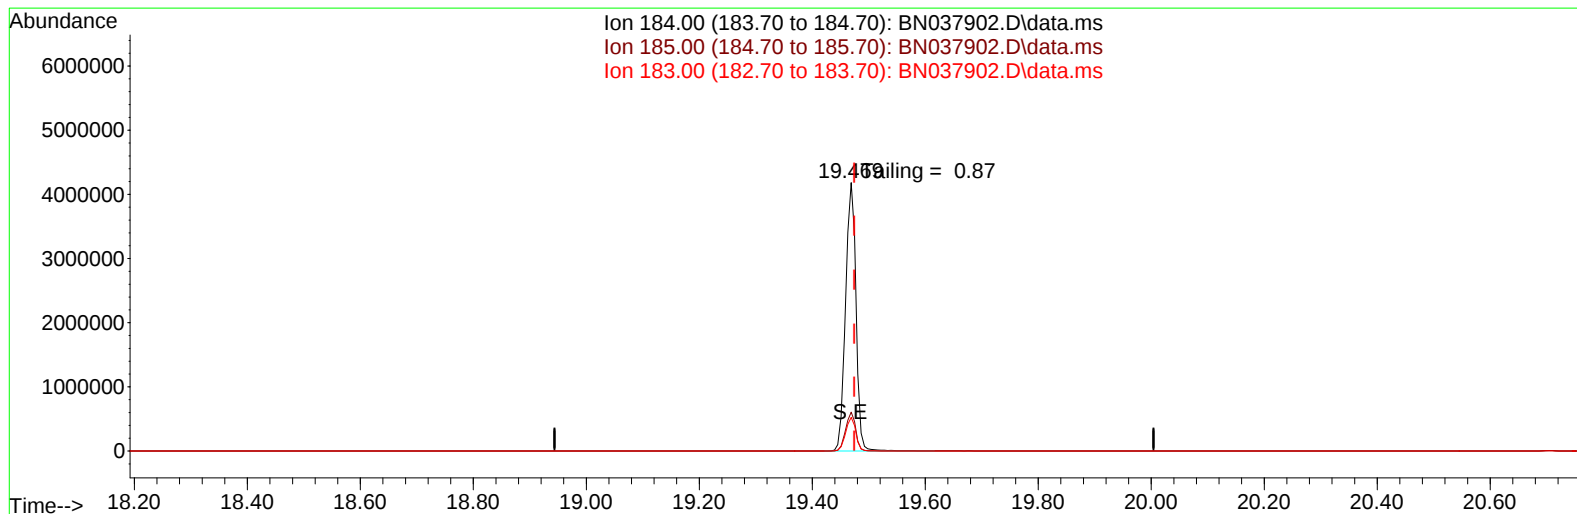

TIC: BN037902.D\data.ms

(77) Benzidine

19.469min (-0.005) 0.00 ng

response 5355817

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/25/2025	BNA_N	<u>BN037902.D</u>
Compound Name	Response	Retention Time
DDT	2417254	20.716
DDD	13785	20.263
DDE	387	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14172	2431426	0.58

Instrument :
BNA_N
ClientSampleId :
DFTPP