

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027854.D
 Acq On : 26 Sep 2023 10:05
 Operator : MA/JU
 Sample : PB155611BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK611

Quant Time: Sep 27 02:59:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	3814	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	13610	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	9304	0.400	ng/ul	0.01
13) Phenanthrene-d10	17.358	188	20951	0.400	ng/ul	0.02
17) Chrysene-d12	21.542	240	20041	0.400	ng/ul	0.02
23) Perylene-d12	24.021	264	24171	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	31016	6.456	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	7684	0.373	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	20990	0.343	ng/ul	0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.600	166	2657	0.064	ng/ul#	15
20) Pyrene	19.752	202	2811	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.857	252	7025	0.081	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027854.D
Acq On : 26 Sep 2023 10:05
Operator : MA/JU
Sample : PB155611BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK611

Quant Time: Sep 27 02:59:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration




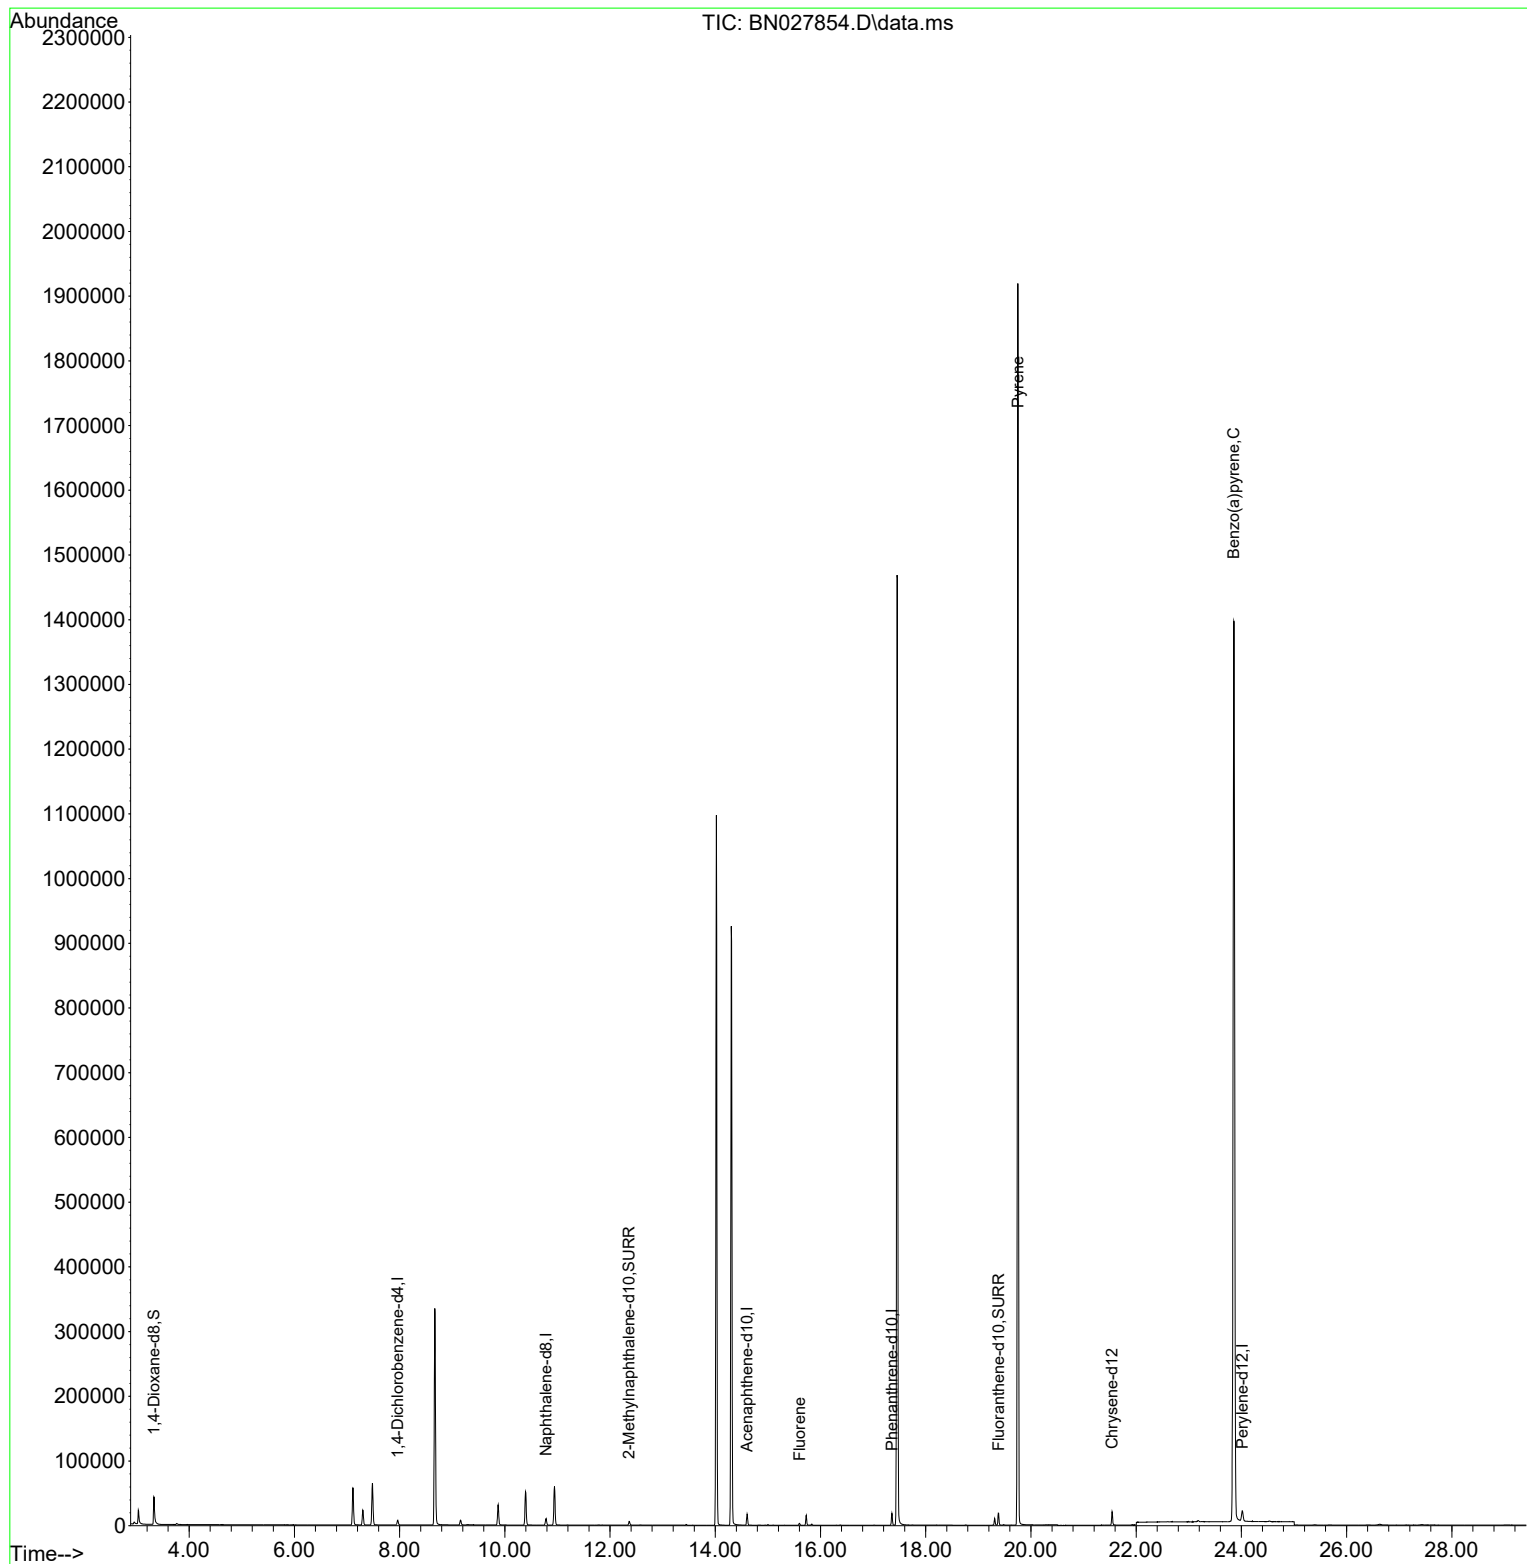


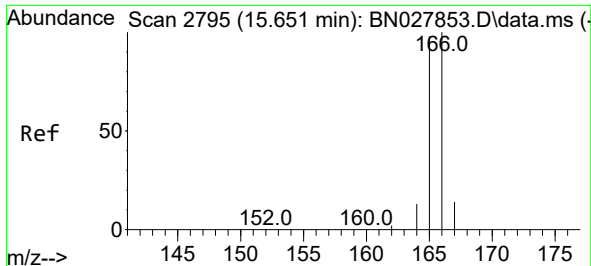

#12
Fluorene
Concen: 0.064 ng/ul
RT: 15.600 min Scan# 21
Delta R.T. -0.038 min
Lab File: BN027854.D
Acq: 26 Sep 2023 10:05




Instrument :
BNA_N
ClientSampleId :
SBLK611


Tgt Ion:166 Resp: 2657
Ion Ratio Lower Upper
166 100
165 8.8 78.0 117.0#
167 36.7 11.4 17.2#

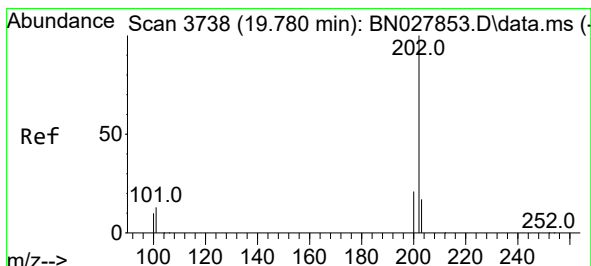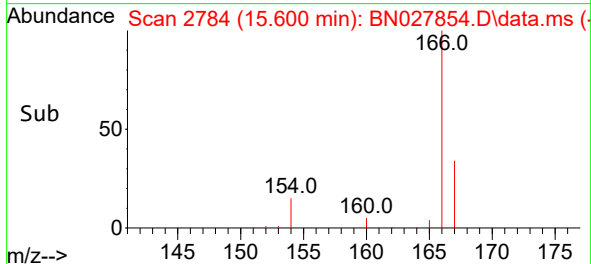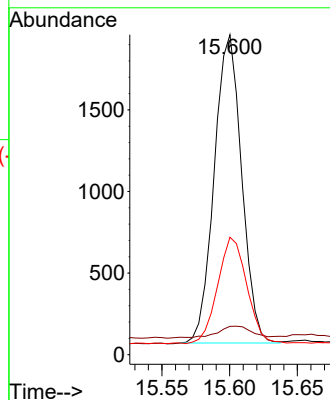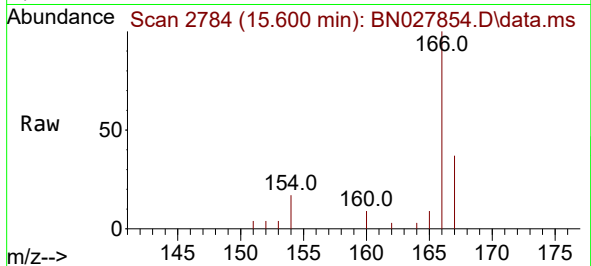

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.752 min Scan# 3732
Delta R.T. -0.010 min
Lab File: BN027854.D
Acq: 26 Sep 2023 10:05


Tgt Ion:202 Resp: 2811
Ion Ratio Lower Upper
202 100
101 156.6 11.4 17.0#
100 1109.1 9.1 13.7#

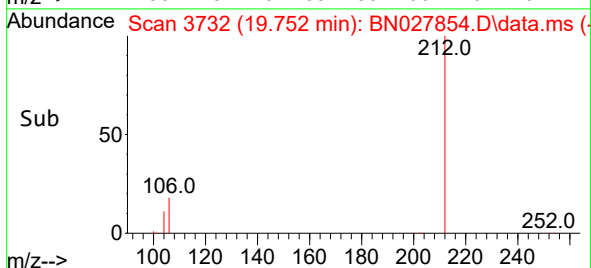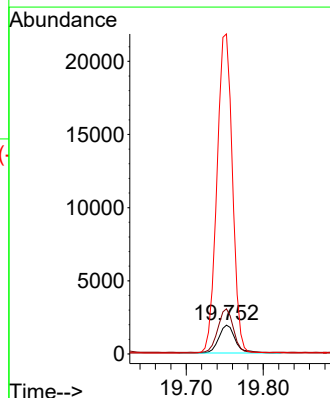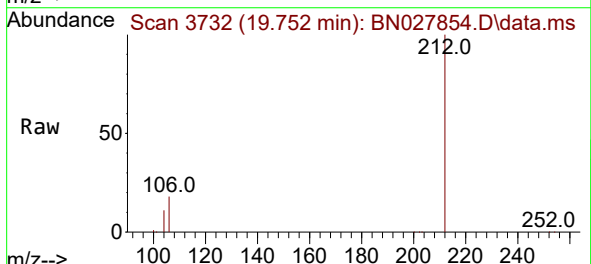

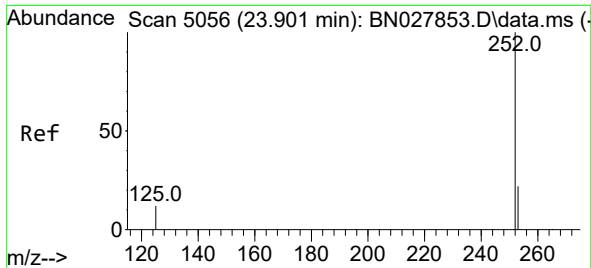

#26
 Benzo(a)pyrene
 Concen: 0.081 ng/ul
 RT: 23.857 min Scan# 5041
 Delta R.T. -0.044 min
 Lab File: BN027854.D
 Acq: 26 Sep 2023 10:05

Instrument :
 BNA_N
 ClientSampleId :
 SBLK611

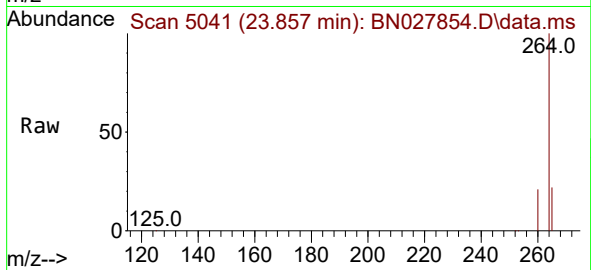

Tgt Ion:252 Resp: 7025
 Ion Ratio Lower Upper
 252 100
 253 48.8 21.9 32.9#
 125 39.7 15.5 23.3#

