

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027863.D
 Acq On : 26 Sep 2023 16:06
 Operator : MA/JU
 Sample : PB155614BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK614

Quant Time: Sep 27 03:00:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	2866	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	10402	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	6945	0.400	ng/ul	0.01
13) Phenanthrene-d10	17.359	188	15955	0.400	ng/ul	0.02
17) Chrysene-d12	21.542	240	15361	0.400	ng/ul	0.02
23) Perylene-d12	24.018	264	19469	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	25402	7.036	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	6197	0.393	ng/ul	0.01
18) Fluoranthene-d10	19.385	212	16821	0.359	ng/ul	0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.600	166	2123	0.069	ng/ul#	15
20) Pyrene	19.752	202	2301	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.857	252	5957	0.085	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027863.D
Acq On : 26 Sep 2023 16:06
Operator : MA/JU
Sample : PB155614BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK614

Quant Time: Sep 27 03:00:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration




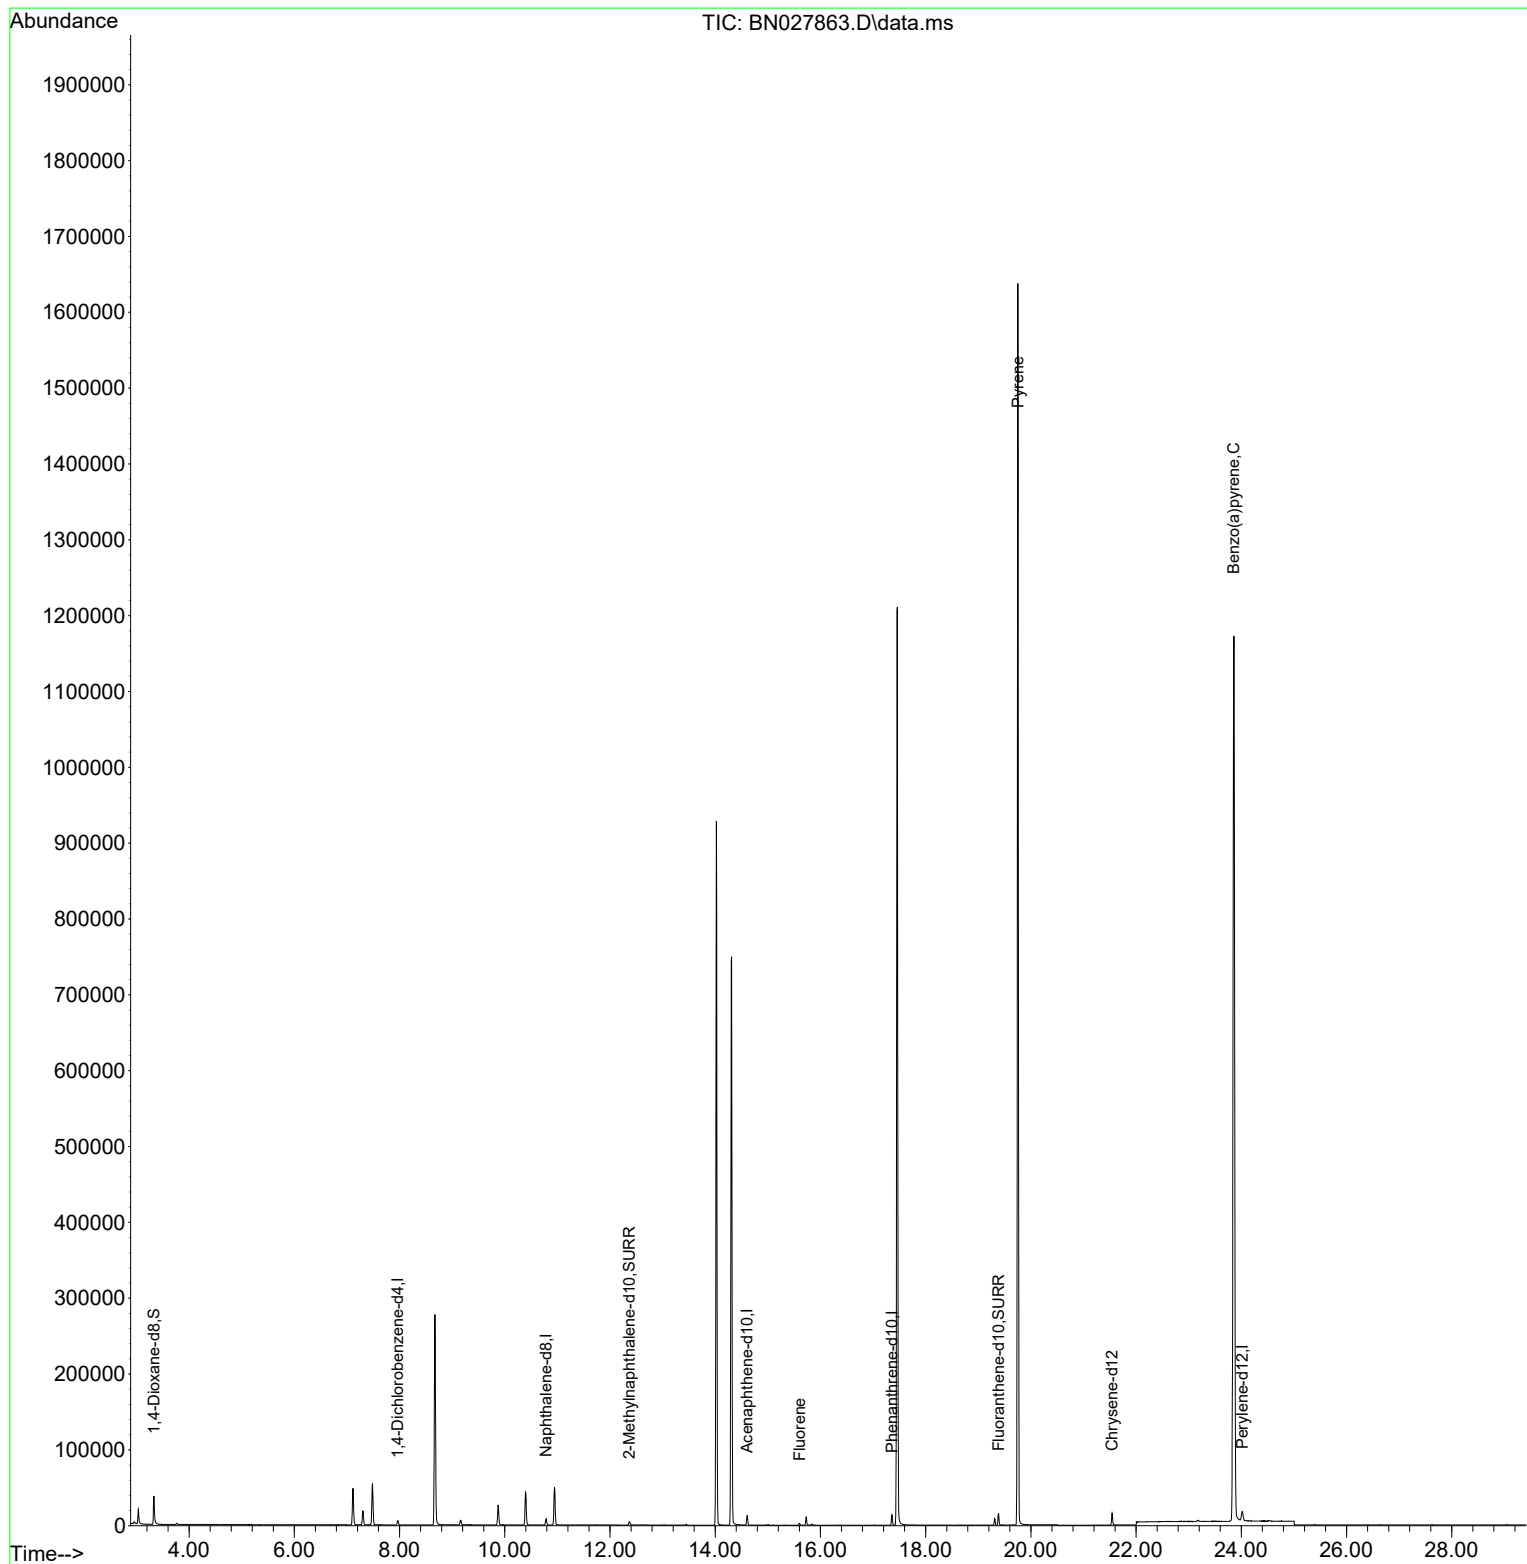


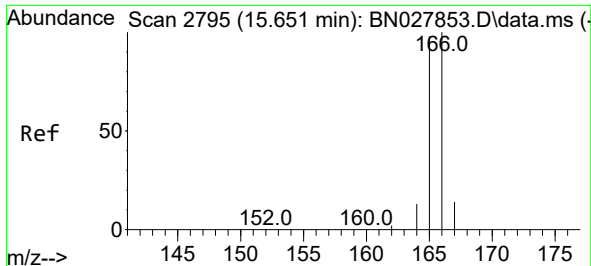

#12
Fluorene
Concen: 0.069 ng/ul
RT: 15.600 min Scan# 21
Delta R.T. -0.038 min
Lab File: BN027863.D
Acq: 26 Sep 2023 16:06




Instrument :
BNA_N
ClientSampleId :
SBLK614


Tgt Ion:166 Resp: 2123
Ion Ratio Lower Upper
166 100
165 9.6 78.0 117.0#
167 37.8 11.4 17.2#

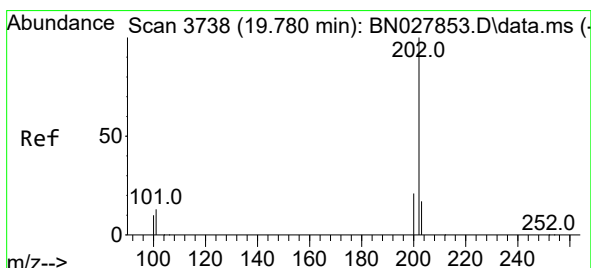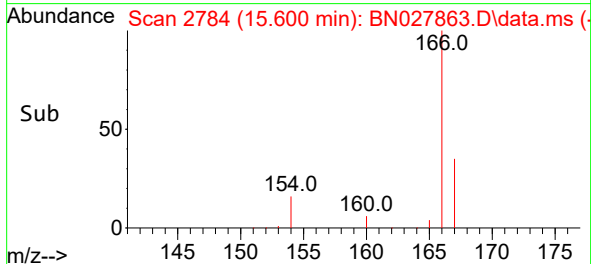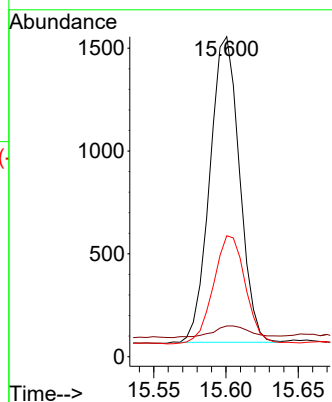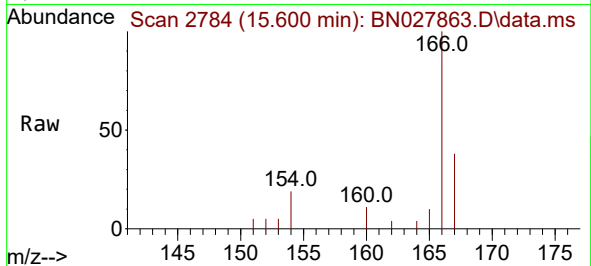

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.752 min Scan# 3732
Delta R.T. -0.010 min
Lab File: BN027863.D
Acq: 26 Sep 2023 16:06


Tgt Ion:202 Resp: 2301
Ion Ratio Lower Upper
202 100
101 153.3 11.4 17.0#
100 1097.8 9.1 13.7#

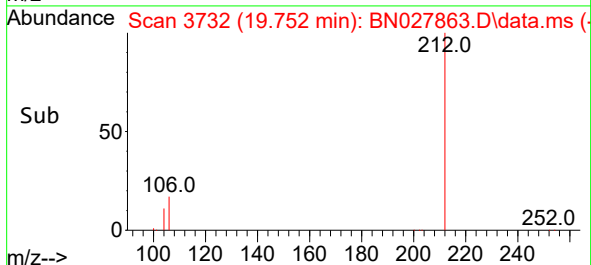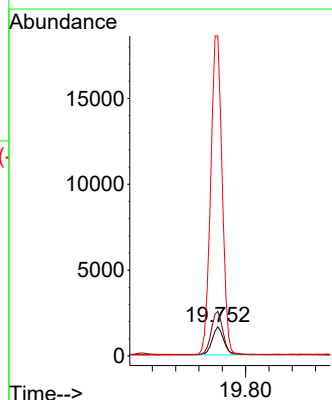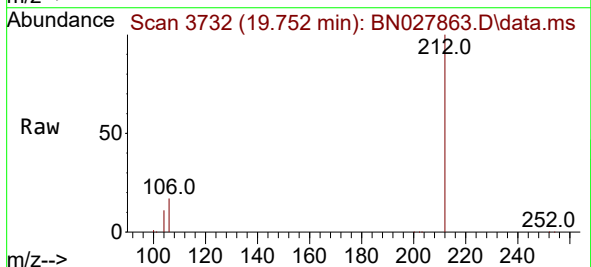

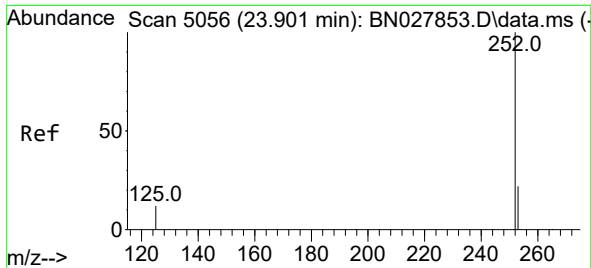

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.857 min Scan# 5056
Delta R.T. -0.043 min
Lab File: BN027863.D
Acq: 26 Sep 2023 16:06

Instrument :
BNA_N
ClientSampleId :
SBLK614

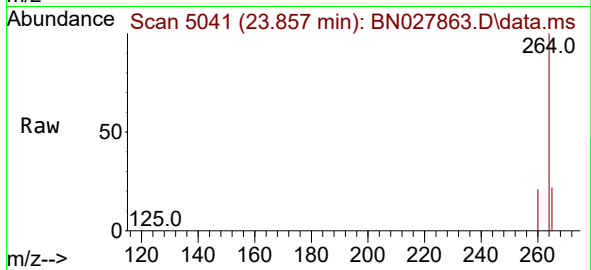

Tgt Ion:252 Resp: 5957
Ion Ratio Lower Upper
252 100
253 50.9 21.9 32.9#
125 41.7 15.5 23.3#

