

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027898.D
 Acq On : 27 Sep 2023 14:20
 Operator : MA/JU
 Sample : PB155730BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK730

Quant Time: Sep 28 00:00:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	2917	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	10968	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	7492	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	16915	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	16893	0.400	ng/ul	0.00
23) Perylene-d12	24.009	264	19965	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	21523	5.858	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	5300	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	14438	0.280	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.748	202	2134	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.851	252	5367	0.075	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027898.D
Acq On : 27 Sep 2023 14:20
Operator : MA/JU
Sample : PB155730BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK730

Quant Time: Sep 28 00:00:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

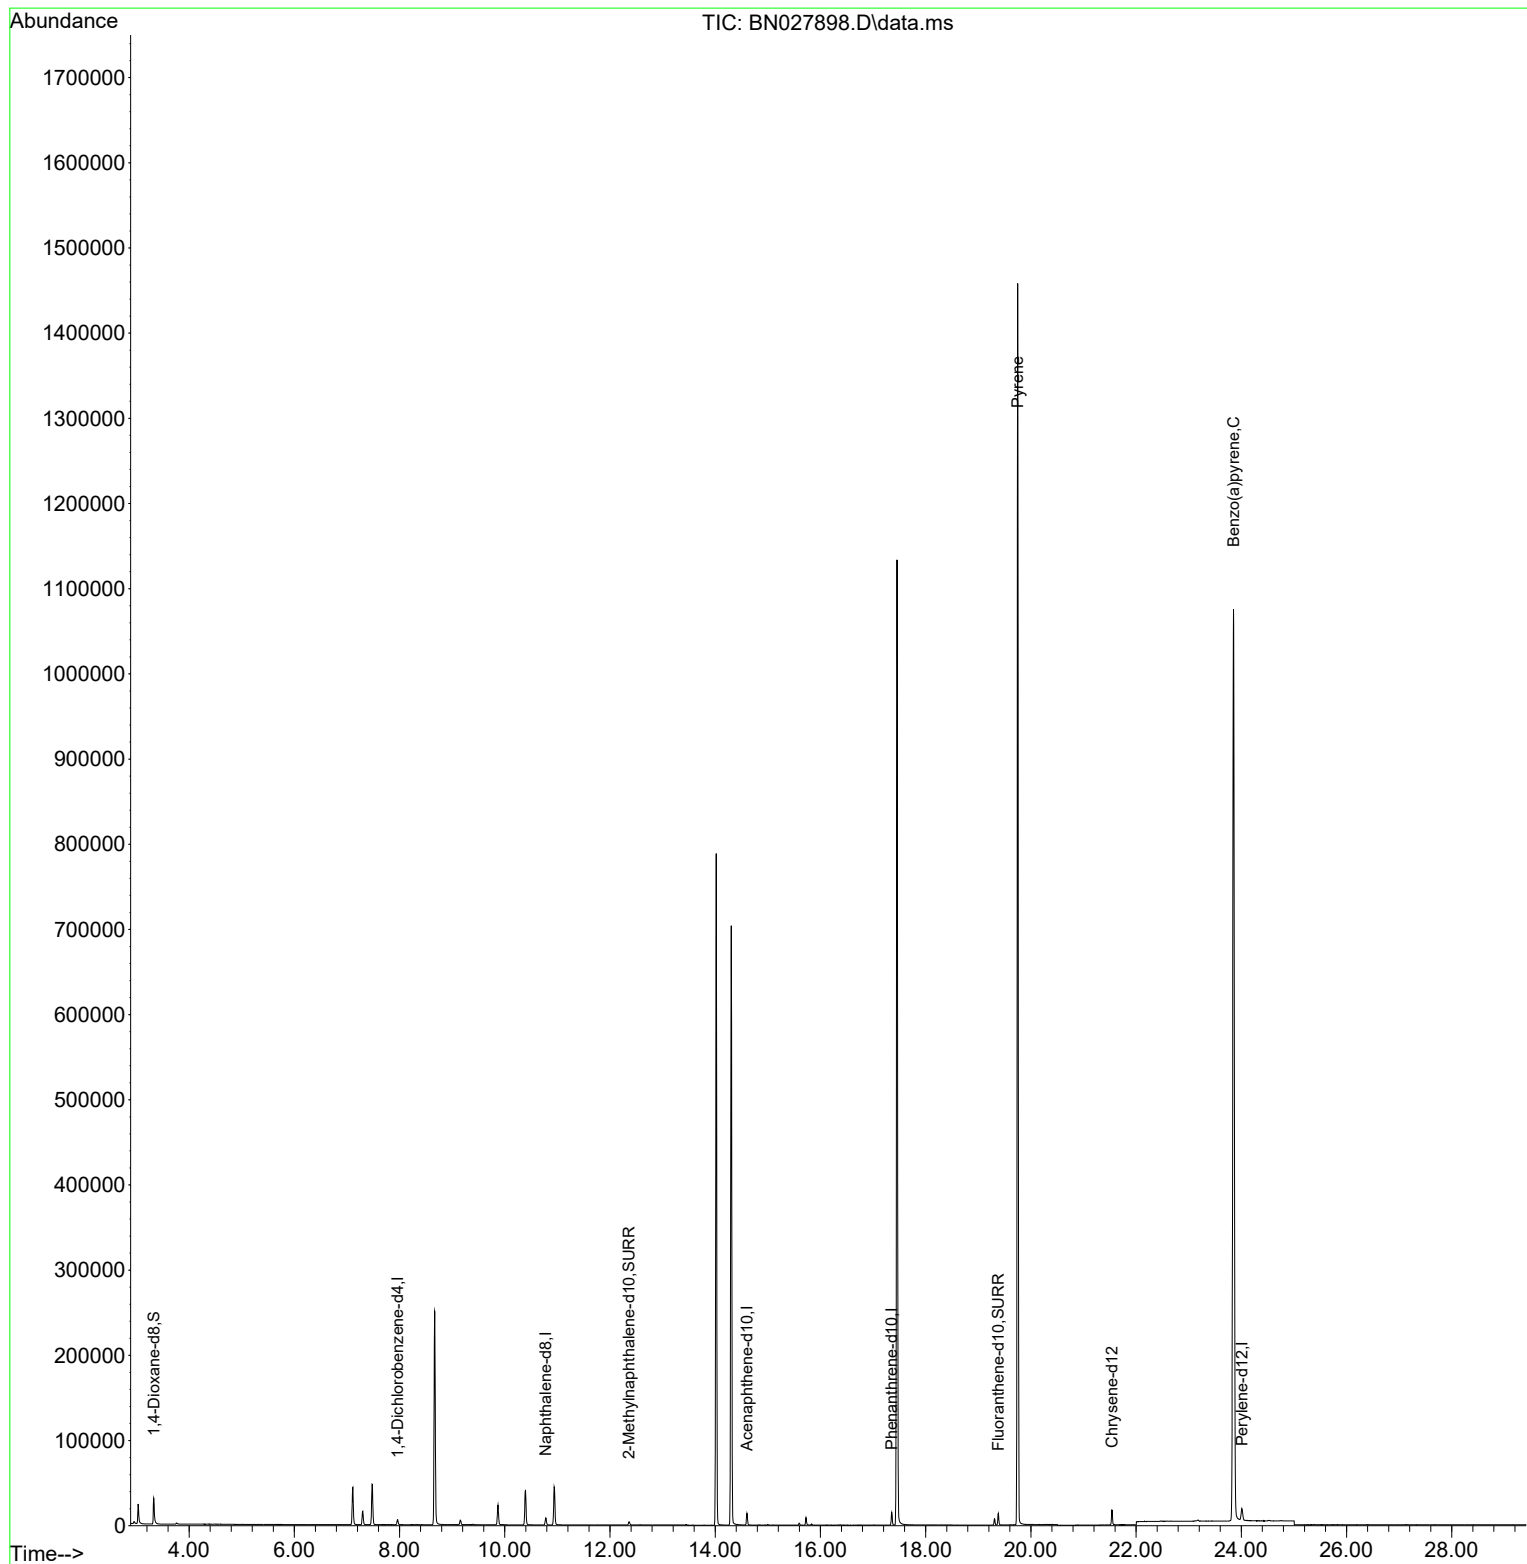

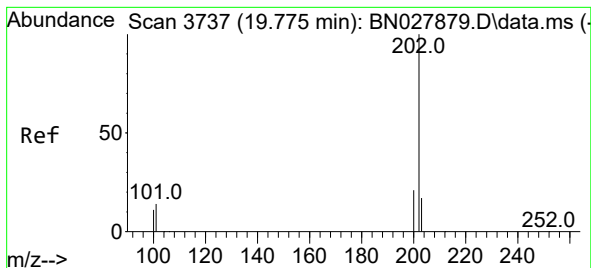

#20

Pyrene

Concen: 0.030 ng/ul

RT: 19.748 min Scan# 31

Delta R.T. -0.028 min

Lab File: BN027898.D

Acq: 27 Sep 2023 14:20

Instrument :

BNA_N

ClientSampleId :

SBLK730





Tgt Ion:202 Resp: 2134

Ion Ratio Lower Upper

202 100

101 157.2 11.4 17.0#

100 1132.5 9.1 13.7#

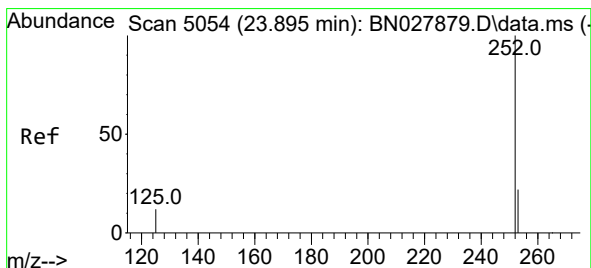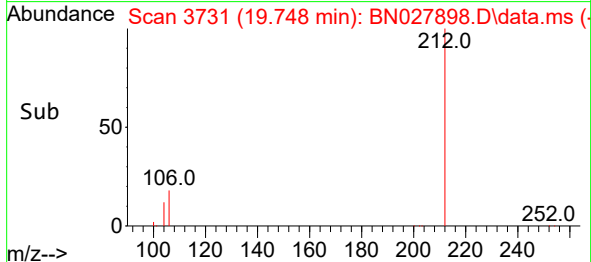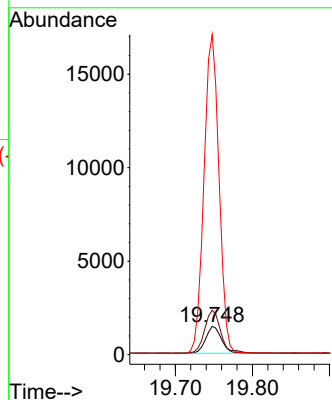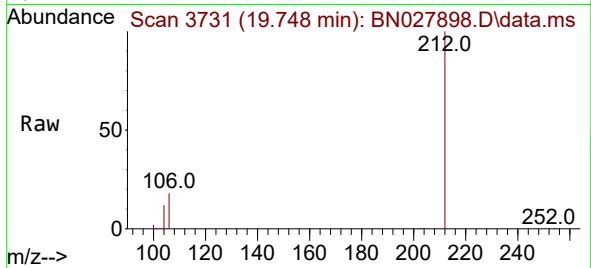

#26

Benzo(a)pyrene

Concen: 0.075 ng/ul

RT: 23.851 min Scan# 5039

Delta R.T. -0.044 min

Lab File: BN027898.D

Acq: 27 Sep 2023 14:20

Tgt Ion:252 Resp: 5367

Ion Ratio Lower Upper

252 100

253 52.2 21.9 32.9#

125 44.0 15.5 23.3#

