




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027889.D
Acq On : 27 Sep 2023 08:20
Operator : MA/JU
Sample : 04472-20
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZYM7

Manual IntegrationsAPPROVED

Quant Time: Sep 27 08:48:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :mohammad ahmed 09/28/2023

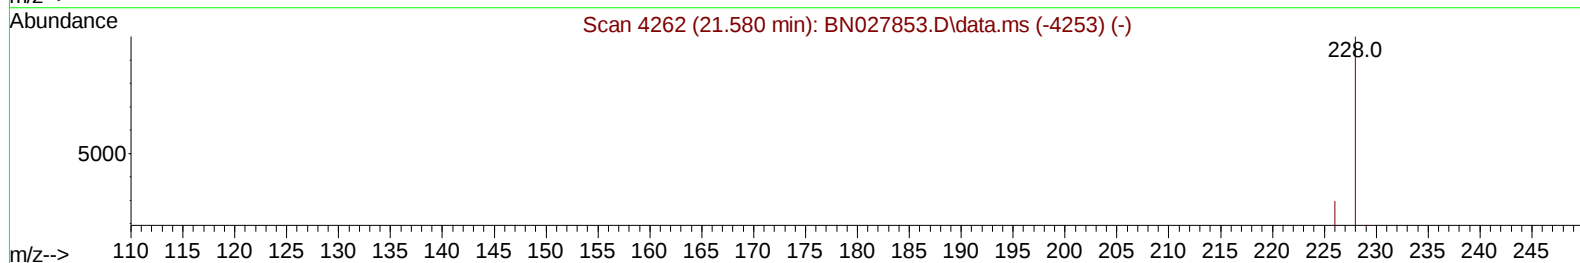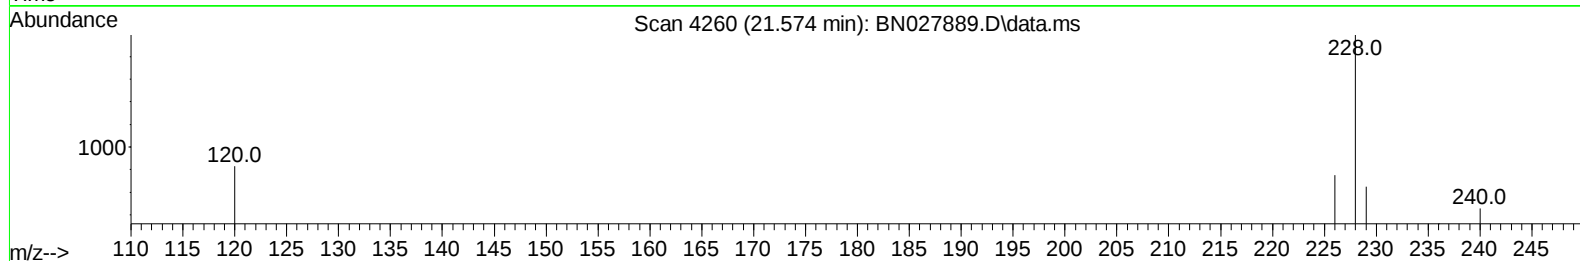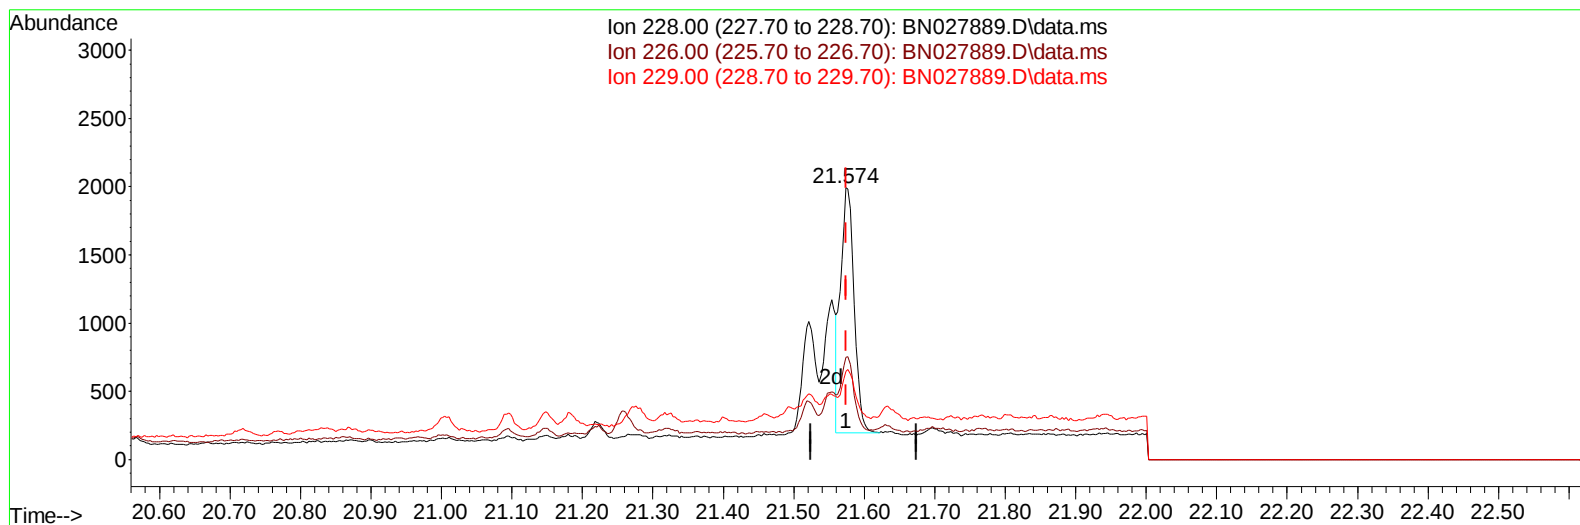

TIC: BN027889.D\data.ms

(22) Chrysene

21.574min (+ 0.000) 0.02 ng/u1

response 2402

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.60	37.62#
229.00	20.00	32.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027889.D
 Acq On : 27 Sep 2023 08:20
 Operator : MA/JU
 Sample : 04472-20
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYM7

Manual IntegrationsAPPROVED

Quant Time: Sep 27 08:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/28/2023

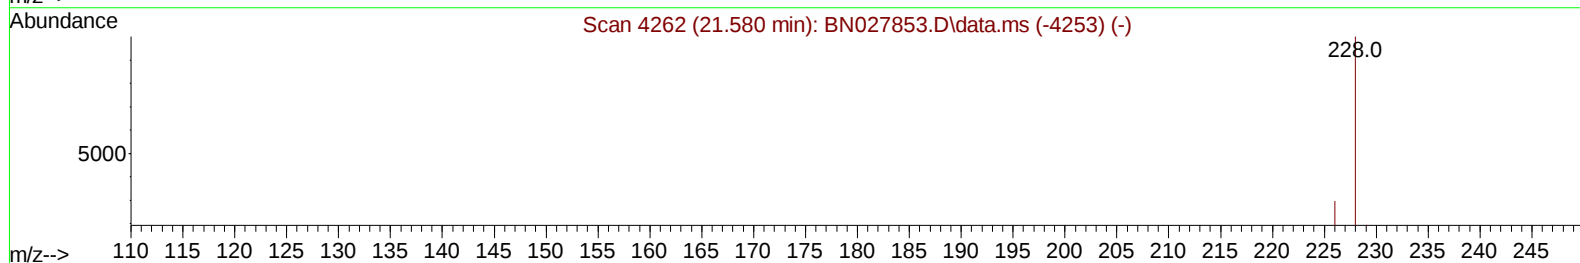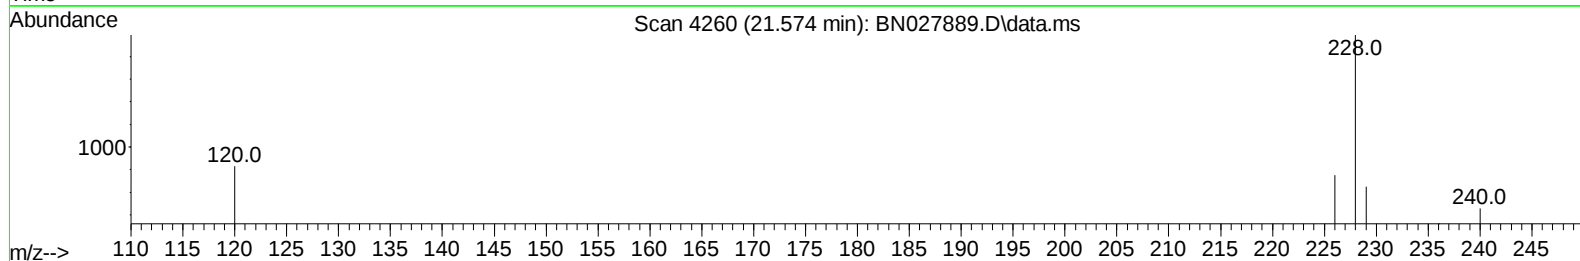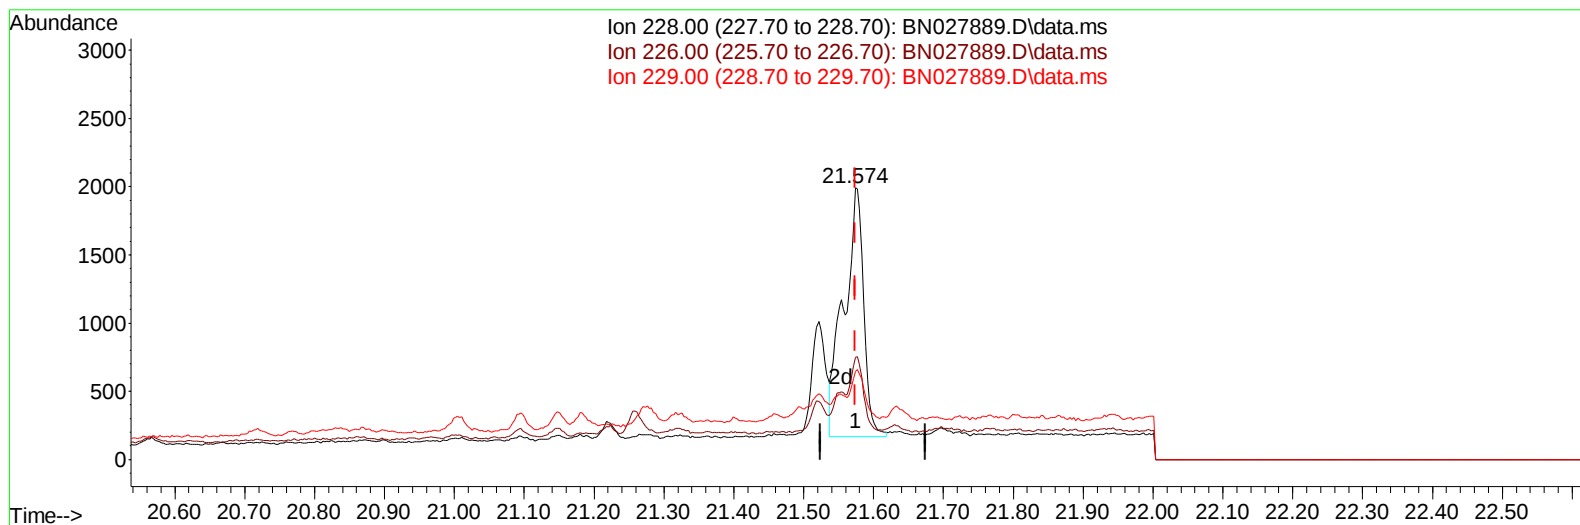

TIC: BN027889.D\data.ms

(22) Chrysene

21.574min (+ 0.000) 0.03 ng/u1 m

response 3605

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.60	37.62#
229.00	20.00	32.55#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027889.D
 Acq On : 27 Sep 2023 08:20
 Operator : MA/JU
 Sample : 04472-20
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYM7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/28/2023

Quant Time: Sep 27 08:48:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	6345	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	23797	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	15362	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	35375	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	34785	0.400	ng/ul	0.00
23) Perylene-d12	24.009	264	40183	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	15801	1.977	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	4475	0.124	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	12522	0.118	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.397	178	8855	0.080	ng/ul	98
19) Fluoranthene	19.408	202	3581	0.025	ng/ul#	88
20) Pyrene	19.776	202	4629	0.032	ng/ul#	85
22) Chrysene	21.574	228	3605m	0.026	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027889.D
Acq On : 27 Sep 2023 08:20
Operator : MA/JU
Sample : 04472-20
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZYM7

Manual IntegrationsAPPROVED

Quant Time: Sep 27 08:48:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :mohammad ahmed 09/28/2023

