




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027892.D
 Acq On : 27 Sep 2023 10:07
 Operator : MA/JU
 Sample : 04410-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHM2

Manual IntegrationsAPPROVED

Quant Time: Sep 27 23:59:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/28/2023
 Supervised By :mohammad ahmed 09/28/2023

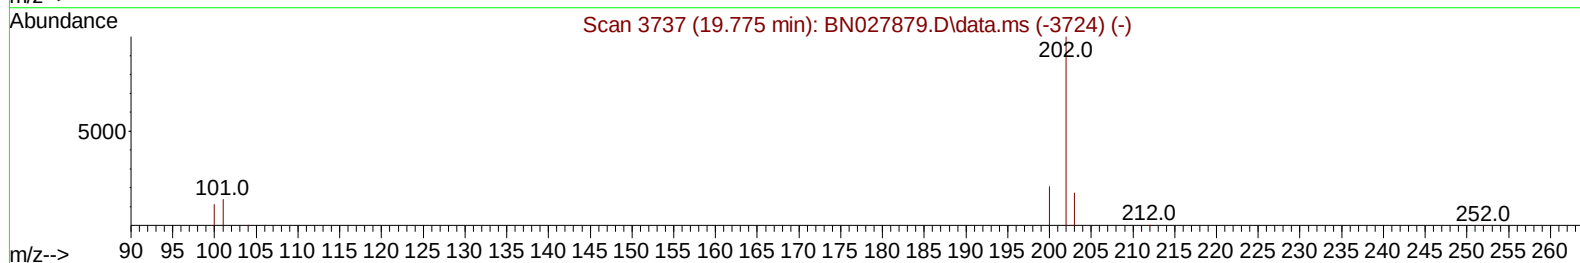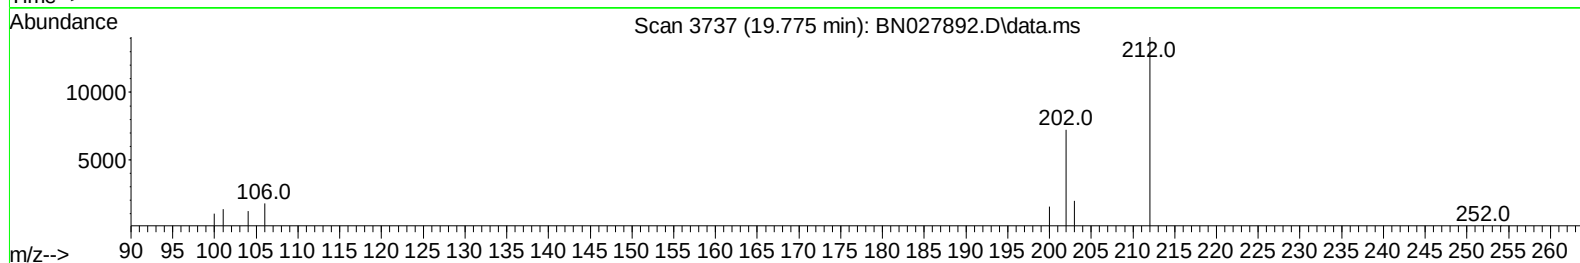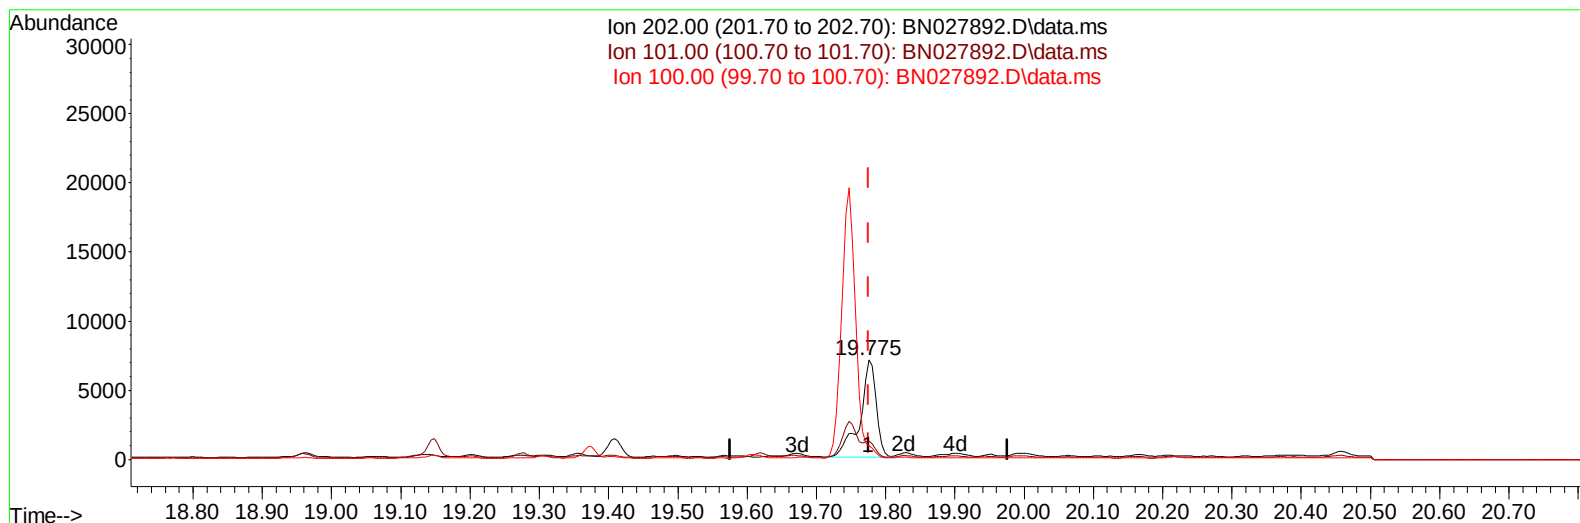

TIC: BN027892.D\data.ms

(20) Pyrene

19.775min (-0.000) 0.18 ng/ul

response 11344

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	18.18#
100.00	11.40	13.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027892.D
 Acq On : 27 Sep 2023 10:07
 Operator : MA/JU
 Sample : 04410-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHM2

Manual IntegrationsAPPROVED

Quant Time: Sep 27 23:59:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/28/2023
 Supervised By :mohammad ahmed 09/28/2023

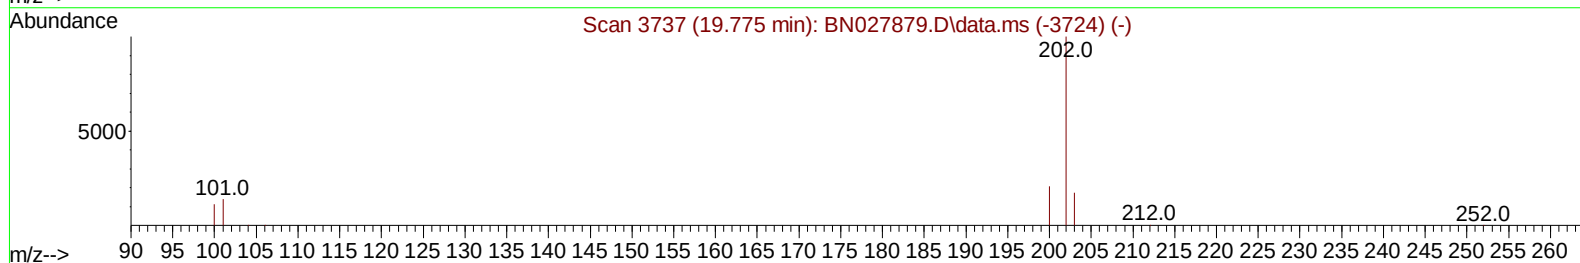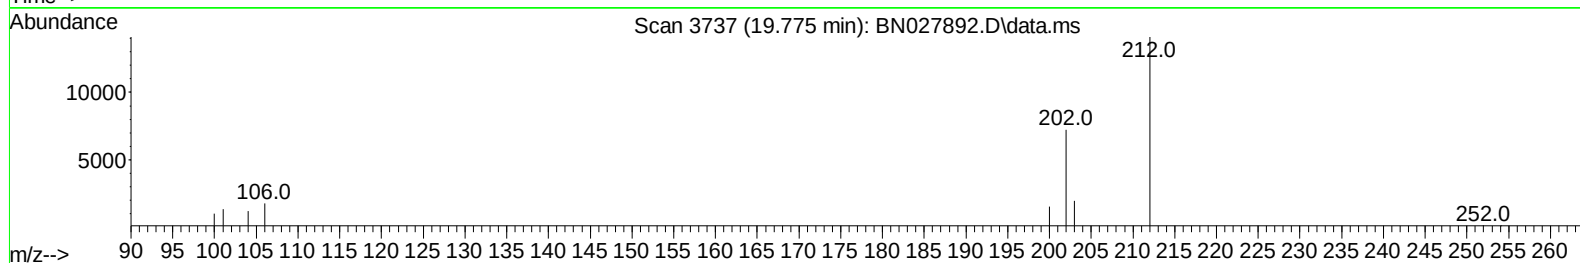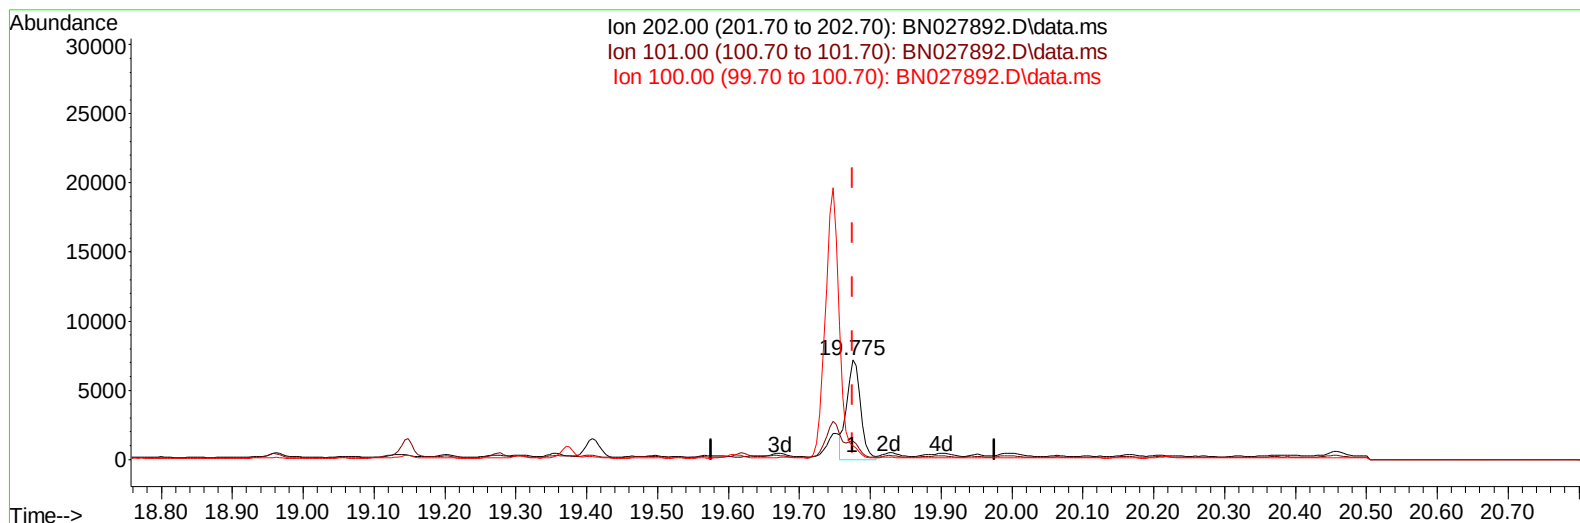

TIC: BN027892.D\data.ms

(20) Pyrene

19.775min (-0.000) 0.15 ng/ul m

response 9708

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	18.18#
100.00	11.40	13.86#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027892.D
 Acq On : 27 Sep 2023 10:07
 Operator : MA/JU
 Sample : 04410-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHM2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/28/2023
 Supervised By :mohammad ahmed 09/28/2023

Quant Time: Sep 27 23:59:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.958	152		2693	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136		10179	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164		7181	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188		15986	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240		15542	0.400	ng/ul	0.00
23) Perylene-d12	24.009	264		18748	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.330	96		14341	4.228	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152		5510	0.357	ng/ul	0.00
18) Fluoranthene-d10	19.380	212		18772	0.395	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.368	88		632	0.179	ng/ul#	87
19) Fluoranthene	19.408	202		1905	0.030	ng/ul#	82
20) Pyrene	19.775	202		9708m	0.150	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027892.D
Acq On : 27 Sep 2023 10:07
Operator : MA/JU
Sample : 04410-17
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHM2

Manual IntegrationsAPPROVED

Quant Time: Sep 27 23:59:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :mohammad ahmed 09/28/2023

