




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027893.D
Acq On : 27 Sep 2023 10:43
Operator : MA/JU
Sample : 04410-18
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJG7

Manual IntegrationsAPPROVED

Quant Time: Sep 28 00:00:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :mohammad ahmed 09/28/2023

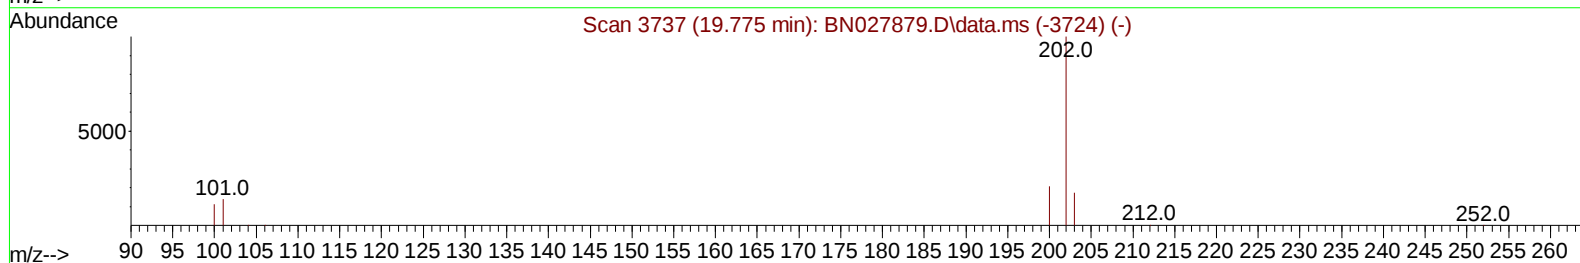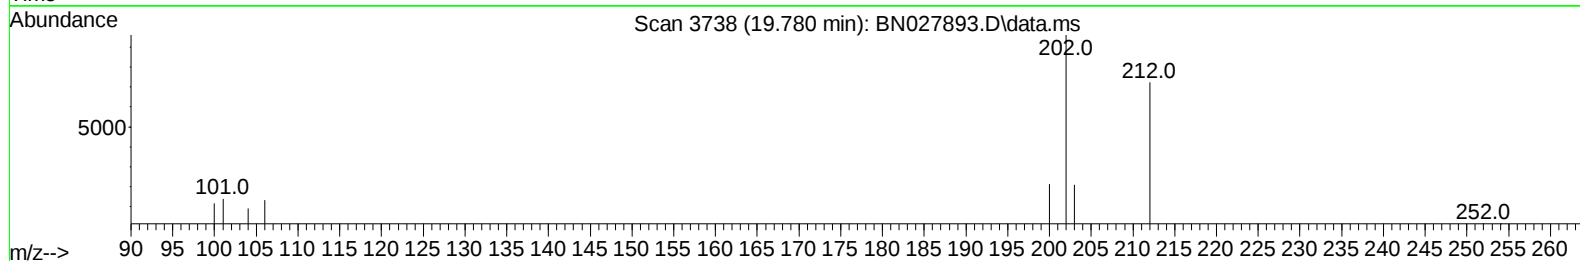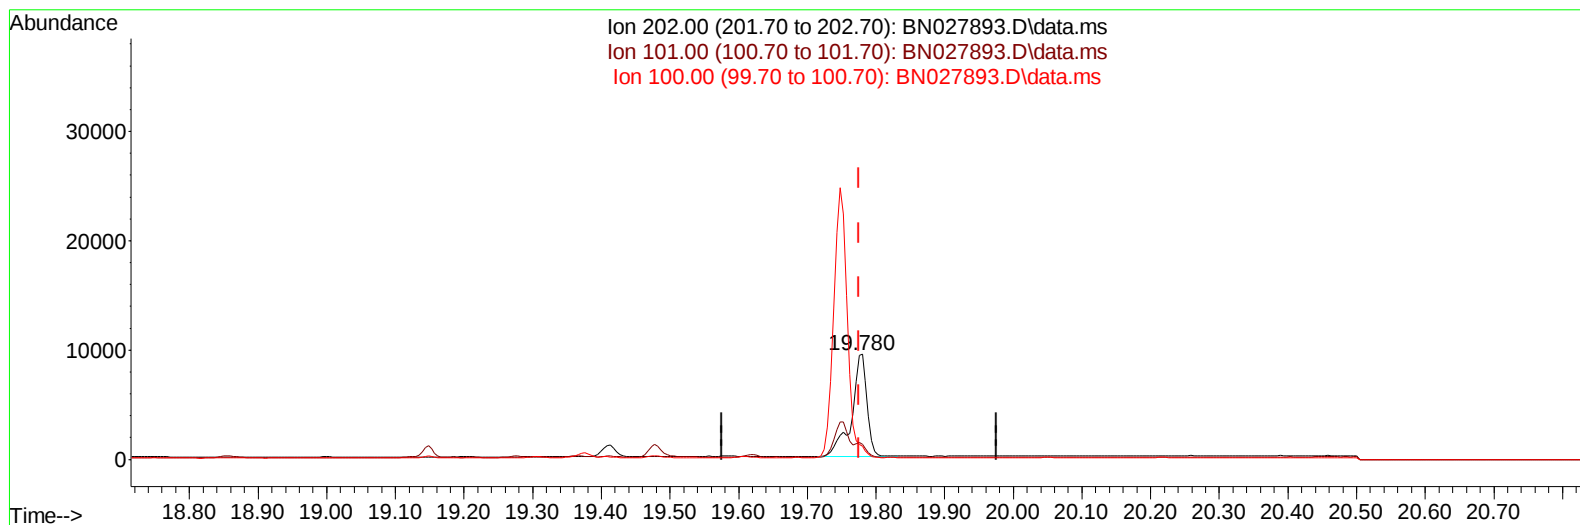

TIC: BN027893.D\data.ms

(20) Pyrene

19.780min (+ 0.004) 0.18 ng/u1

response 14870

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	14.62
100.00	11.40	12.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027893.D
Acq On : 27 Sep 2023 10:43
Operator : MA/JU
Sample : 04410-18
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJG7

Manual IntegrationsAPPROVED

Quant Time: Sep 28 00:00:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :mohammad ahmed 09/28/2023

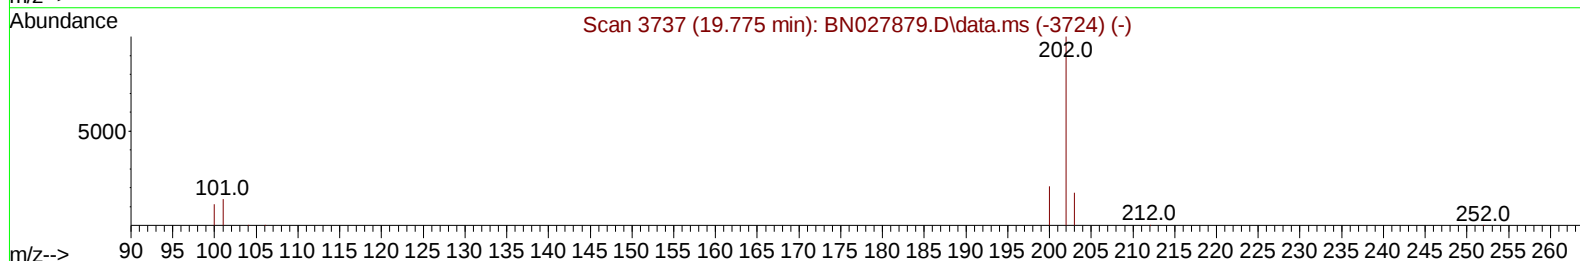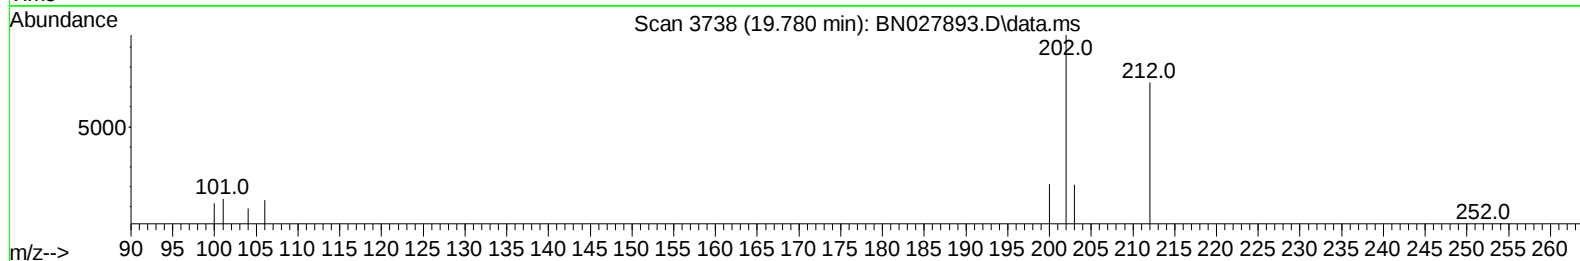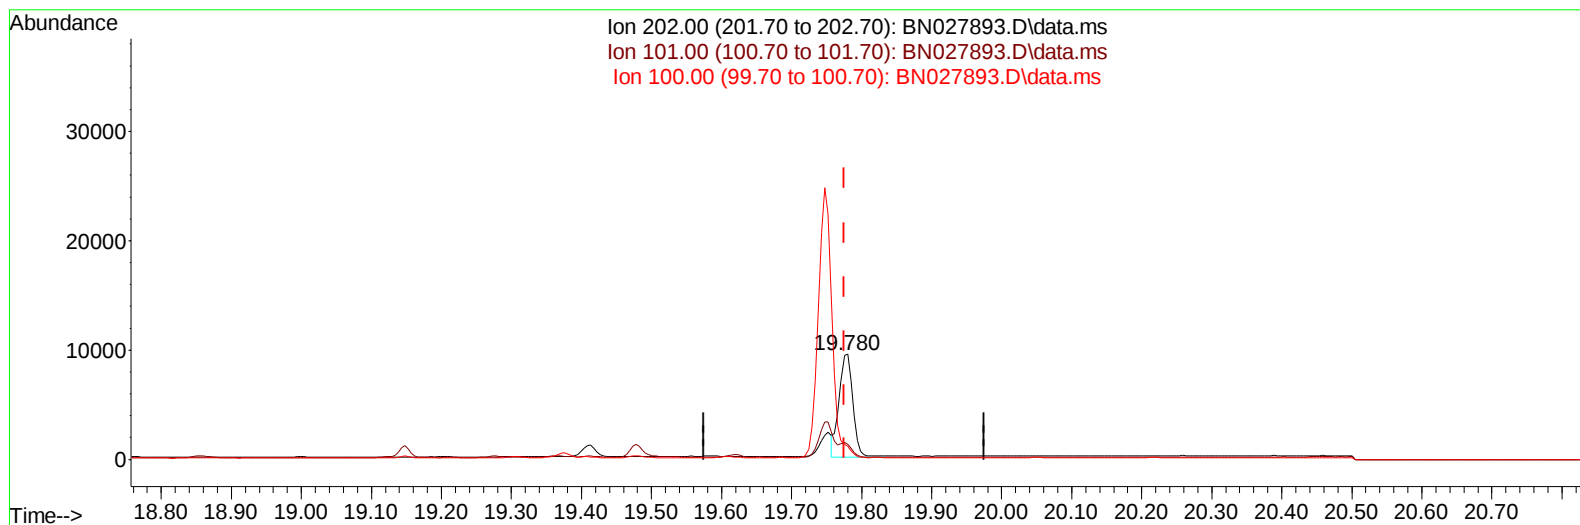

TIC: BN027893.D\data.ms

(20) Pyrene

19.780min (+ 0.004) 0.16 ng/ul m

response 12773

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	14.62
100.00	11.40	12.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027893.D
 Acq On : 27 Sep 2023 10:43
 Operator : MA/JU
 Sample : 04410-18
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJG7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/28/2023
 Supervised By :mohammad ahmed 09/28/2023

Quant Time: Sep 28 00:00:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.962	152		3446	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136		12891	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164		8631	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188		19841	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240		19681	0.400	ng/ul	0.00
23) Perylene-d12	24.012	264		23752	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.330	96		16608	3.826	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.362	152		7913	0.405	ng/ul	0.00
18) Fluoranthene-d10	19.380	212		24534	0.408	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.367	88		2789	0.617	ng/ul	90
16) Anthracene	17.489	178		1974	0.038	ng/ul#	76
20) Pyrene	19.780	202		12773m	0.156	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027893.D
Acq On : 27 Sep 2023 10:43
Operator : MA/JU
Sample : 04410-18
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJG7

Manual IntegrationsAPPROVED

Quant Time: Sep 28 00:00:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :mohammad ahmed 09/28/2023

