

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027865.D
 Acq On : 26 Sep 2023 17:19
 Operator : MA/JU
 Sample : 04410-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBBK3

Quant Time: Sep 27 03:01:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	3330	0.400	ng/u1	0.00
4) Naphthalene-d8	10.784	136	12388	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.606	164	8216	0.400	ng/u1	0.01
13) Phenanthrene-d10	17.358	188	19276	0.400	ng/u1	0.02
17) Chrysene-d12	21.542	240	18831	0.400	ng/u1	0.02
23) Perylene-d12	24.021	264	22997	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	16845	4.016	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.368	152	6423	0.342	ng/u1	0.01
18) Fluoranthene-d10	19.385	212	21246	0.369	ng/u1	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	3922	0.898	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027865.D
Acq On : 26 Sep 2023 17:19
Operator : MA/JU
Sample : 04410-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBBK3

Quant Time: Sep 27 03:01:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration

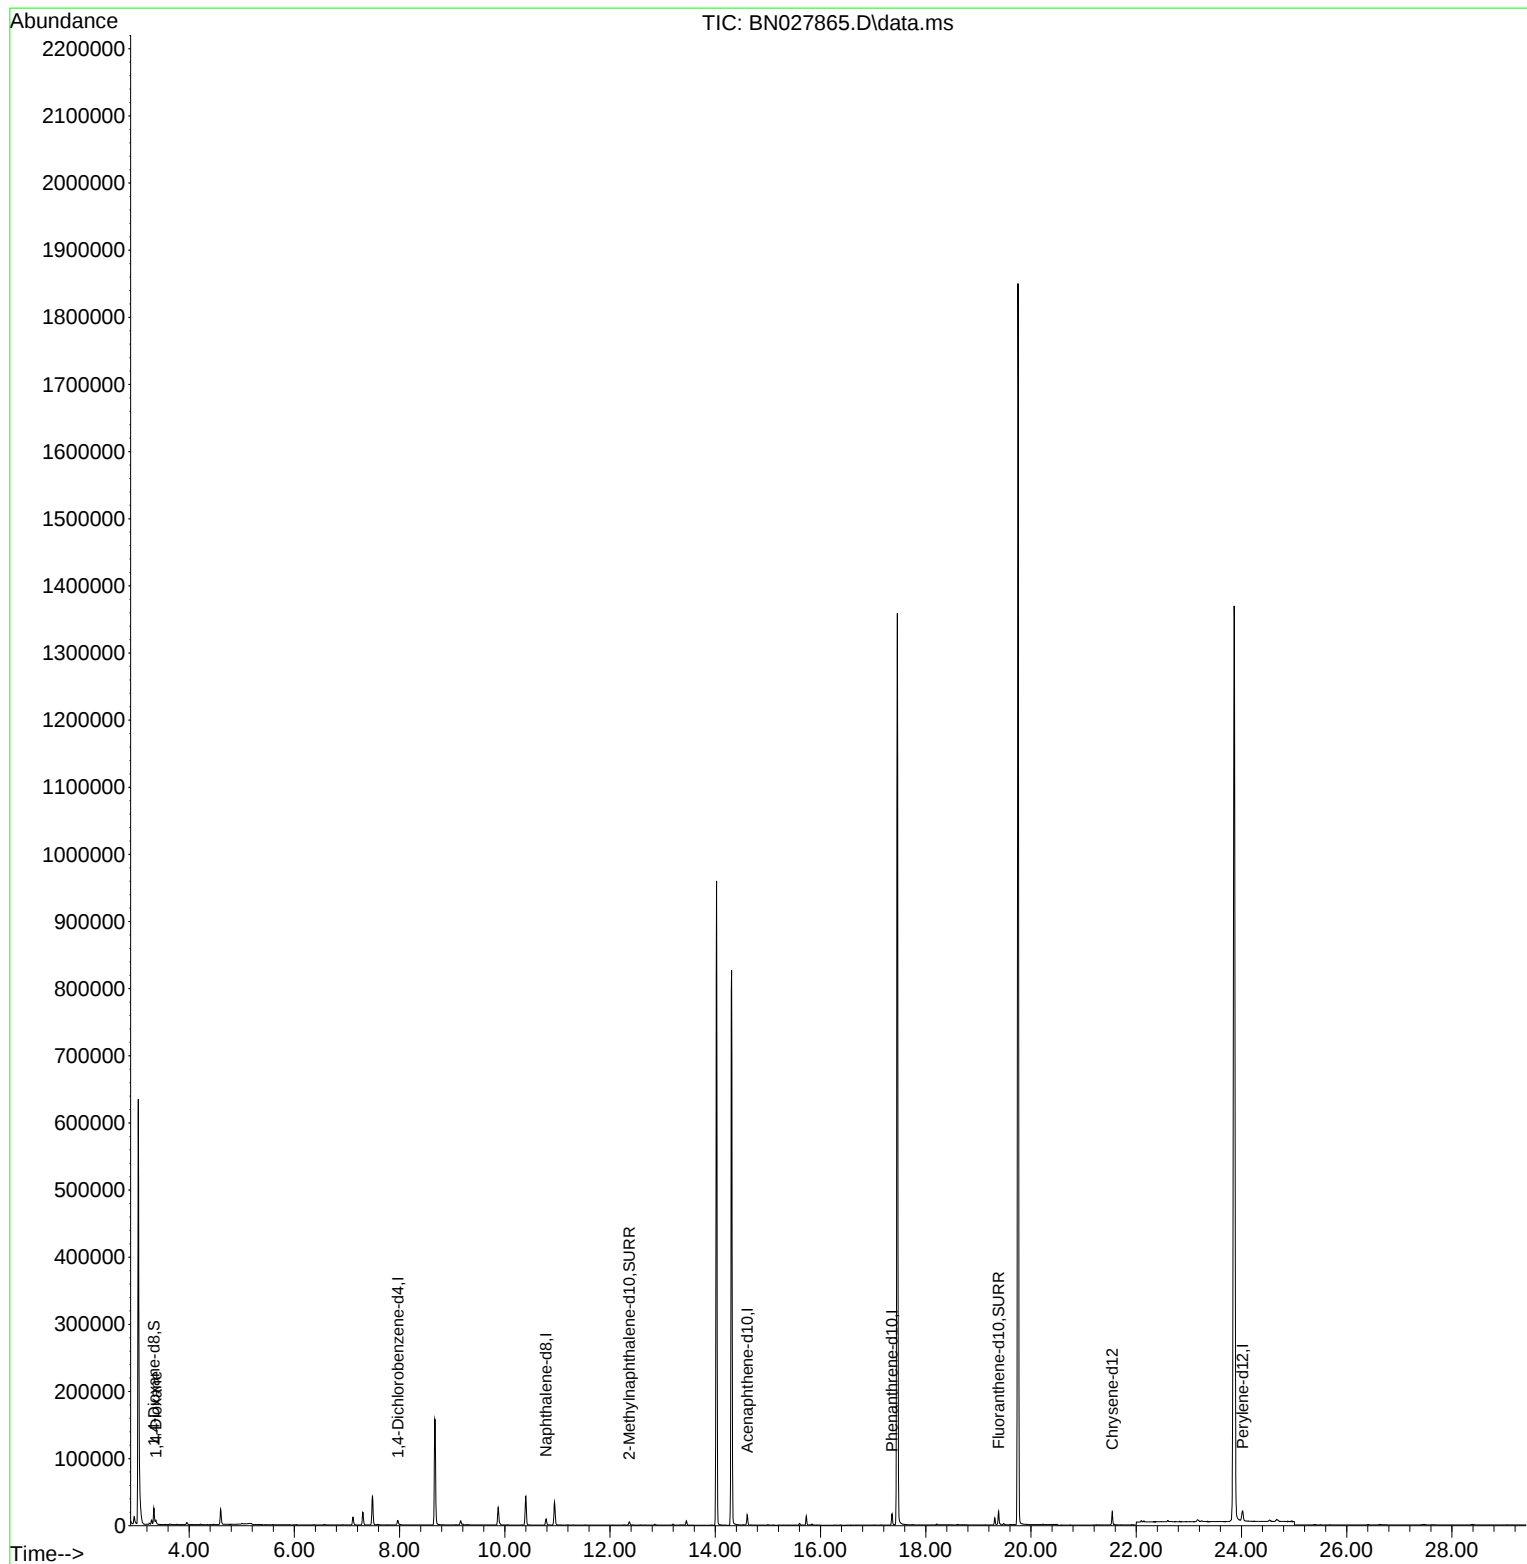

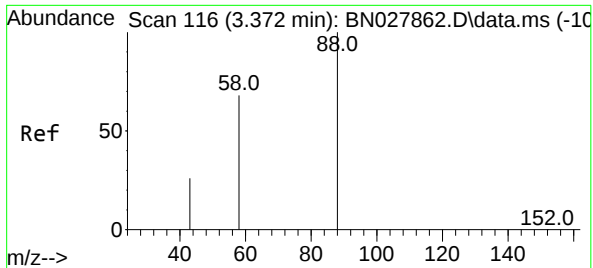

#2
 1,4-Dioxane
 Concen: 0.898 ng/ul
 RT: 3.368 min Scan# 11
 Delta R.T. -0.005 min
 Lab File: BN027865.D
 Acq: 26 Sep 2023 17:19

Instrument :
 BNA_N
 ClientSampleId :
 BBBK3

Tgt Ion:	88	Resp:	3922
Ion	Ratio	Lower	Upper
88	100		
43	39.9	39.6	59.4
58	63.5	48.3	72.5

