

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027867.D
 Acq On : 26 Sep 2023 18:32
 Operator : MA/JU
 Sample : 04410-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBBK1

Quant Time: Sep 27 03:01:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	2701	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	10032	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	6910	0.400	ng/ul	0.01
13) Phenanthrene-d10	17.358	188	16123	0.400	ng/ul	0.02
17) Chrysene-d12	21.545	240	15867	0.400	ng/ul	0.02
23) Perylene-d12	24.021	264	19860	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	15459	4.544	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	6160	0.405	ng/ul	0.01
18) Fluoranthene-d10	19.385	212	20895	0.431	ng/ul	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	1193	0.337	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027867.D
Acq On : 26 Sep 2023 18:32
Operator : MA/JU
Sample : 04410-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBBK1


Quant Time: Sep 27 03:01:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration

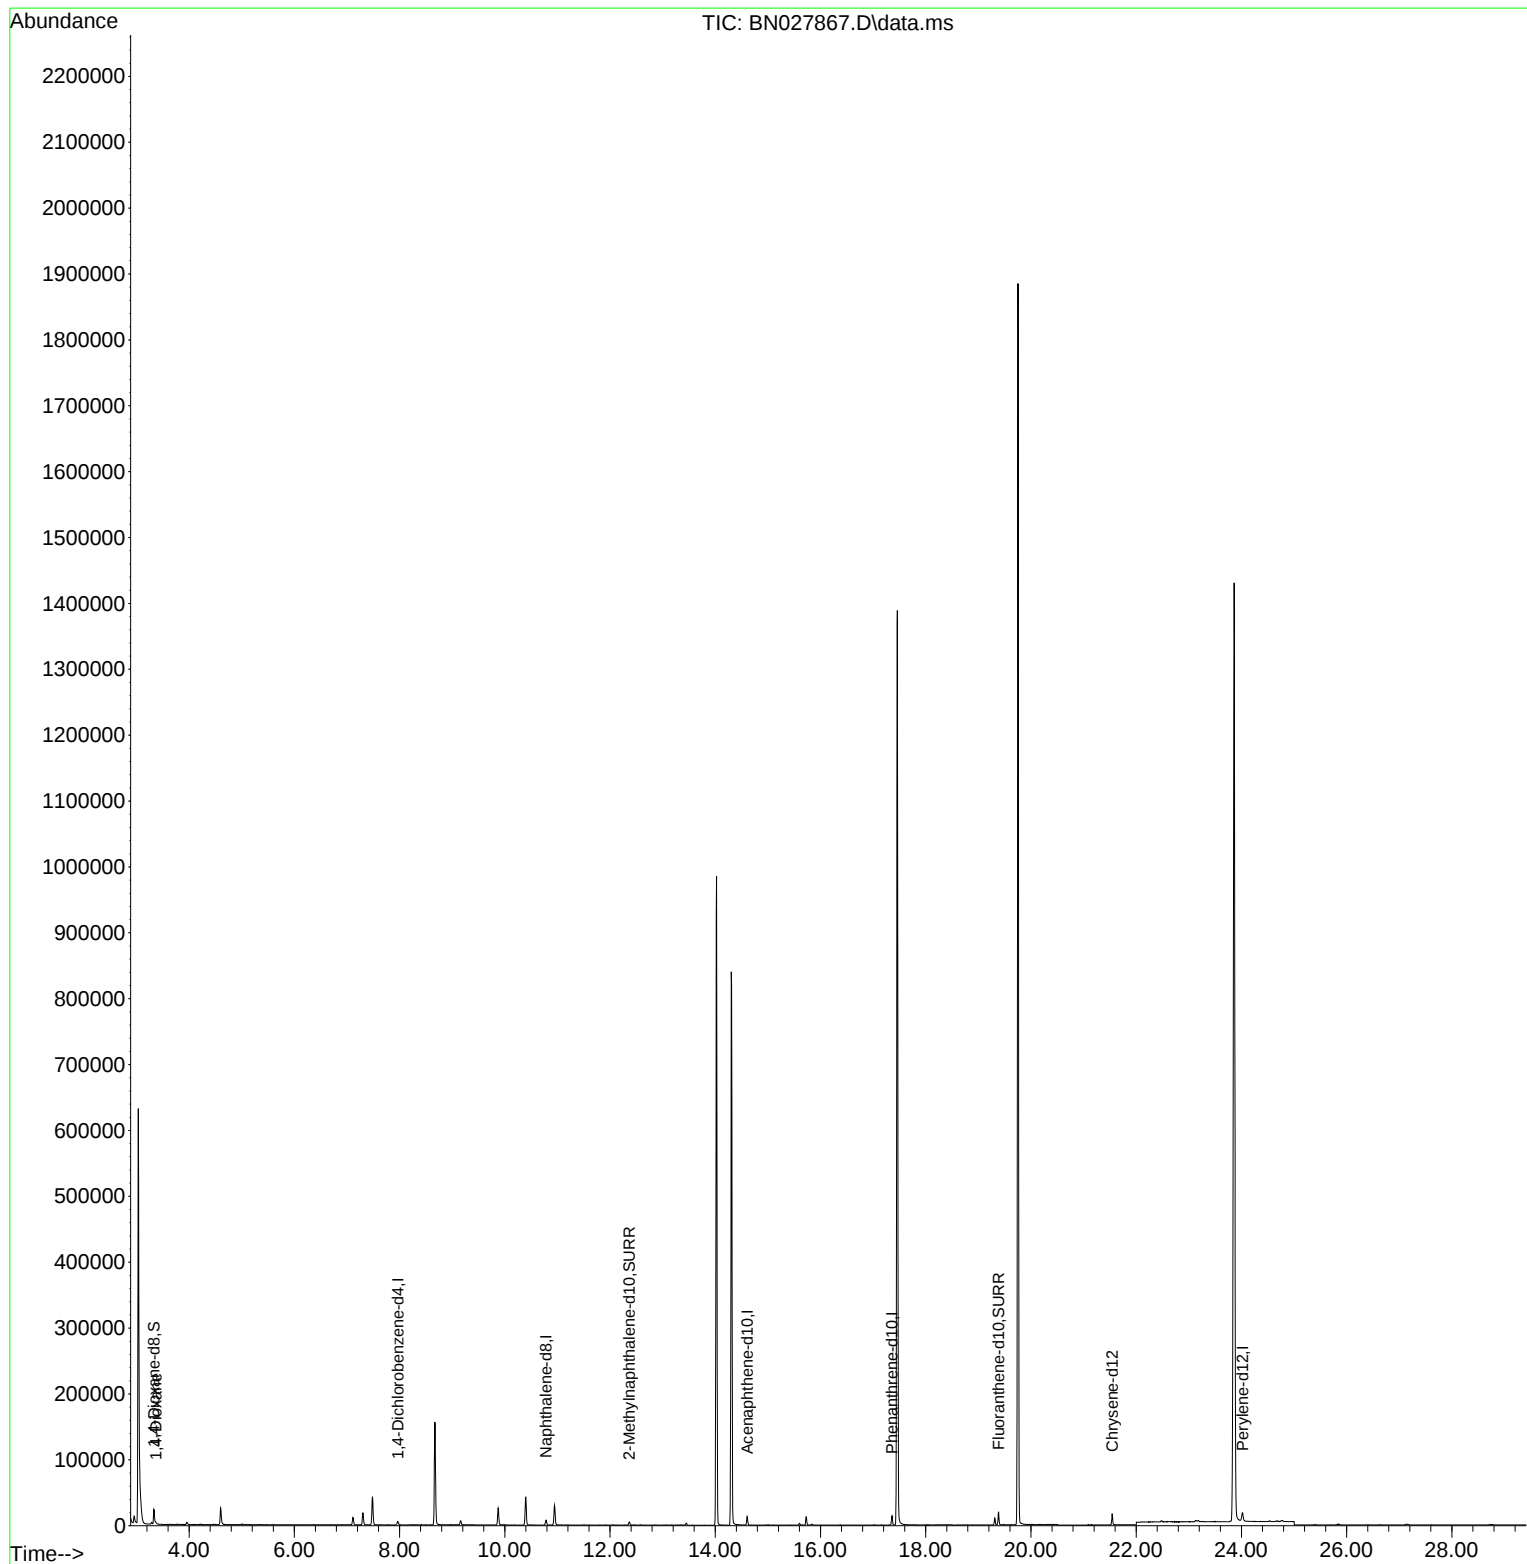

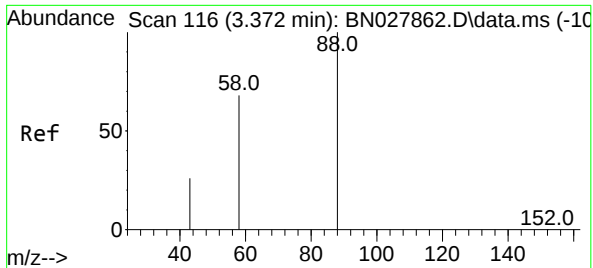

#2
1,4-Dioxane
Concen: 0.337 ng/ul
RT: 3.368 min Scan# 11
Delta R.T. -0.005 min
Lab File: BN027867.D
Acq: 26 Sep 2023 18:32

Instrument :
BNA_N
ClientSampleId :
BBBK1

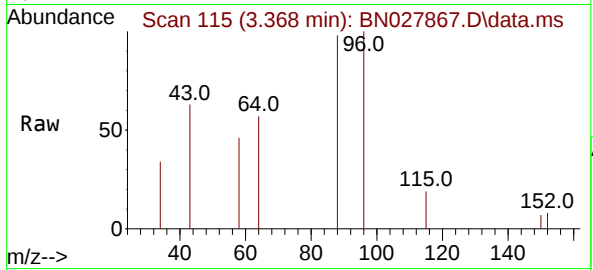

Tgt Ion: 88 Resp: 1193
Ion Ratio Lower Upper
88 100
43 63.8 39.6 59.4#
58 46.6 48.3 72.5#

