

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027869.D
 Acq On : 26 Sep 2023 19:44
 Operator : MA/JU
 Sample : 04410-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHE1

Quant Time: Sep 27 03:01:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	2559	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	9608	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	6620	0.400	ng/ul	0.01
13) Phenanthrene-d10	17.358	188	15449	0.400	ng/ul	0.02
17) Chrysene-d12	21.545	240	15246	0.400	ng/ul	0.02
23) Perylene-d12	24.018	264	18795	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	11718	3.635	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	5268	0.362	ng/ul	0.01
18) Fluoranthene-d10	19.385	212	18787	0.403	ng/ul	0.02
Target Compounds				Qvalue		
2) 1,4-Dioxane	3.368	88	806	0.240	ng/ul#	76
10) Acenaphthylene	14.337	152	1189	0.041	ng/ul#	75
16) Anthracene	17.493	178	2986	0.073	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027869.D
Acq On : 26 Sep 2023 19:44
Operator : MA/JU
Sample : 04410-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHE1

Quant Time: Sep 27 03:01:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration




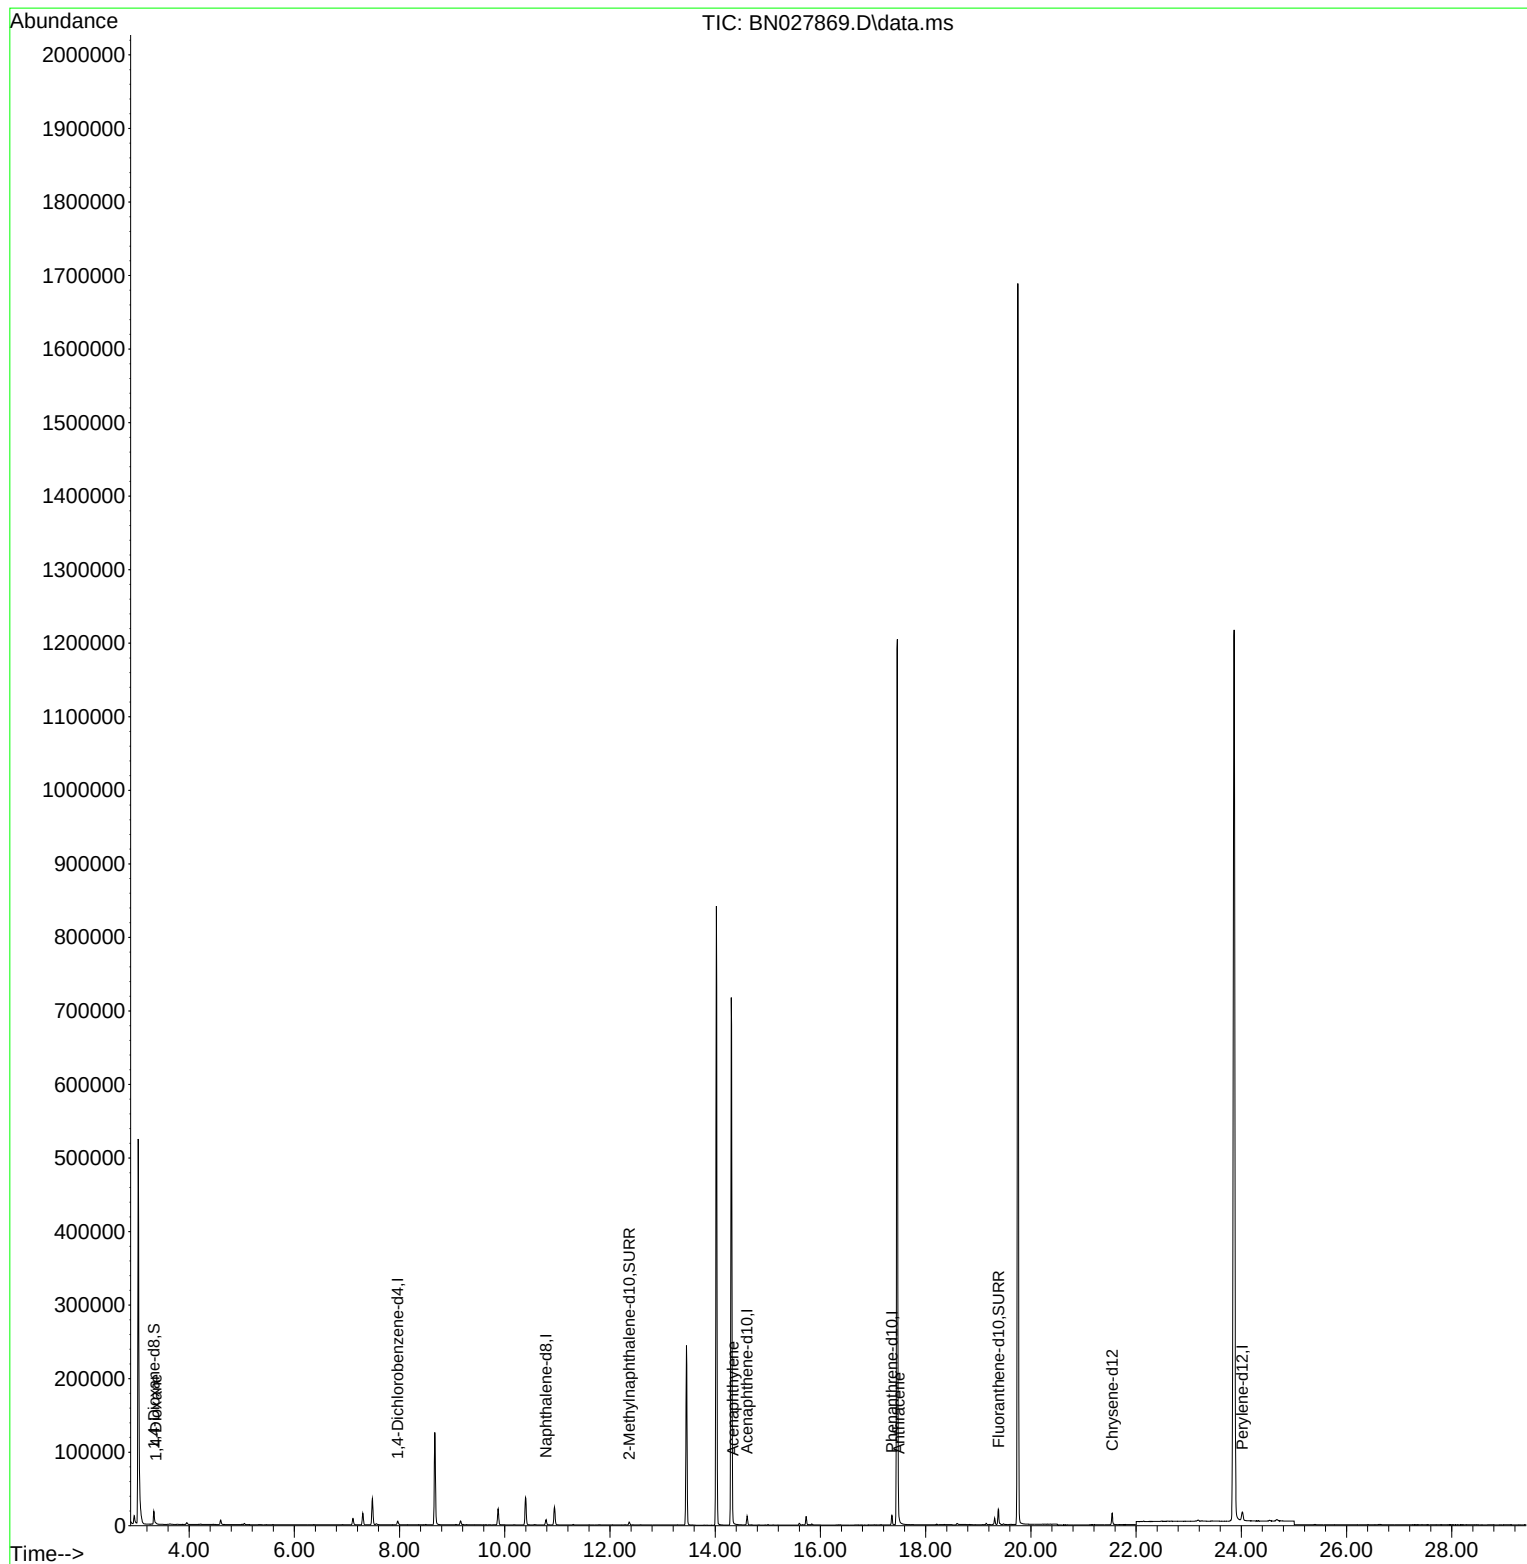


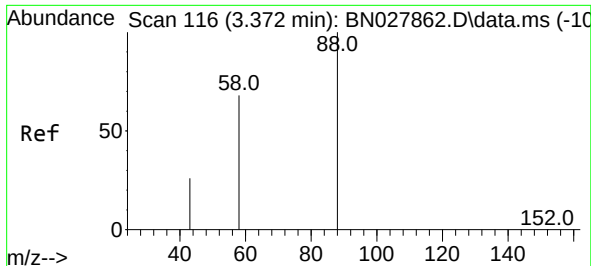

#2
1,4-Dioxane
Concen: 0.240 ng/ul
RT: 3.368 min Scan# 116
Delta R.T. -0.005 min
Lab File: BN027869.D
Acq: 26 Sep 2023 19:44




Instrument :
BNA_N
ClientSampleId :
BBHE1


Tgt Ion: 88 Resp: 806
Ion Ratio Lower Upper
88 100
43 77.4 39.6 59.4#
58 52.5 48.3 72.5

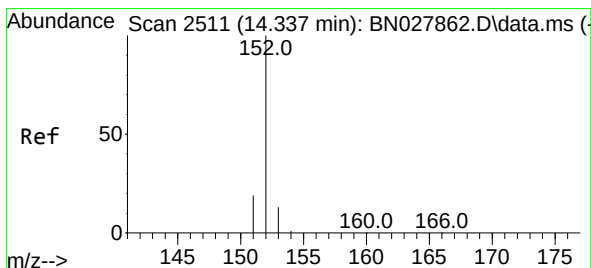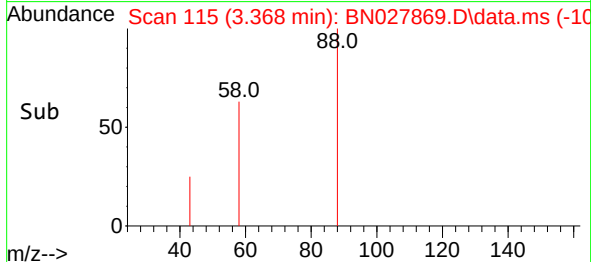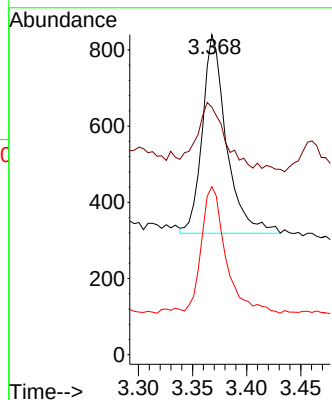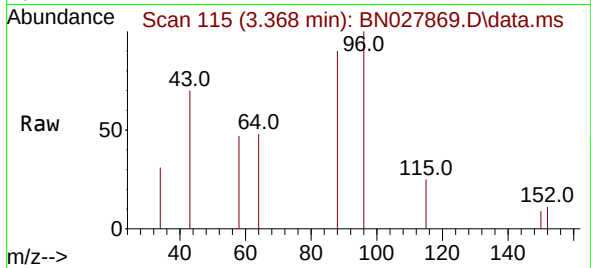

#10
Acenaphthylene
Concen: 0.041 ng/ul
RT: 14.337 min Scan# 2511
Delta R.T. 0.018 min
Lab File: BN027869.D
Acq: 26 Sep 2023 19:44


Tgt Ion: 152 Resp: 1189
Ion Ratio Lower Upper
152 100
151 32.1 16.6 25.0#
153 24.4 11.0 16.6#

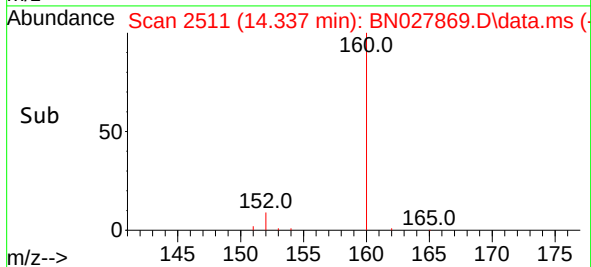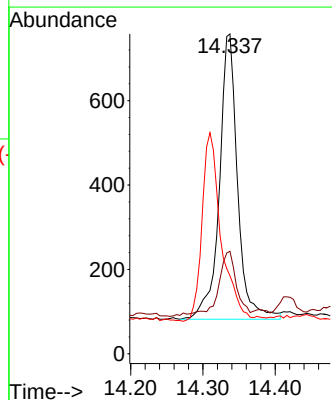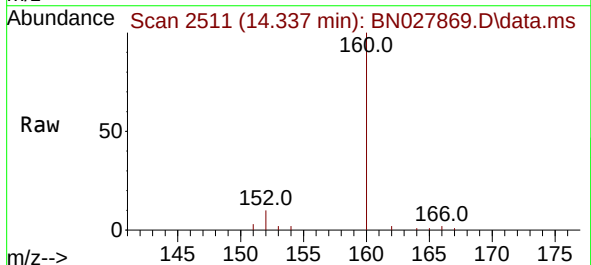

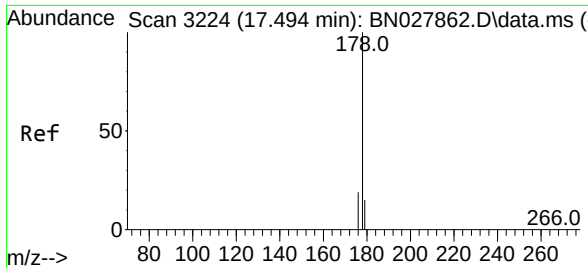

#16
 Anthracene
 Concen: 0.073 ng/ul
 RT: 17.493 min Scan# 31
 Delta R.T. 0.016 min
 Lab File: BN027869.D
 Acq: 26 Sep 2023 19:44

Instrument :
 BNA_N
 ClientSampleId :
 BBHE1

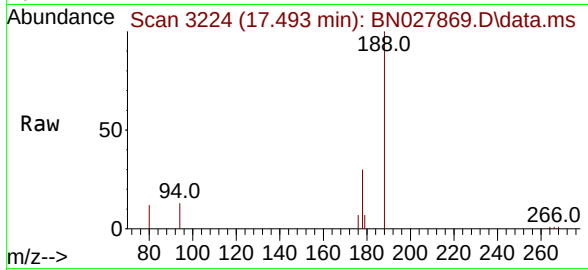

Tgt Ion:	178	Resp:	2986
Ion	Ratio	Lower	Upper
178	100		
179	22.6	12.6	19.0#
176	22.9	15.5	23.3

