

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027878.D
 Acq On : 27 Sep 2023 01:09
 Operator : MA/JU
 Sample : 04410-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKJ0

Quant Time: Sep 27 03:02:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:58:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.962	152	3758	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	13670	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	9209	0.400	ng/ul	0.01
13) Phenanthrene-d10	17.354	188	21296	0.400	ng/ul	0.01
17) Chrysene-d12	21.539	240	20793	0.400	ng/ul	0.02
23) Perylene-d12	24.012	264	25799	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	20728	4.379	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	7928	0.383	ng/ul	0.00
18) Fluoranthene-d10	19.380	212	23678	0.373	ng/ul	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	17766	3.606	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027878.D
Acq On : 27 Sep 2023 01:09
Operator : MA/JU
Sample : 04410-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKJ0

Quant Time: Sep 27 03:02:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:58:00 2023
Response via : Initial Calibration

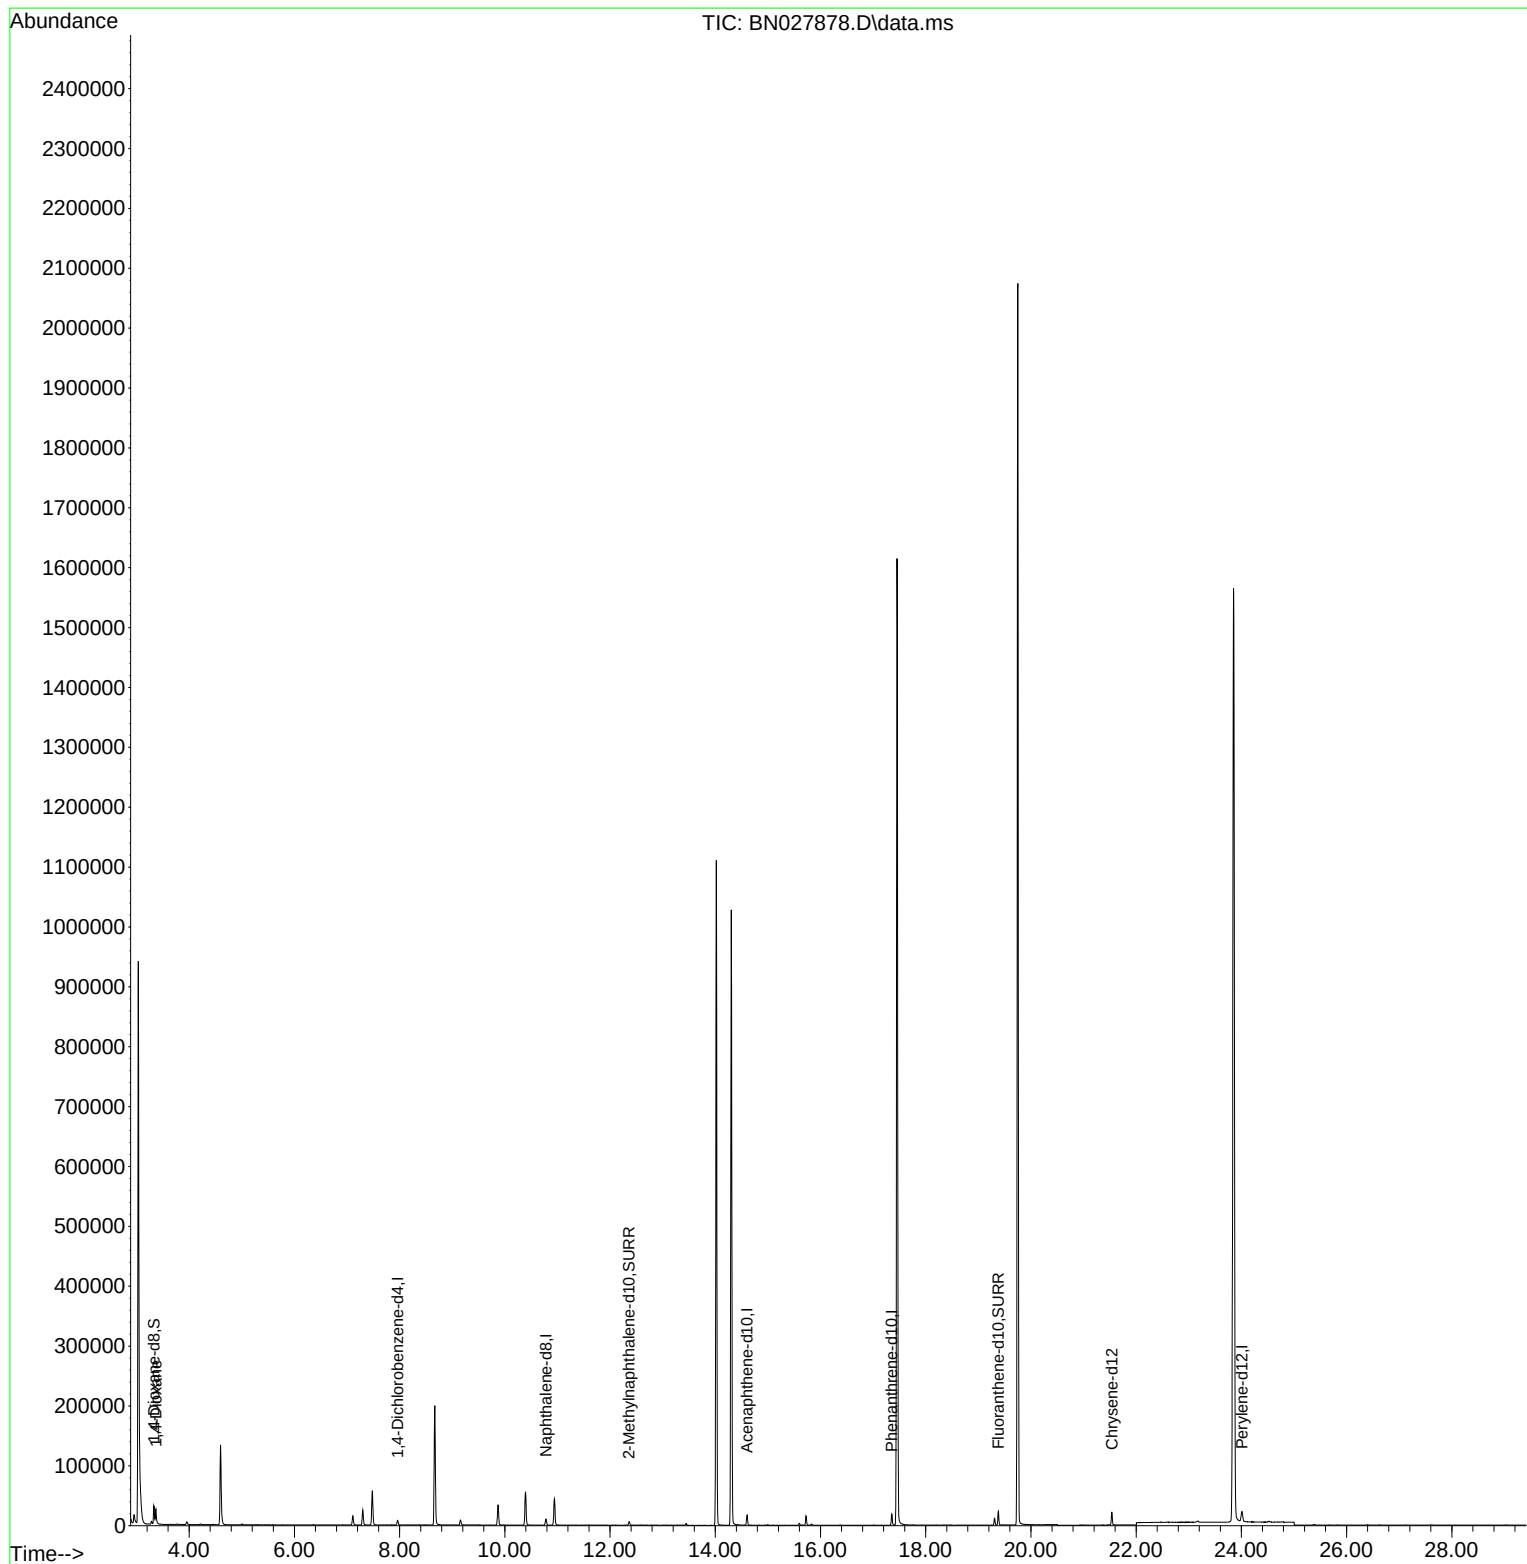

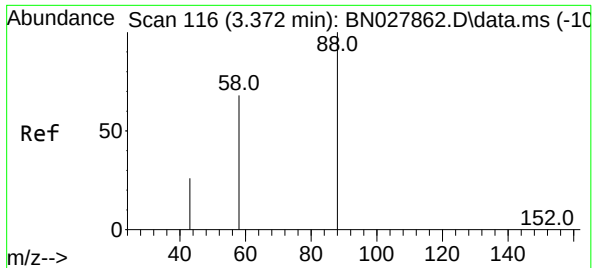

#2
 1,4-Dioxane
 Concen: 3.606 ng/ul
 RT: 3.368 min Scan# 11
 Delta R.T. -0.005 min
 Lab File: BN027878.D
 Acq: 27 Sep 2023 01:09

Instrument :
 BNA_N
 ClientSampleId :
 BBKJ0

Tgt Ion: 88 Resp: 17766
 Ion Ratio Lower Upper
 88 100
 43 28.6 39.6 59.4#
 58 63.2 48.3 72.5

