

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
 Data File : BN027894.D
 Acq On : 27 Sep 2023 11:19
 Operator : MA/JU
 Sample : 04410-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBK36

Quant Time: Sep 28 00:00:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 27 03:52:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	2476	0.400	ng/u1	0.00
4) Naphthalene-d8	10.779	136	9455	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.601	164	6346	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.354	188	14633	0.400	ng/u1	0.00
17) Chrysene-d12	21.539	240	14523	0.400	ng/u1	0.00
23) Perylene-d12	24.009	264	17751	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	12432	3.986	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.363	152	5351	0.374	ng/u1	0.00
18) Fluoranthene-d10	19.381	212	17496	0.394	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	2029	0.625	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092623\
Data File : BN027894.D
Acq On : 27 Sep 2023 11:19
Operator : MA/JU
Sample : 04410-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBK36


Quant Time: Sep 28 00:00:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 27 03:52:19 2023
Response via : Initial Calibration

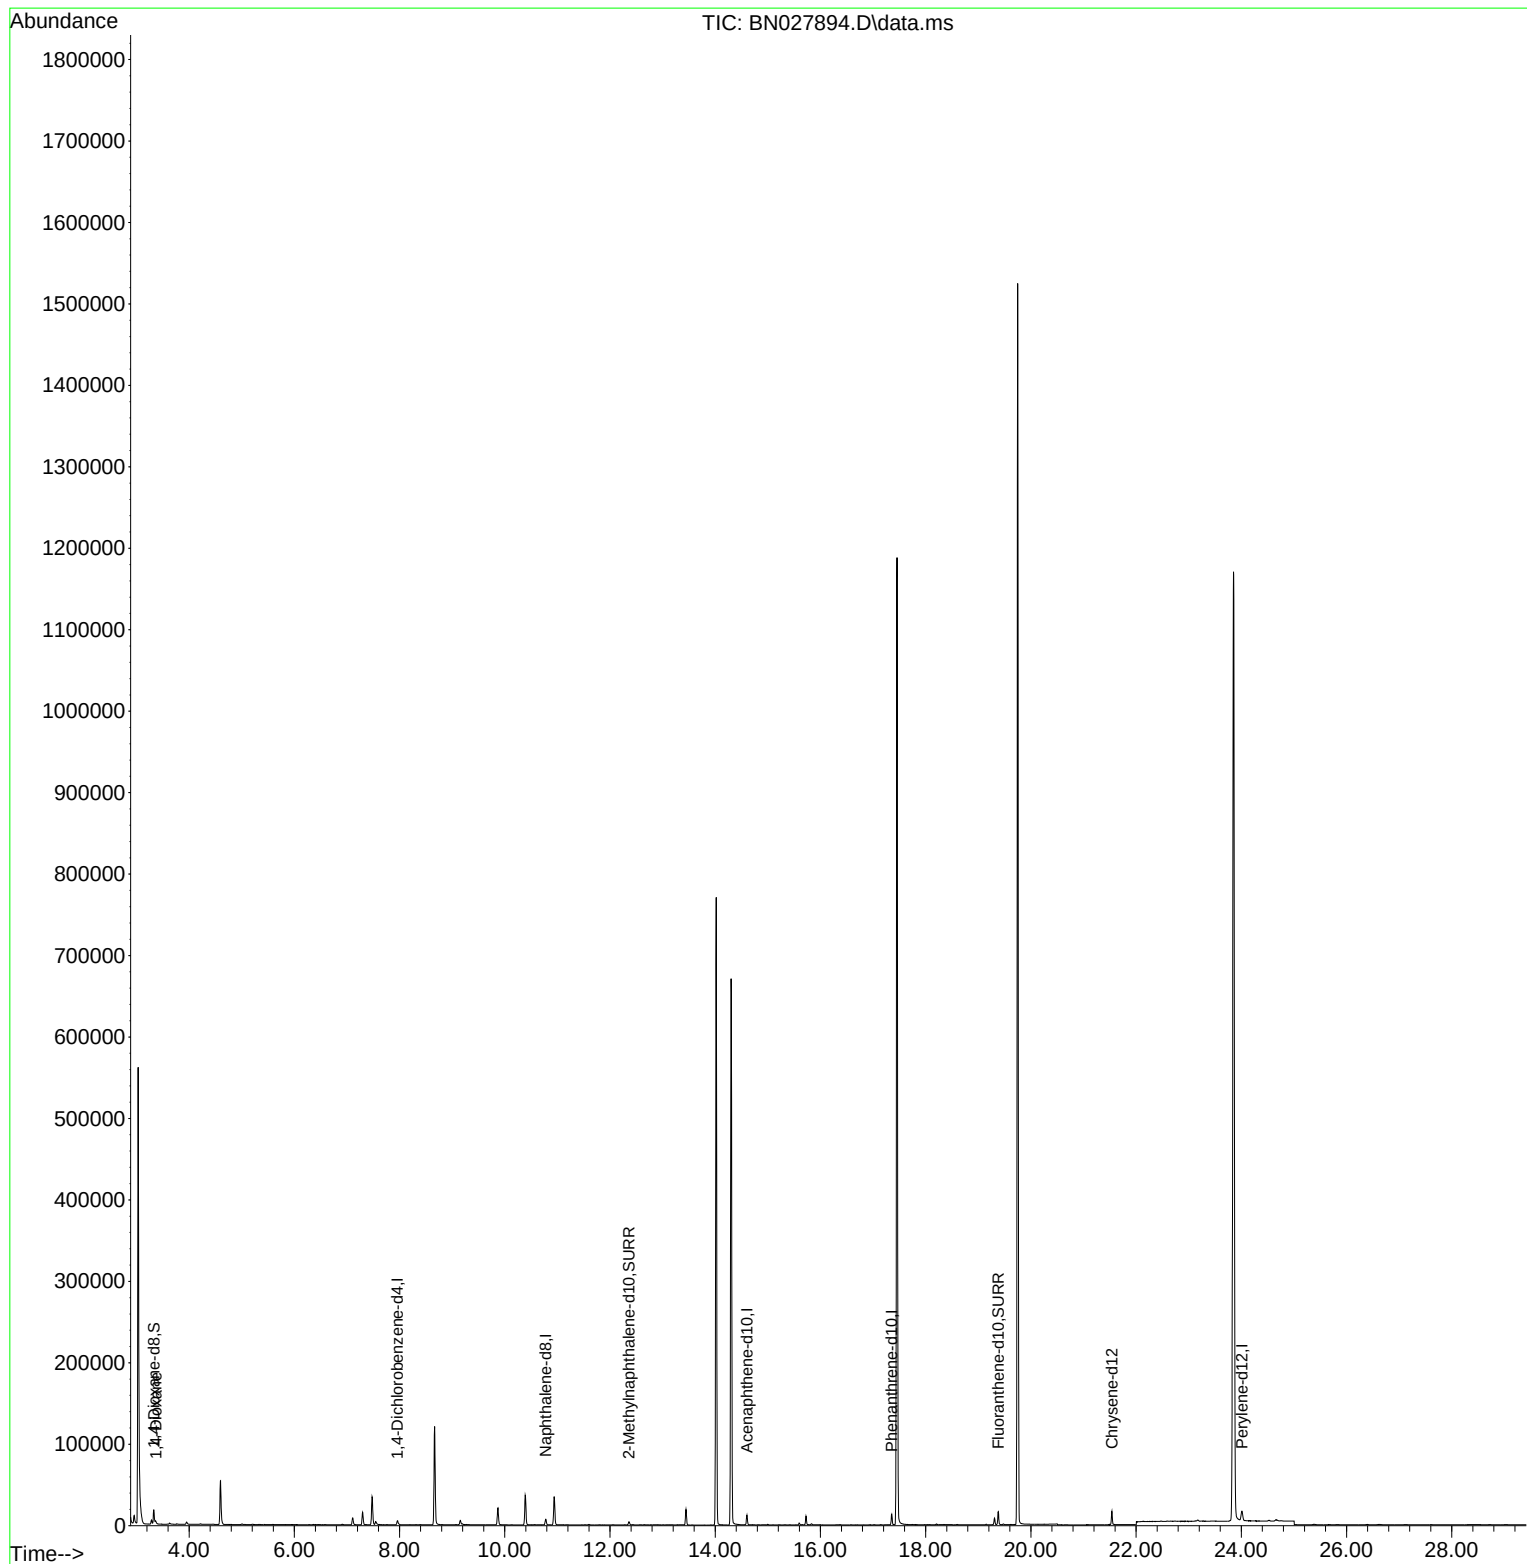

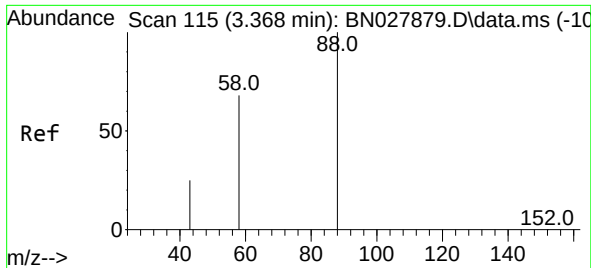

#2
 1,4-Dioxane
 Concen: 0.625 ng/ul
 RT: 3.368 min Scan# 115
 Delta R.T. 0.000 min
 Lab File: BN027894.D
 Acq: 27 Sep 2023 11:19

Instrument :
 BNA_N
 ClientSampleId :
 BBK36

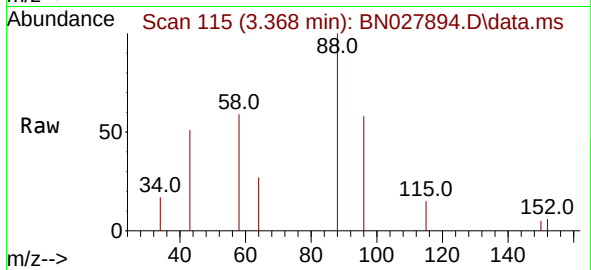

Tgt Ion:	88	Resp:	2029
Ion	Ratio	Lower	Upper
88	100		
43	50.5	39.6	59.4
58	58.8	48.3	72.5

