
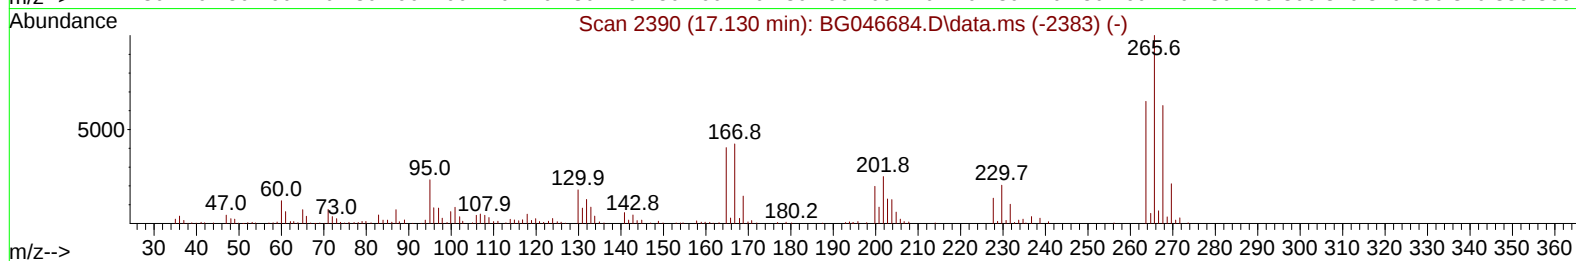
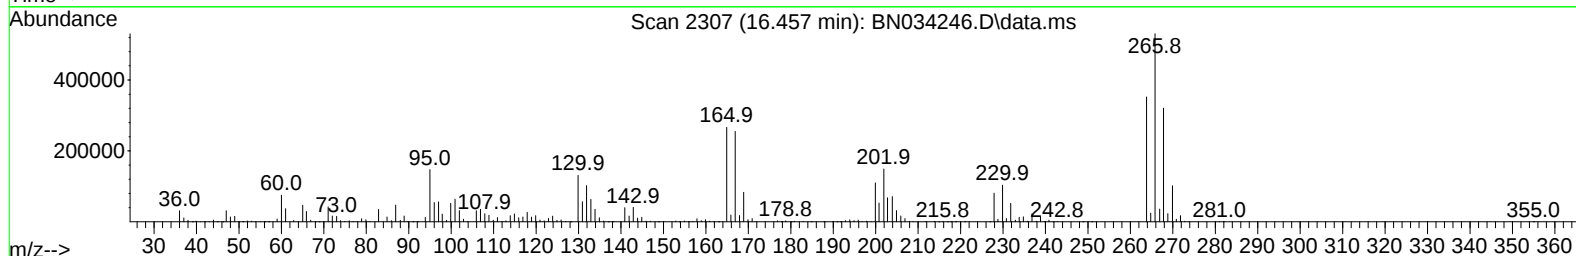


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034246.D
Acq On : 26 Sep 2024 13:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 16:19:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 26 05:44:15 2024
Response via : Initial Calibration

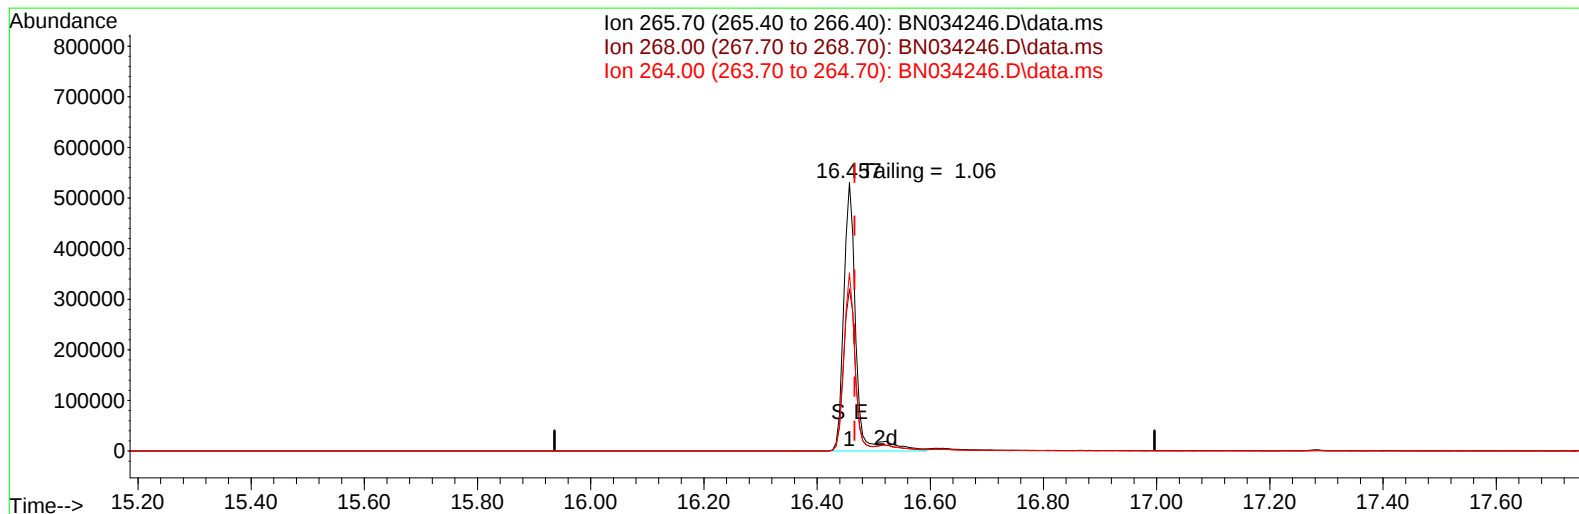

TIC: BN034246.D\data.ms

(70) Pentachlorophenol (C)




16.457min (-0.009) 19262.06 ng

response 740098

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.42
264.00	61.60	66.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034246.D
Acq On : 26 Sep 2024 13:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 16:23:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 26 05:44:15 2024
Response via : Initial Calibration

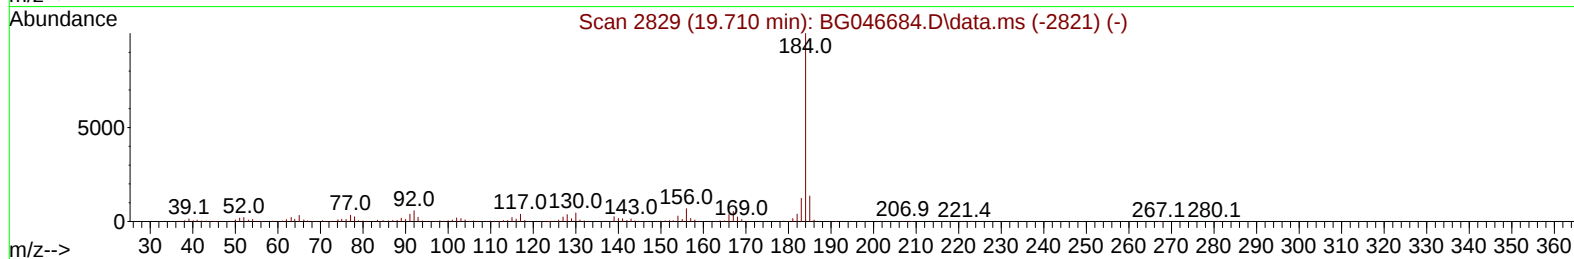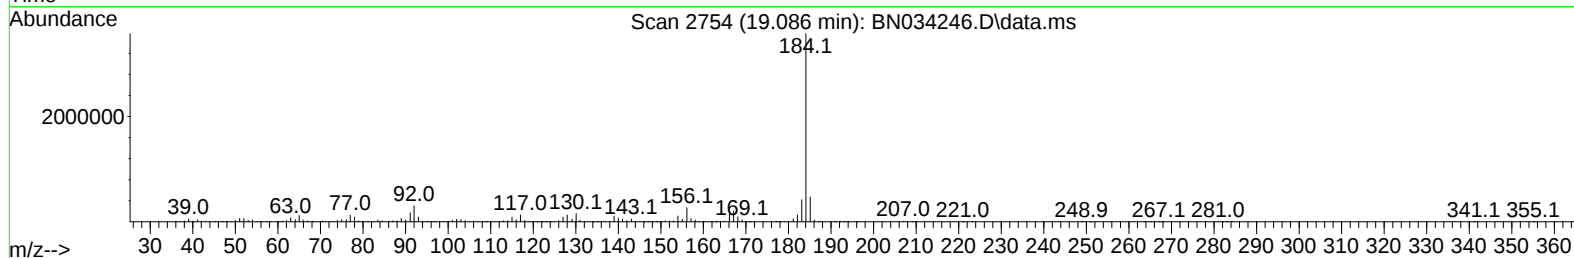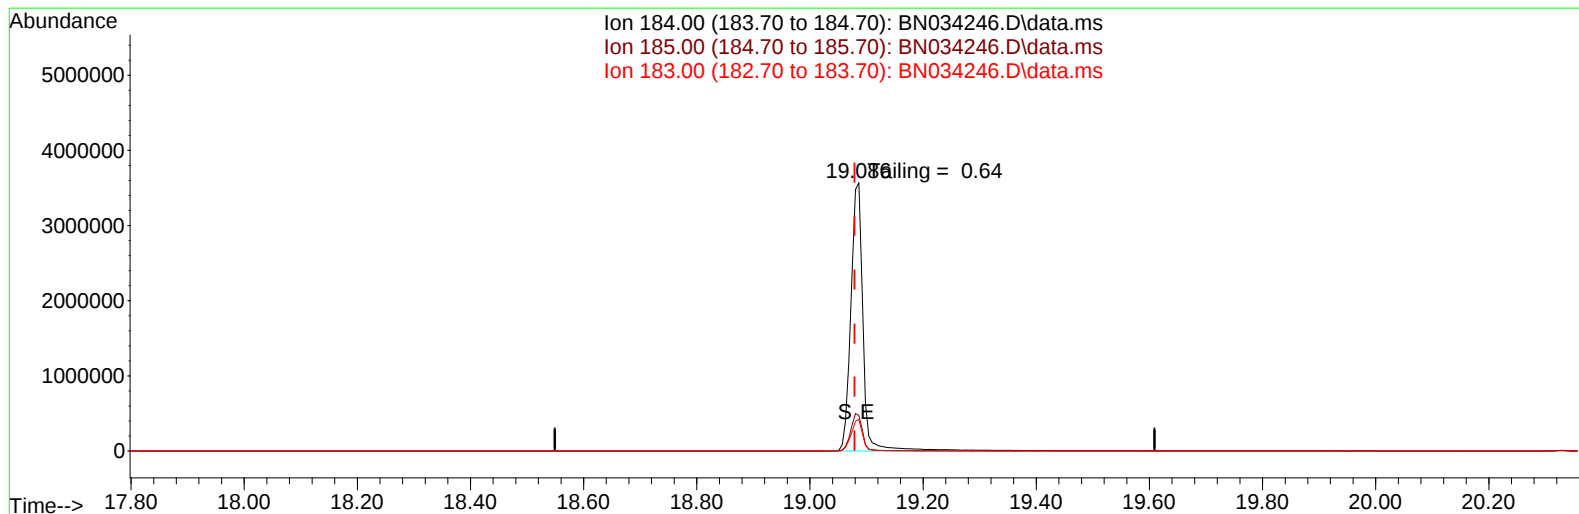

TIC: BN034246.D\data.ms

(77) Benzidine

19.086min (+ 0.007) 0.00 ng

response 5340629

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.23
183.00	13.20	11.78
0.00	0.00	0.00