
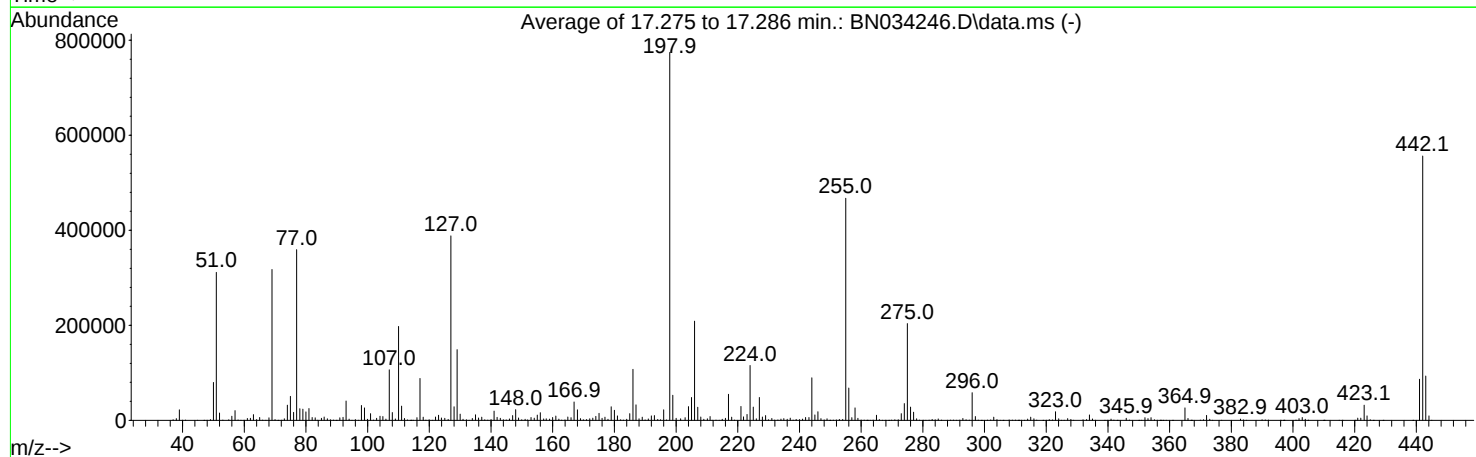


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034246.D
Acq On : 26 Sep 2024 13:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 26 14:44:02 2024

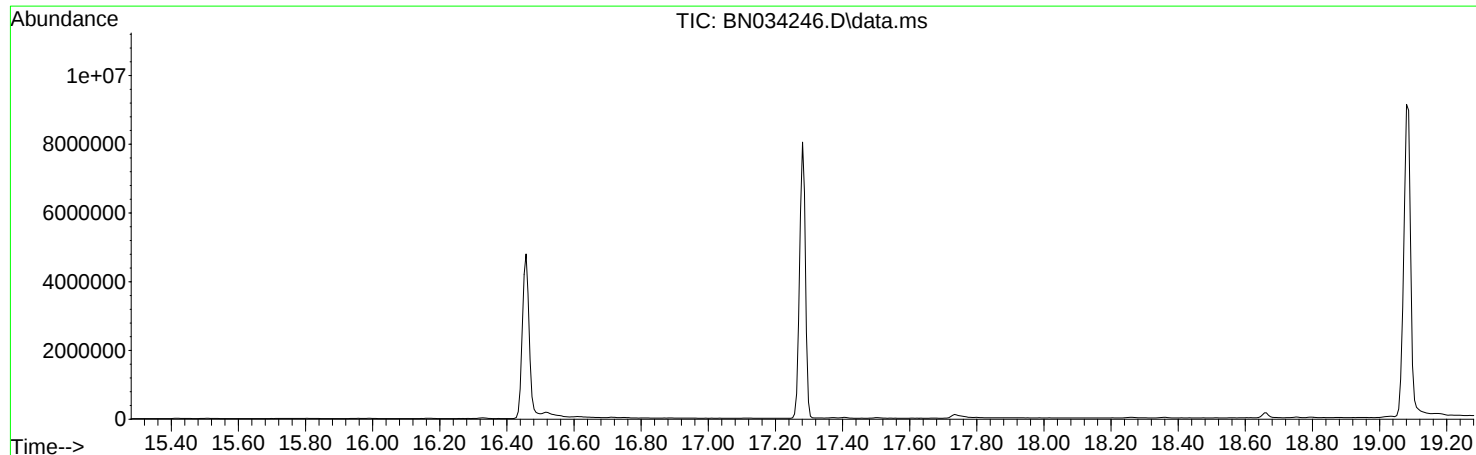




AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	311639	PASS
68	69	0.00	2	1.7	5275	PASS
69	198	0.00	100	41.0	317678	PASS
70	69	0.00	2	0.5	1616	PASS
127	198	10	80	50.1	388181	PASS
197	198	0.00	2	0.2	1173	PASS
198	198	100	100	100.0	774165	PASS
199	198	5	9	6.8	52853	PASS
275	198	10	60	26.3	203584	PASS
365	198	1	100	3.4	26248	PASS
441	198	0.01	100	11.2	86480	PASS
442	442	50	100	100.0	556309	PASS
443	442	15	24	16.8	93352	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034246.D
Acq On : 26 Sep 2024 13:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 16:19:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 26 05:44:15 2024
Response via : Initial Calibration

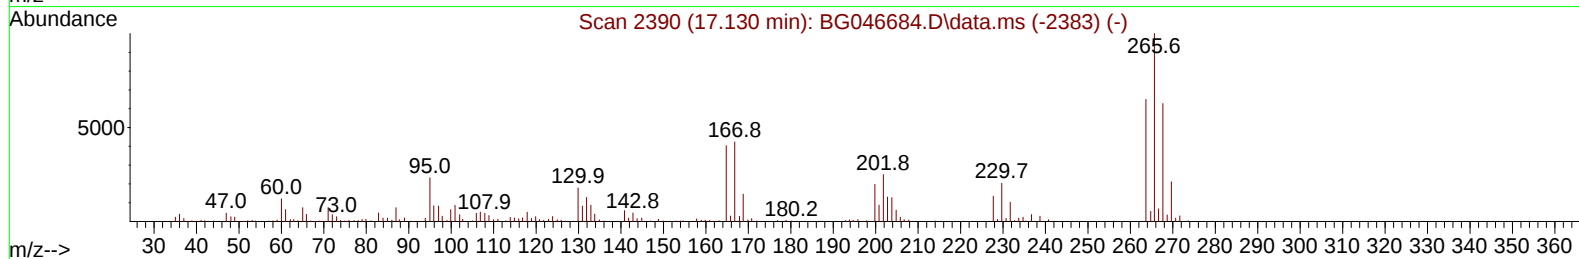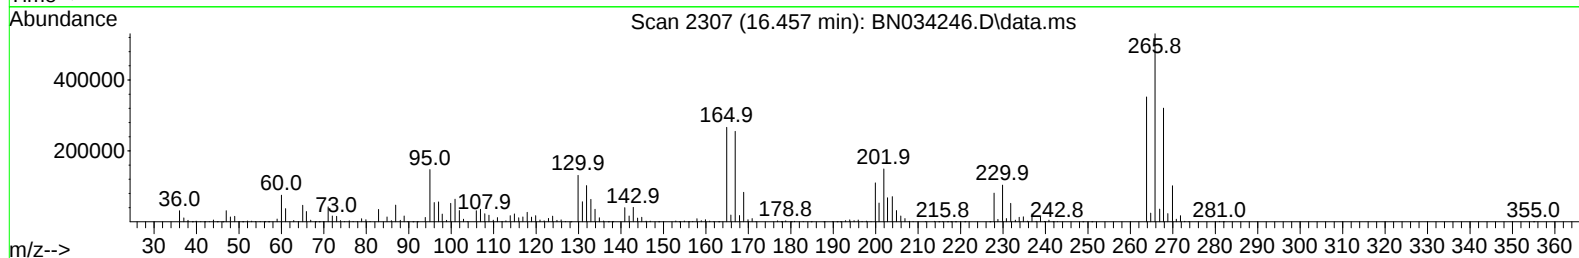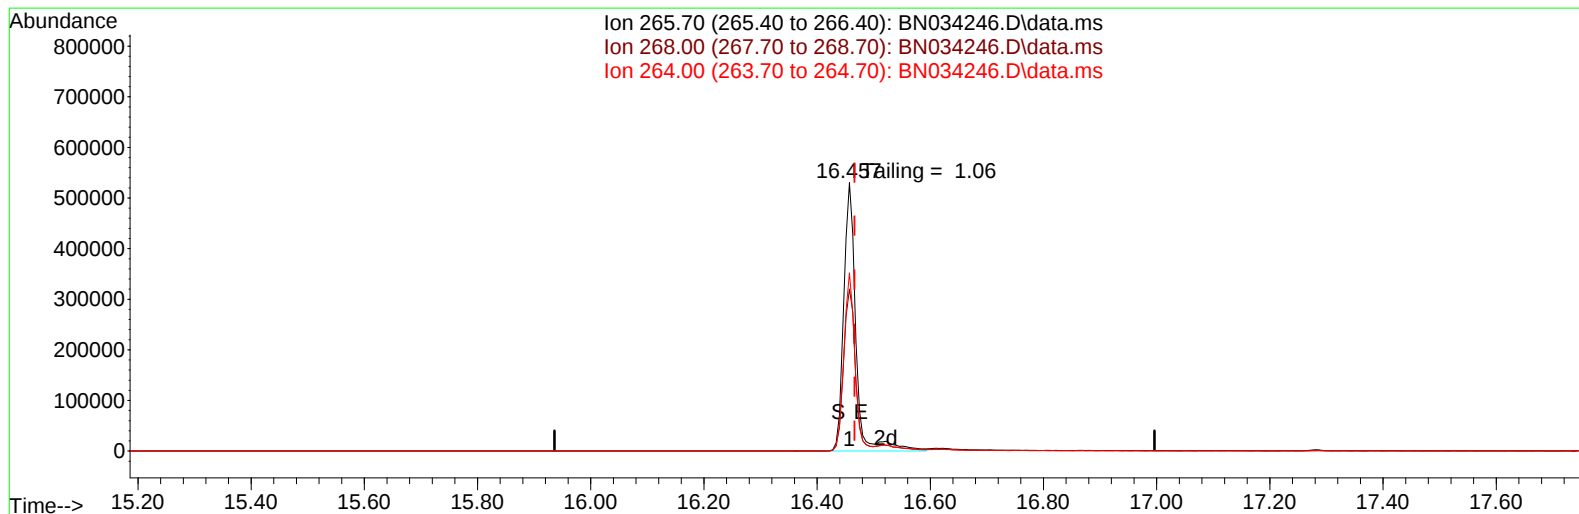

TIC: BN034246.D\data.ms

(70) Pentachlorophenol (C)

16.457min (-0.009) 19262.06 ng




response 740098

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.42
264.00	61.60	66.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034246.D
Acq On : 26 Sep 2024 13:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 26 16:23:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 26 05:44:15 2024
Response via : Initial Calibration

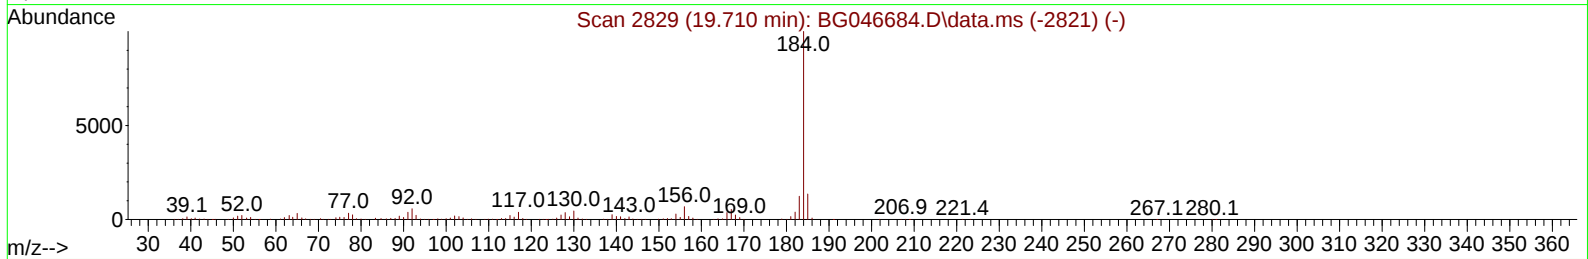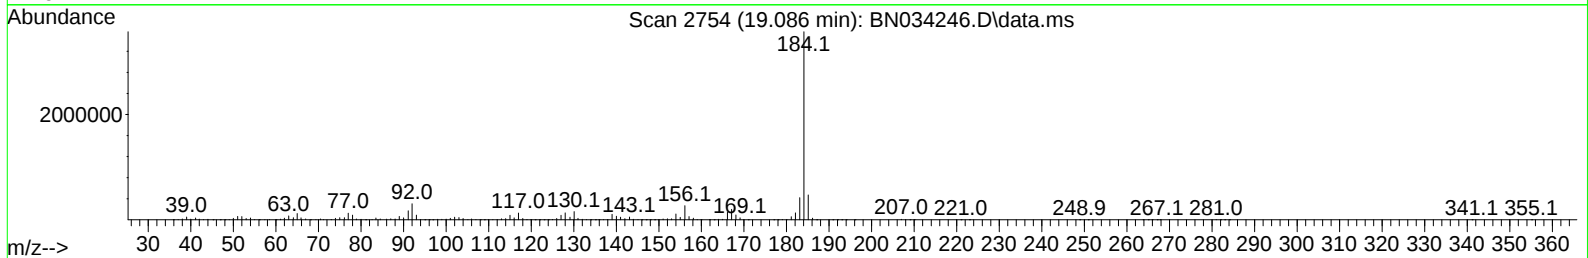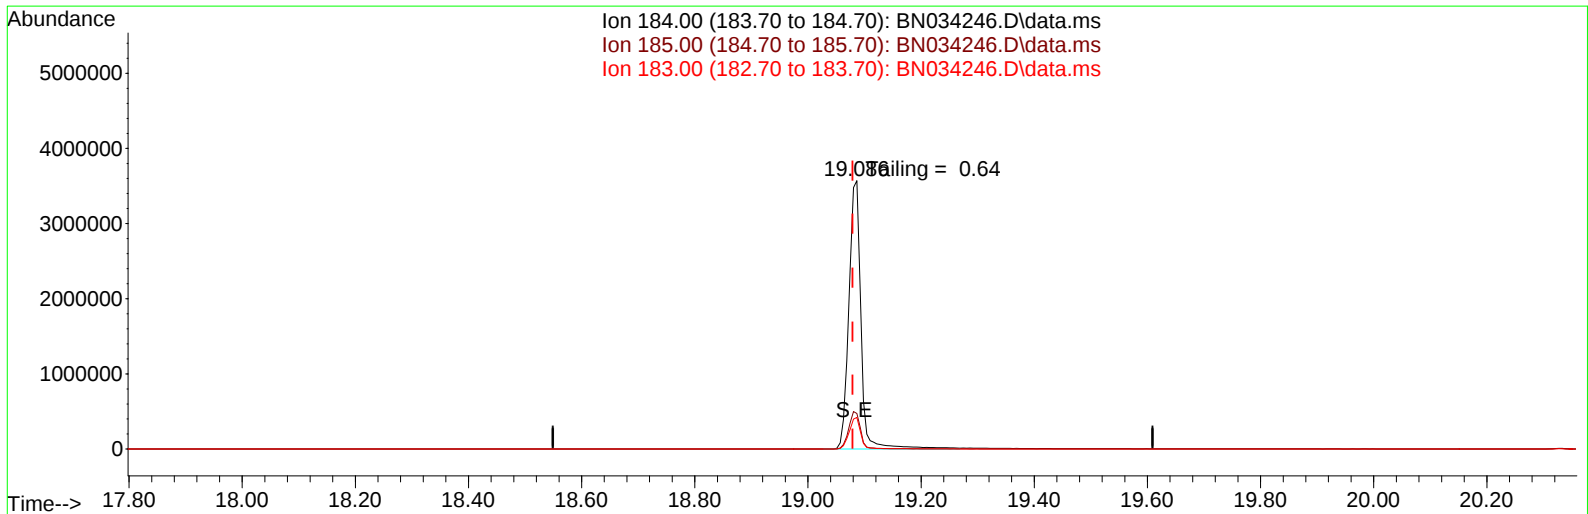

TIC: BN034246.D\data.ms

(77) Benzidine

19.086min (+ 0.007) 0.00 ng

response 5340629

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.23
183.00	13.20	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2024	BNA_N	<u>BN034246.D</u>
Compound Name	Response	Retention Time
DDT	2615121	20.333
DDD	40167	19.933
DDE	1672	19.375
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41839	2656960	1.57

Instrument :
BNA_N
ClientSampleId :
DFTPP