
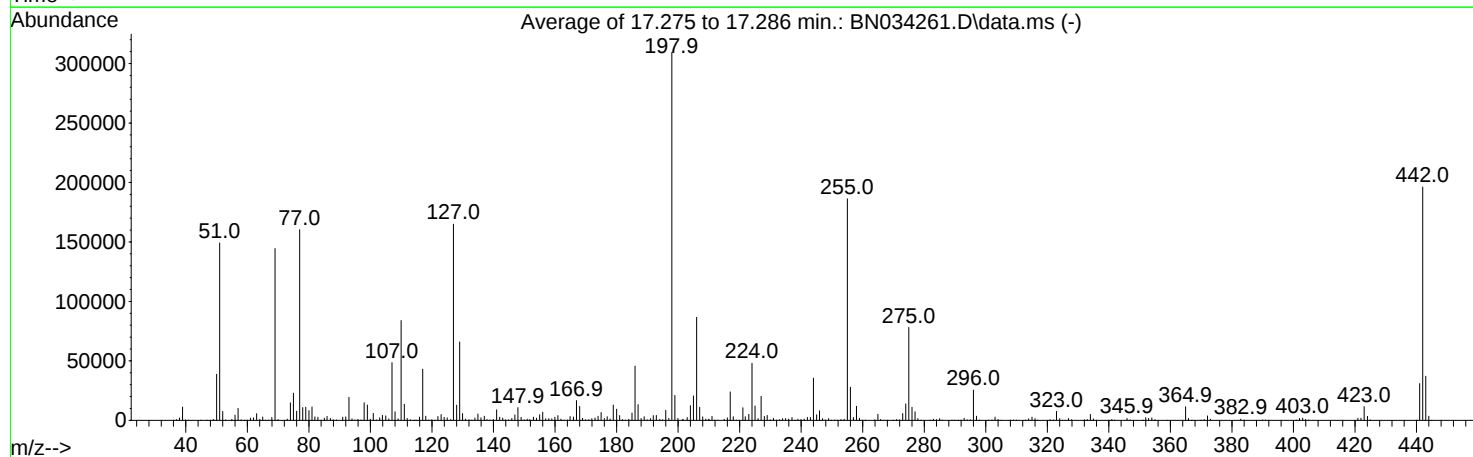


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034261.D
Acq On : 27 Sep 2024 01:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 26 14:44:02 2024

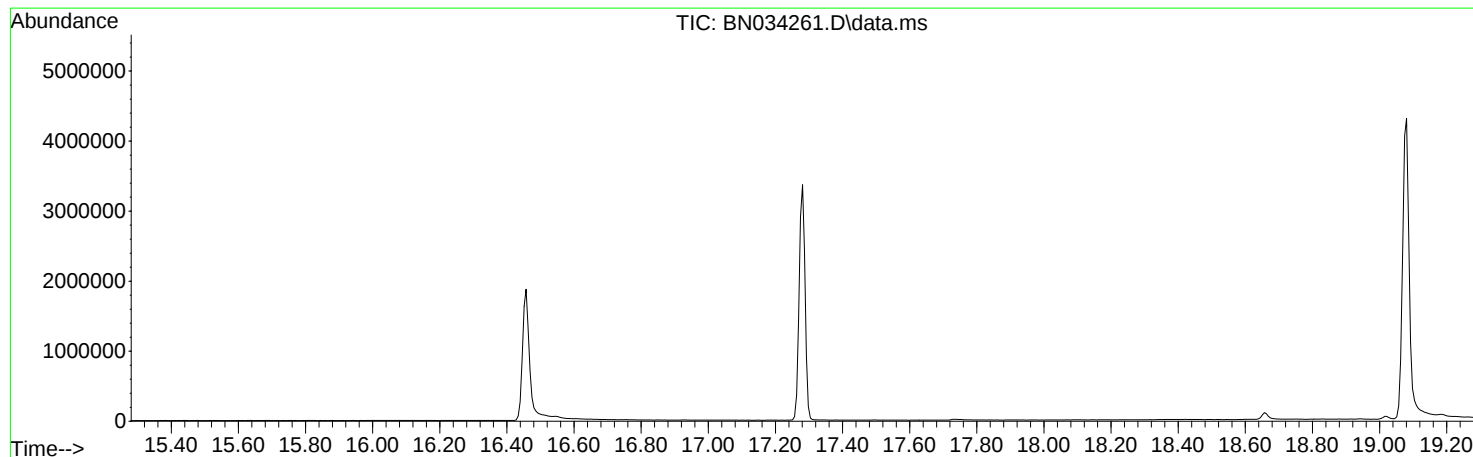




AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	149216	PASS
68	69	0.00	2	1.7	2449	PASS
69	198	0.00	100	46.7	144515	PASS
70	69	0.00	2	0.5	700	PASS
127	198	10	80	53.3	164947	PASS
197	198	0.00	2	0.5	1583	PASS
198	198	100	100	100.0	309269	PASS
199	198	5	9	6.8	21048	PASS
275	198	10	60	25.3	78131	PASS
365	198	1	100	3.7	11391	PASS
441	198	0.01	100	10.0	30901	PASS
442	442	50	100	100.0	196117	PASS
443	442	15	24	18.9	37141	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034261.D
Acq On : 27 Sep 2024 01:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 27 02:40:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 27 02:40:30 2024
Response via : Initial Calibration

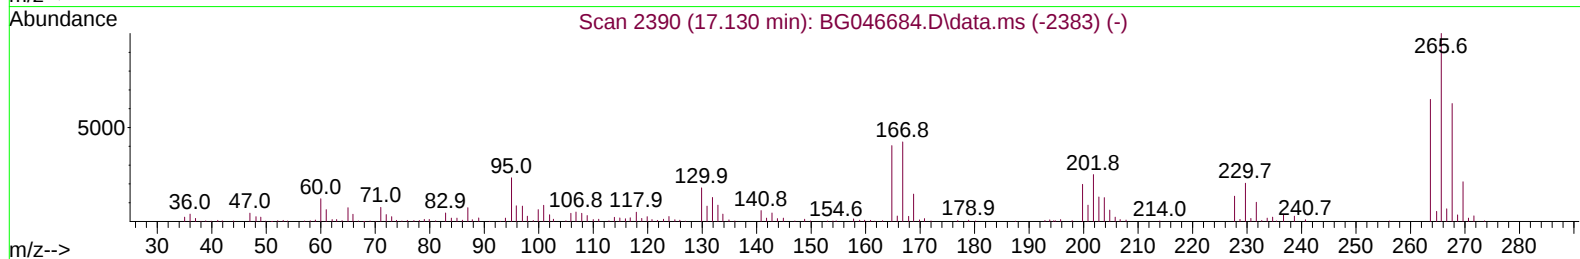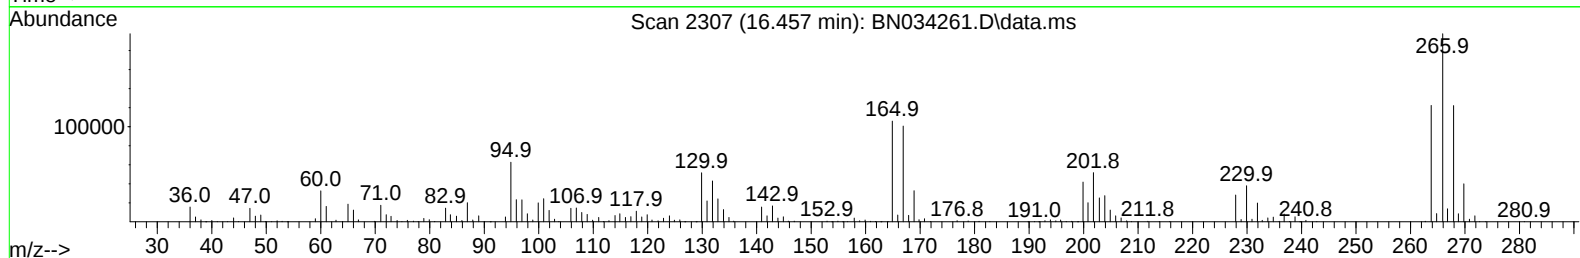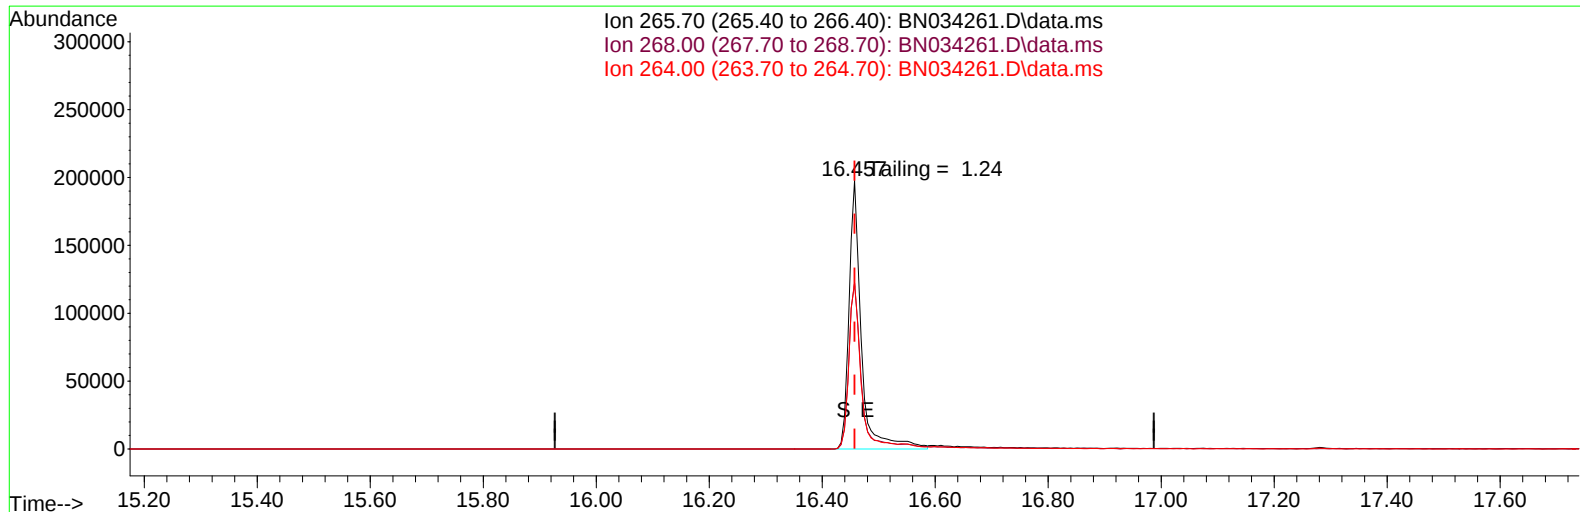

TIC: BN034261.D\data.ms

(70) Pentachlorophenol (C)

16.457min (0.000) 17318.27 ng




response 301583

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.84
264.00	61.60	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092624\
Data File : BN034261.D
Acq On : 27 Sep 2024 01:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 27 02:40:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 27 02:40:30 2024
Response via : Initial Calibration

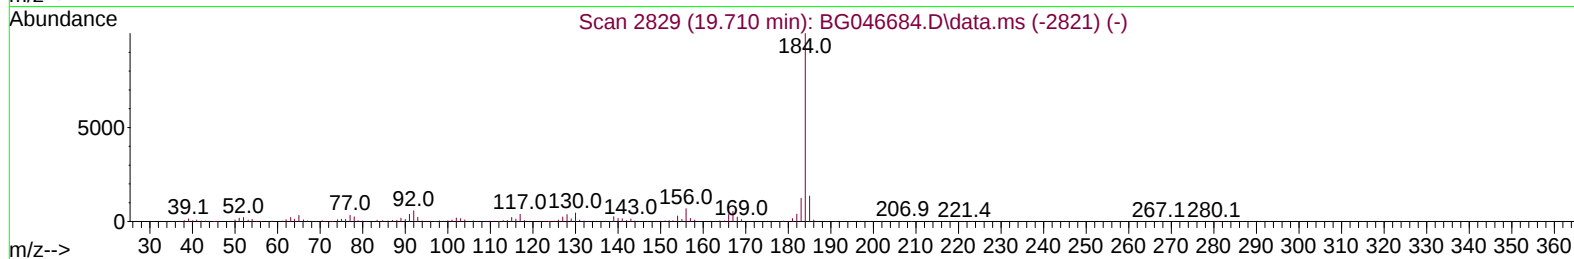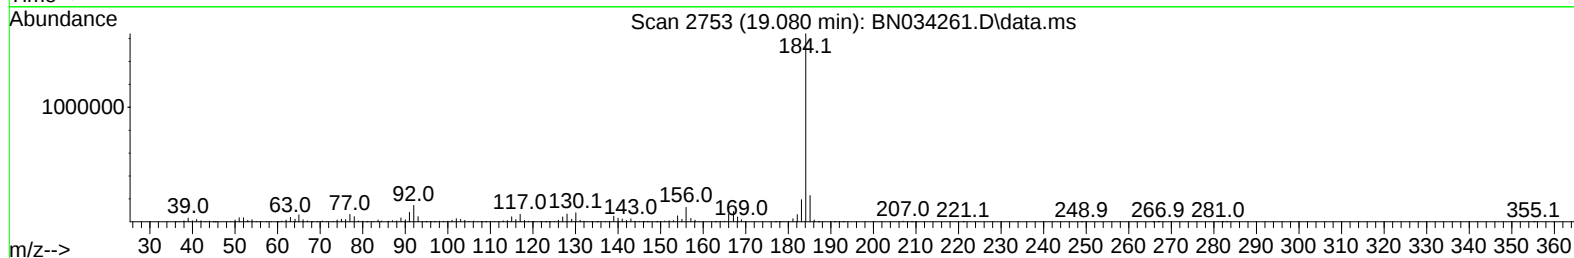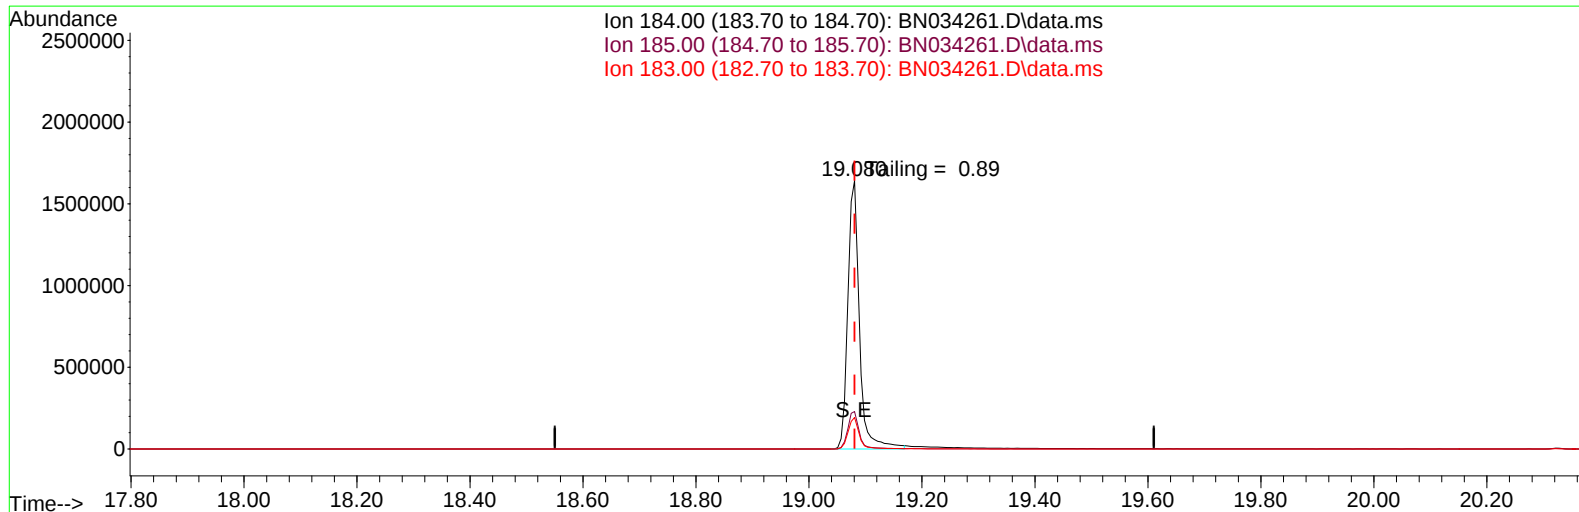

TIC: BN034261.D\data.ms

(77) Benzidine

19.080min (0.000) 0.00 ng

response 2441676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2024	BNA_N	<u>BN034261.D</u>
Compound Name	Response	Retention Time
DDT	1140628	20.327
DDD	14060	19.933
DDE	402	19.375
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14462	1155090	1.25

Instrument :
BNA_N
ClientSampleId :
DFTPP