
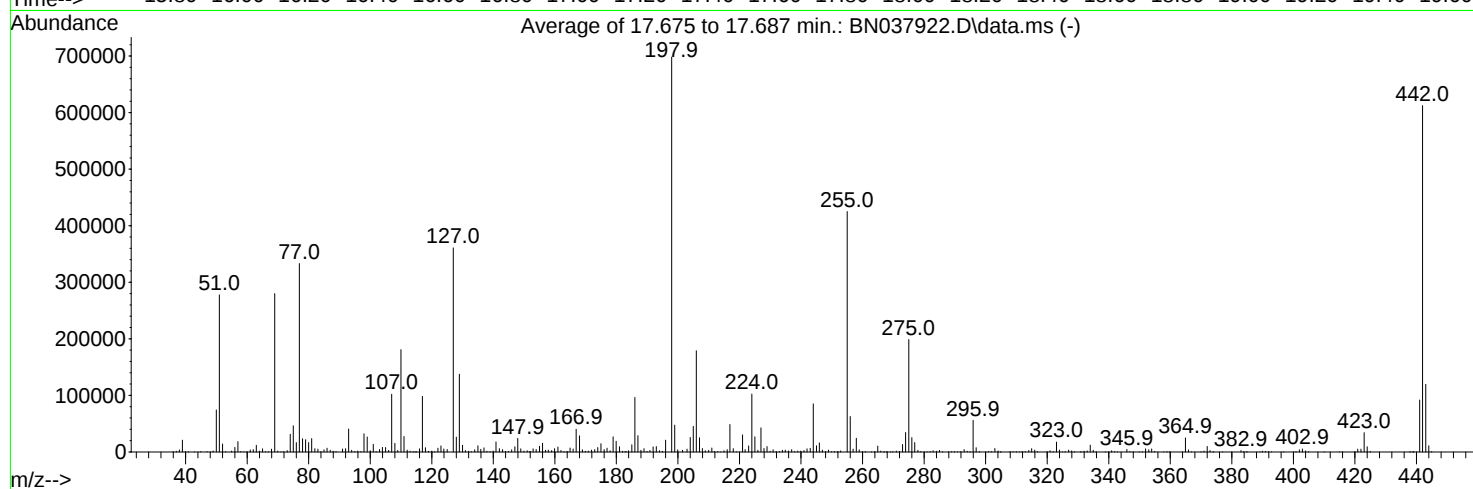


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092625\
Data File : BN037922.D
Acq On : 26 Sep 2025 12:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

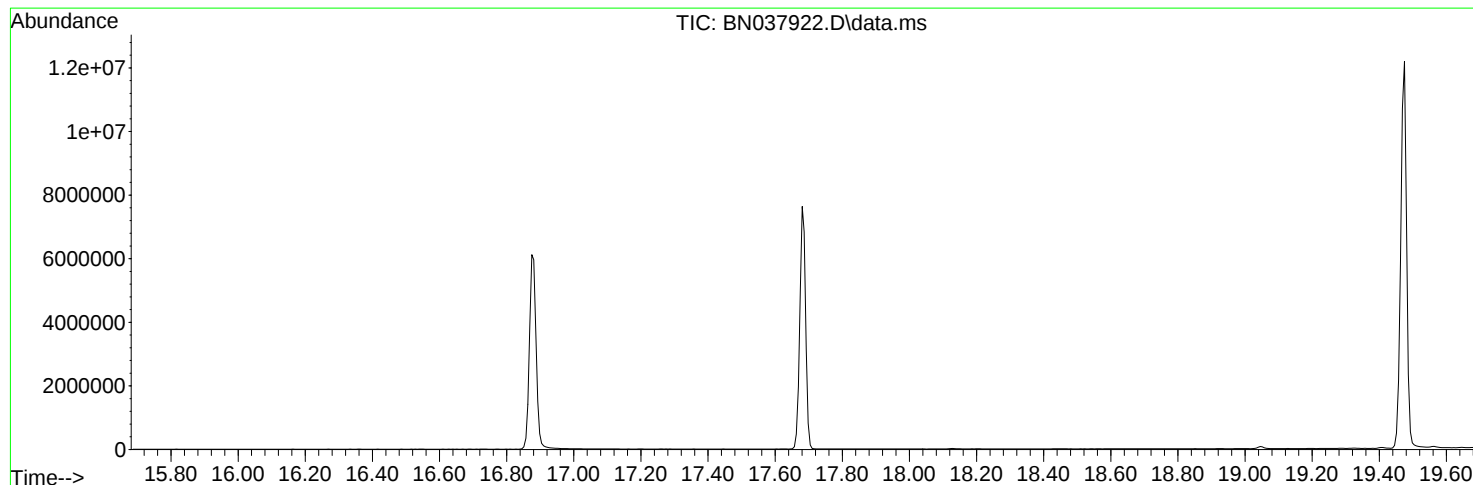

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	5079	PASS
69	69	100	100	100.0	280043	PASS
70	69	0.00	2	0.5	1531	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	698133	PASS
199	198	5	9	6.8	47523	PASS
365	198	1	100	3.5	24722	PASS
441	443	0.01	150	76.9	91856	PASS
442	442	100	100	100.0	612480	PASS
443	442	15	24	19.5	119517	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/26/2025	BNA_N	<u>BN037922.D</u>
Compound Name	Response	Retention Time
DDT	2863271	20.71
DDD	19415	20.269
DDE	521	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19936	2883207	0.69

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092625\
Data File : BN037922.D
Acq On : 26 Sep 2025 12:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 29 10:38:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

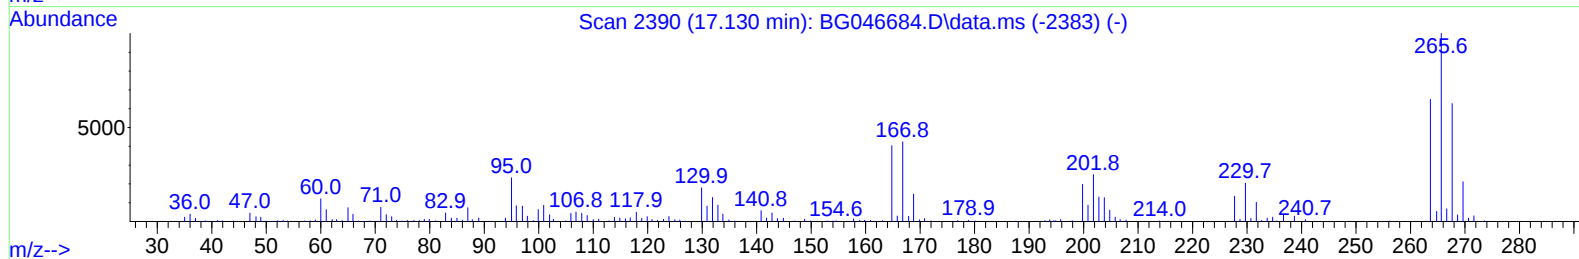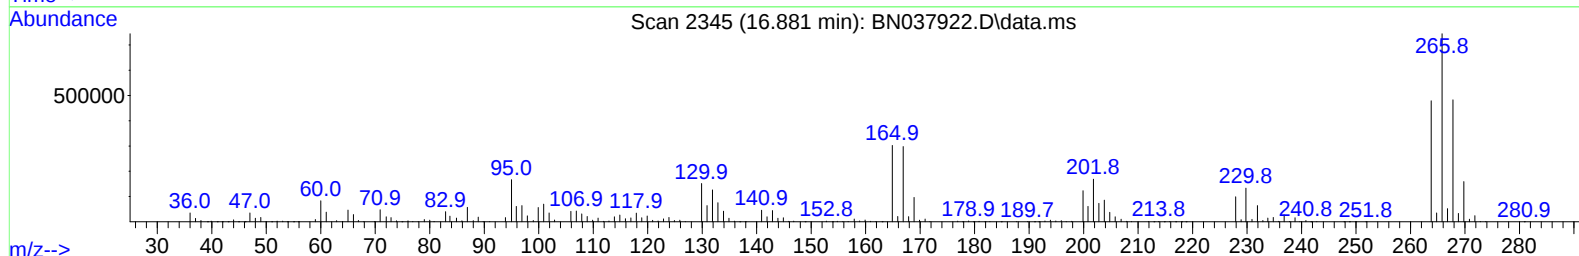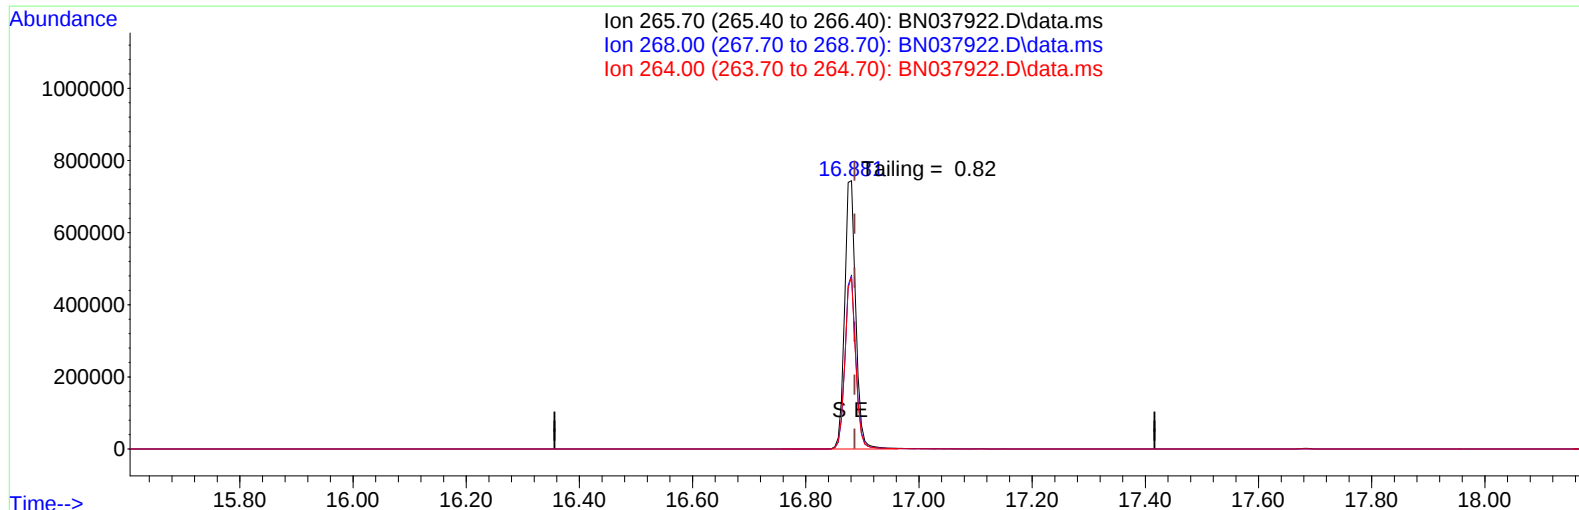

TIC: BN037922.D\data.ms

(70) Pentachlorophenol (C)

16.881min (-0.005) 28751.81 ng




response 1019202

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.83
264.00	61.60	64.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092625\
Data File : BN037922.D
Acq On : 26 Sep 2025 12:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 29 10:38:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

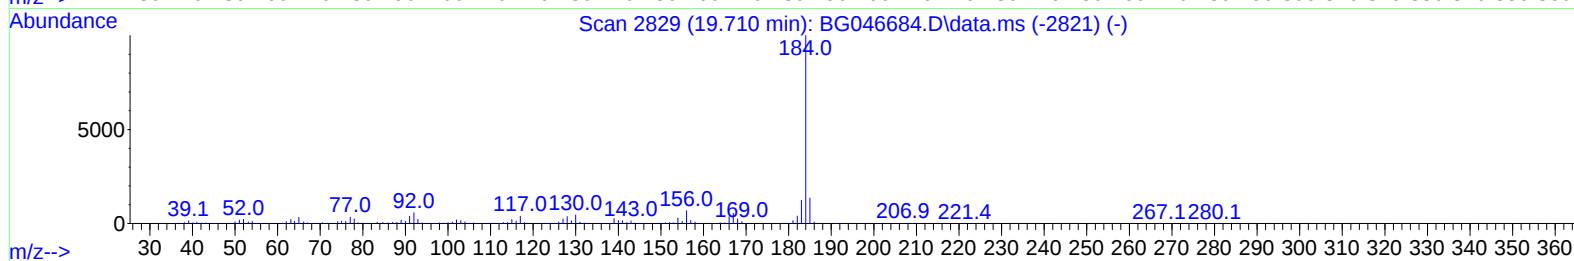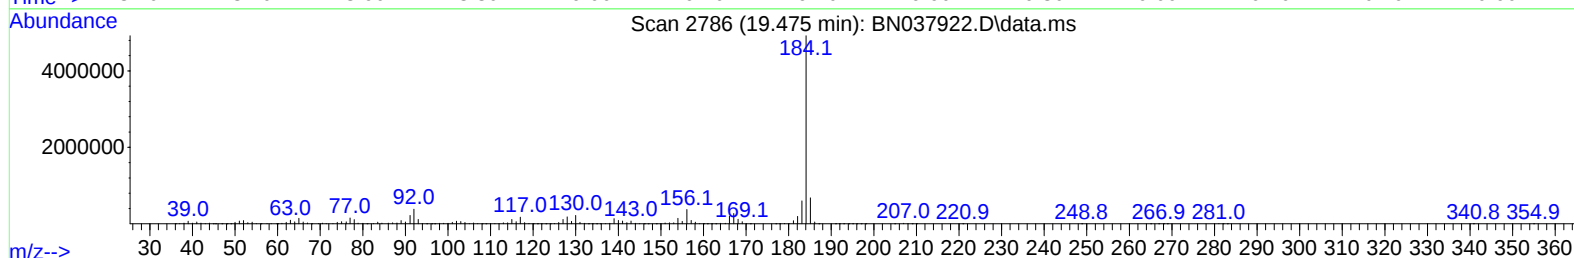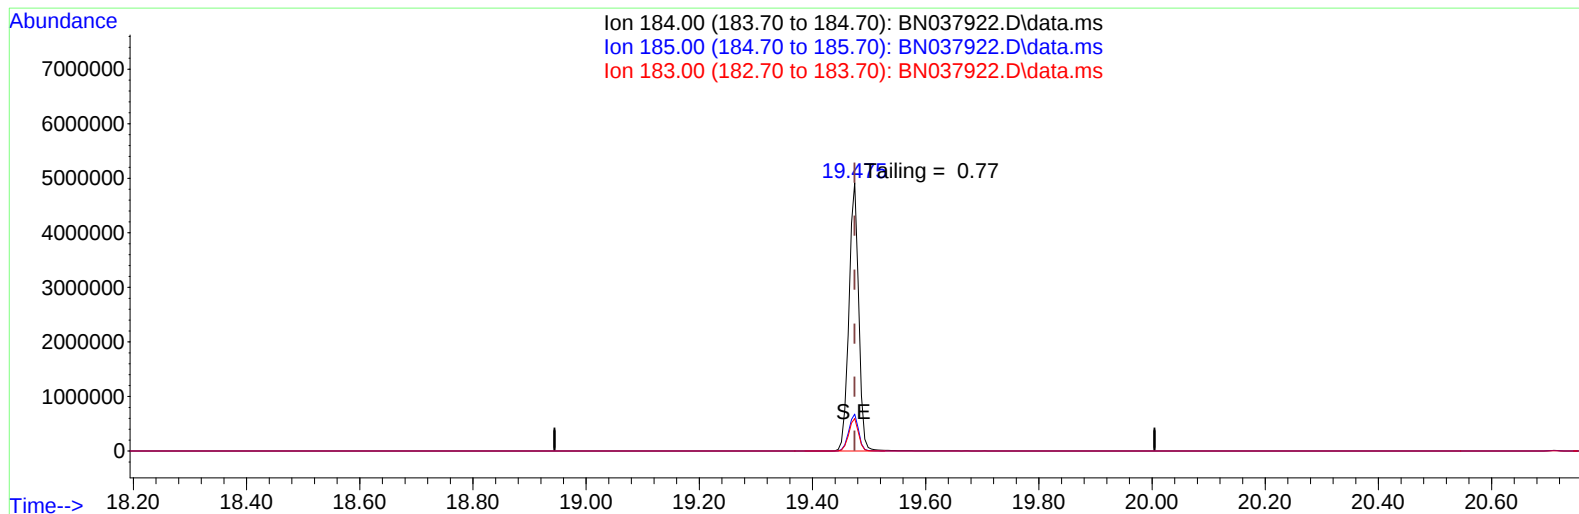

TIC: BN037922.D\data.ms

(77) Benzidine

19.475min (+ 0.001) 0.00 ng

response 5937981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.80
183.00	13.20	12.14
0.00	0.00	0.00